

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052722\
 Data File : PP048127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 00:57
 Operator : YP\AJ
 Sample : N2927-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P010-SS004-1218-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2022
 Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:22:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 27 23:53:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.037	3.220	49711954	42662853	21.228	21.648
2) SA Decachlor...	10.393	8.662	30708893	27073903	15.800	16.749

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052722\
Data File : PP048127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 00:57
Operator : YP\AJ
Sample : N2927-08
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
P010-SS004-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:22:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 27 23:53:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

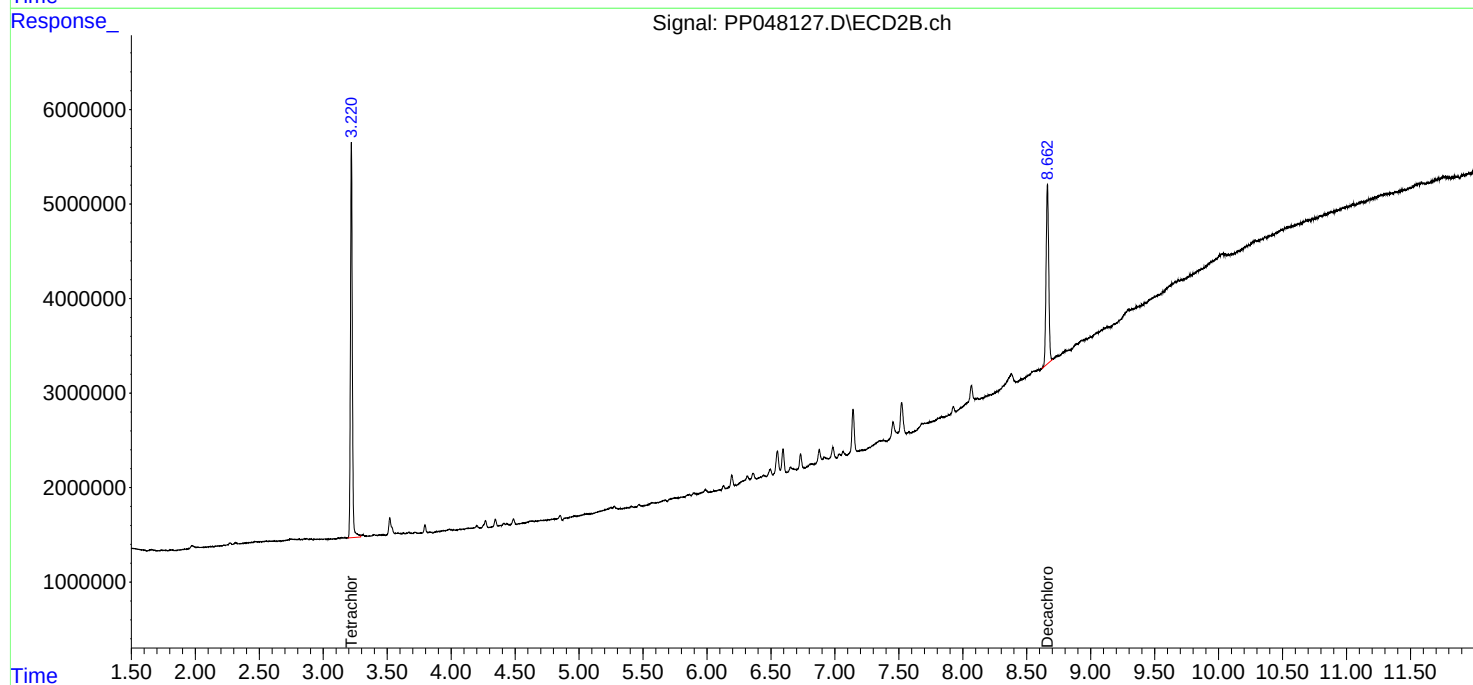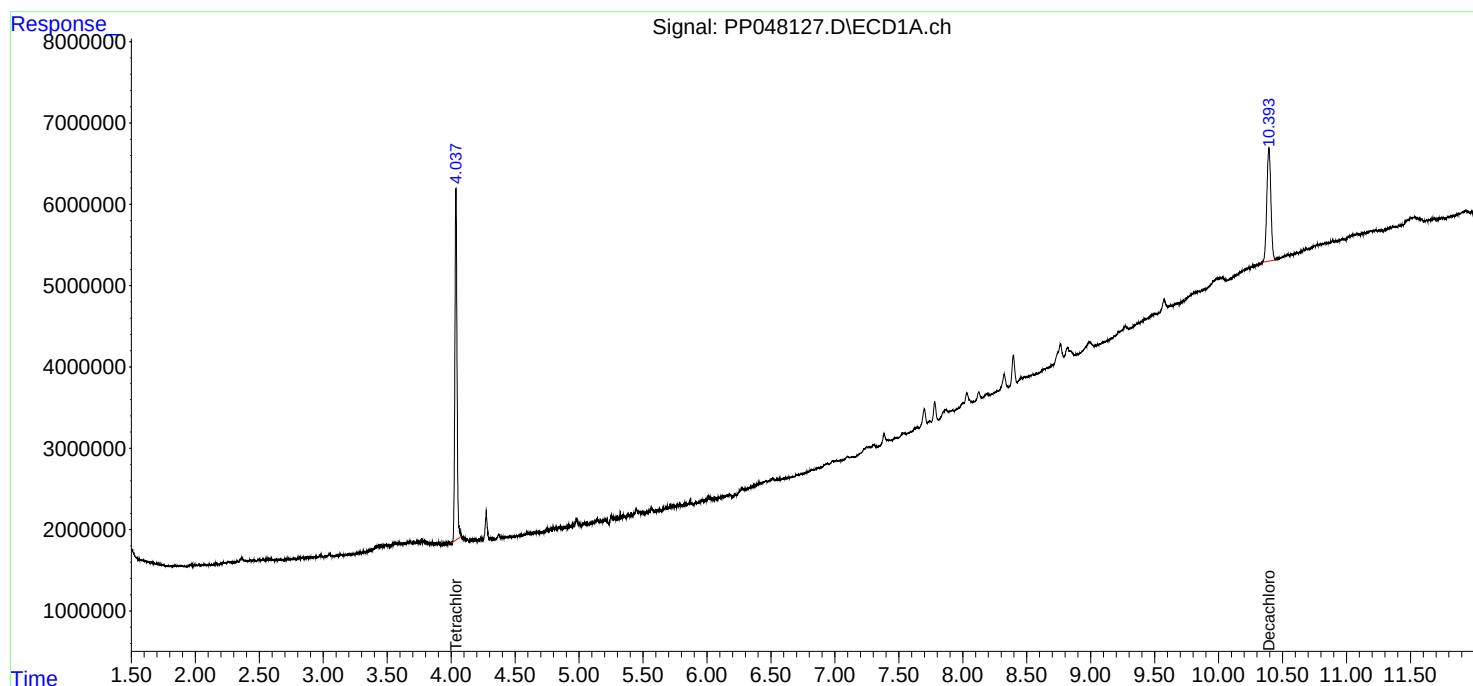

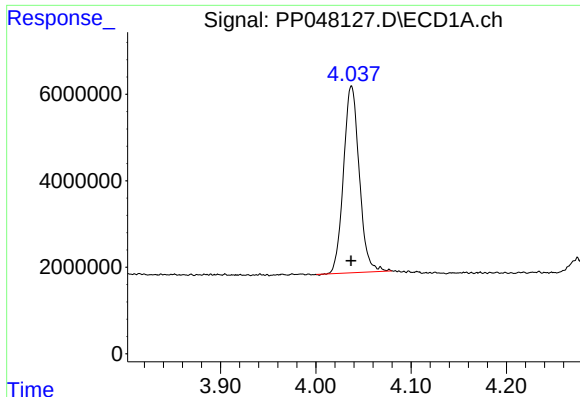


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 49711954
Conc: 21.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
P010-SS004-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

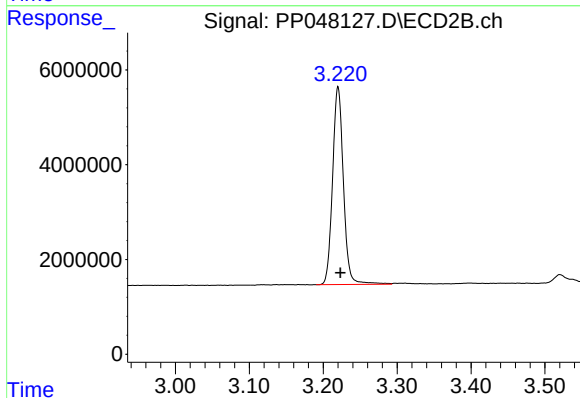


#1 Tetrachloro-m-xylene

R.T.: 3.220 min
Delta R.T.: -0.003 min
Response: 42662853
Conc: 21.65 ng/ml

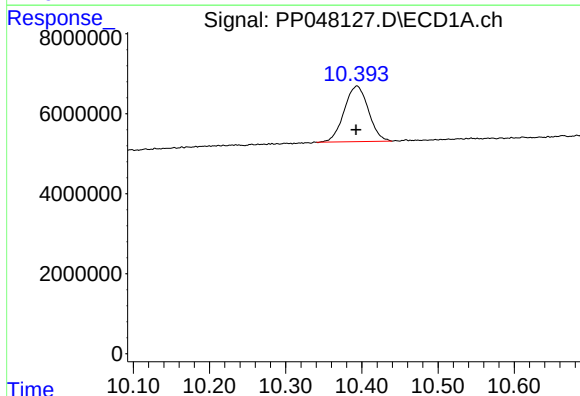

#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 30708893
Conc: 15.80 ng/ml

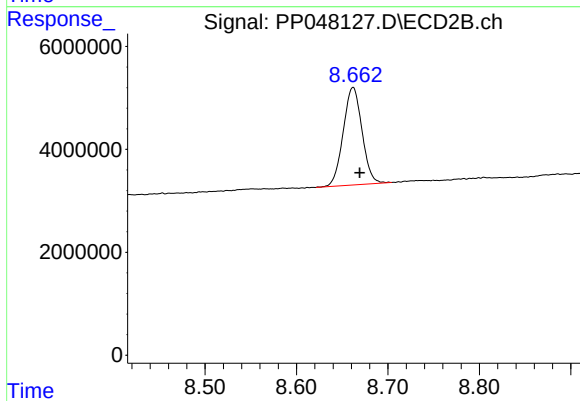

#2 Decachlorobiphenyl

R.T.: 8.662 min
Delta R.T.: -0.007 min
Response: 27073903
Conc: 16.75 ng/ml