

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052722\
 Data File : PP048128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 01:12
 Operator : YP\AJ
 Sample : N2927-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P010-SS004-1824-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2022
 Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:23:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 27 23:53:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.037	3.220	52030462	44269797	22.218	22.463
2) SA Decachlor...	10.392	8.662	28817718	25866494	14.827	16.002

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052722\
Data File : PP048128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 01:12
Operator : YP\AJ
Sample : N2927-09
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
P010-SS004-1824-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:23:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 27 23:53:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

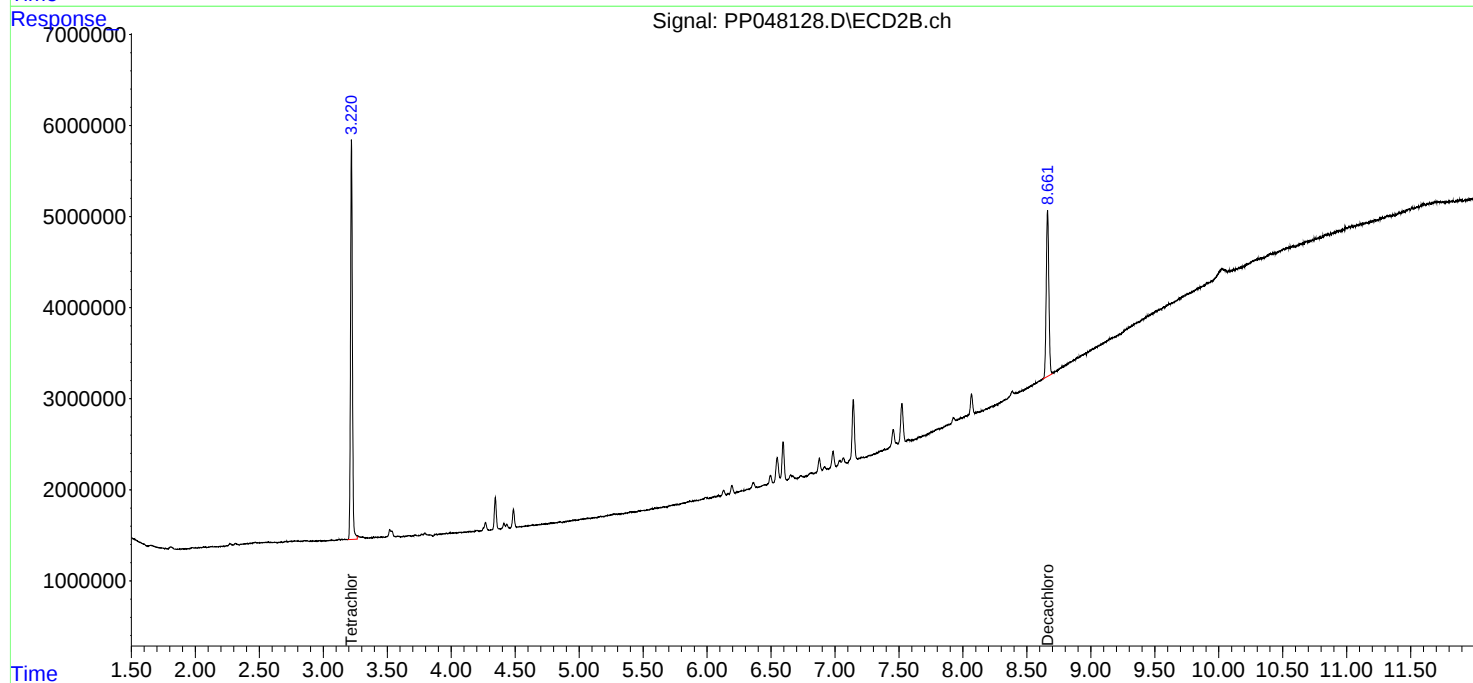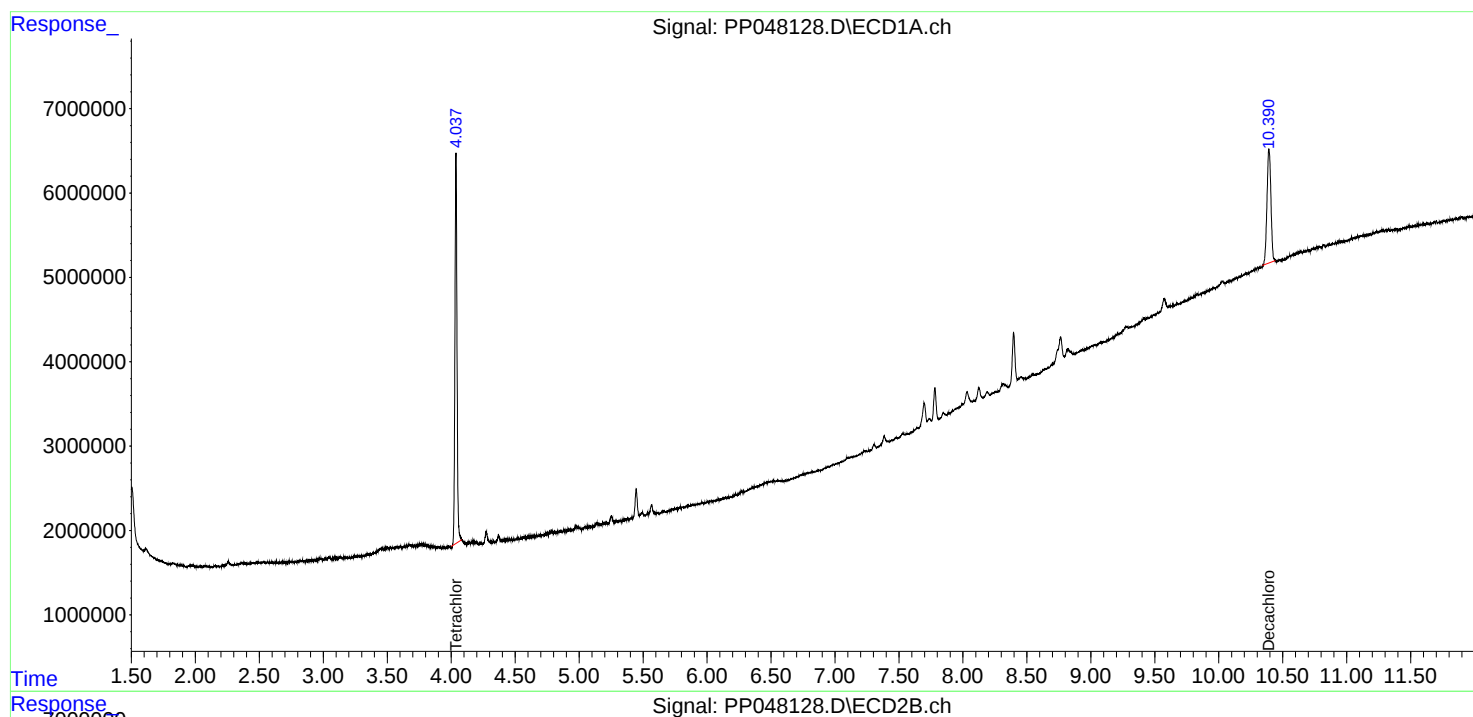

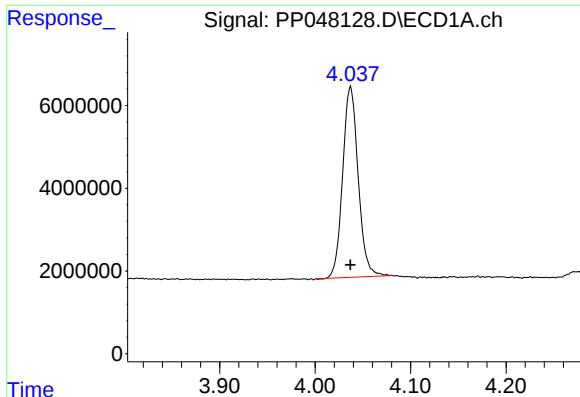


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 52030462
Conc: 22.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
P010-SS004-1824-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

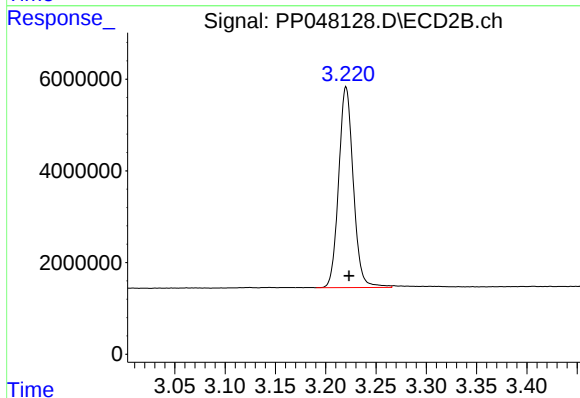


#1 Tetrachloro-m-xylene

R.T.: 3.220 min
Delta R.T.: -0.003 min
Response: 44269797
Conc: 22.46 ng/ml

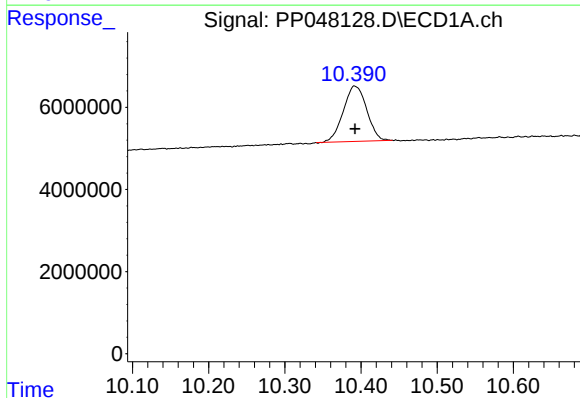

#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 28817718
Conc: 14.83 ng/ml

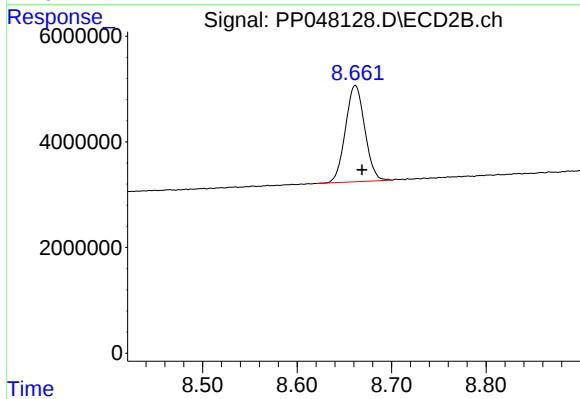

#2 Decachlorobiphenyl

R.T.: 8.662 min
Delta R.T.: -0.007 min
Response: 25866494
Conc: 16.00 ng/ml