

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052824\
 Data File : PP065256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2024 14:21
 Operator : YP\AJ
 Sample : PB161152BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB161152BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/29/2024
 Supervised By :Ankita Jodhani 05/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 01:18:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.470	3.751	32104373	29190529	20.341	19.228
2) SA Decachlor...	10.213	8.820	31718937	28654334	24.394m	21.739

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052824\
Data File : PP065256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2024 14:21
Operator : YP\AJ
Sample : PB161152BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB161152BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2024
Supervised By :Ankita Jodhani 05/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 01:18:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

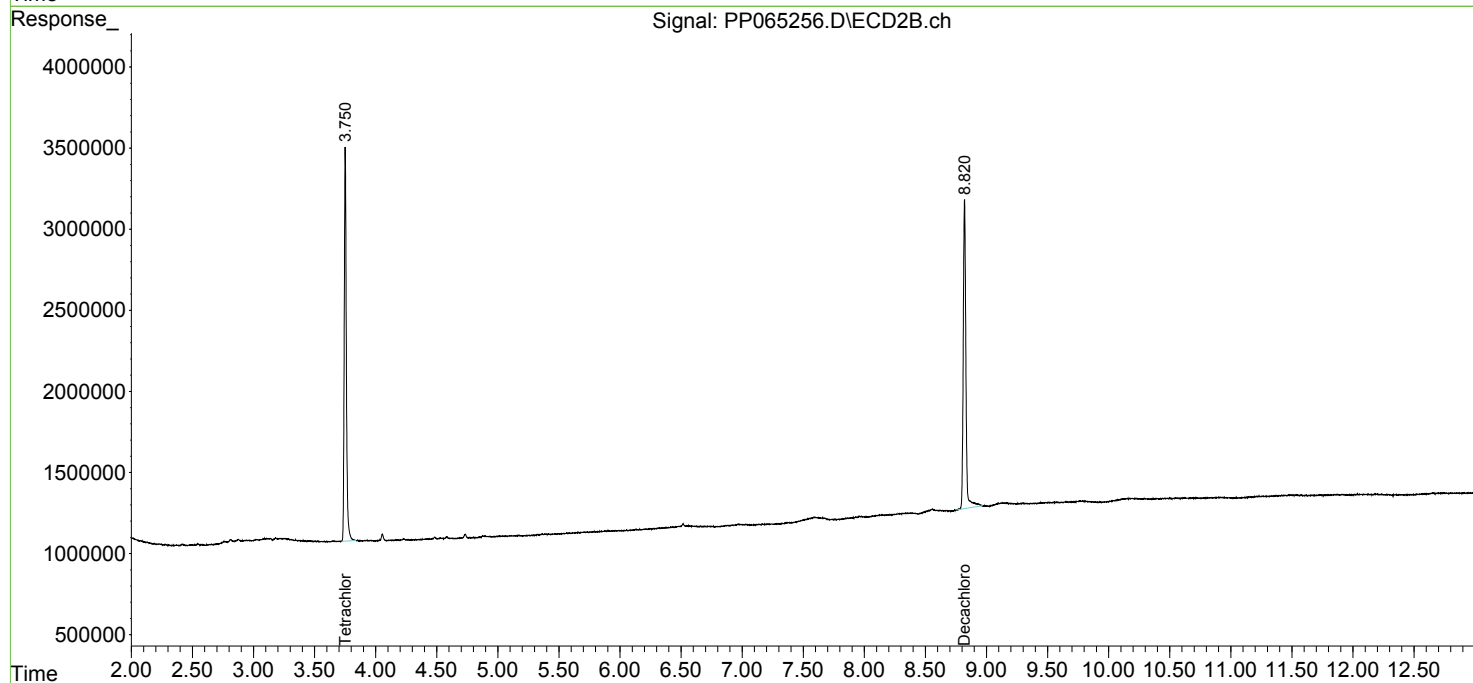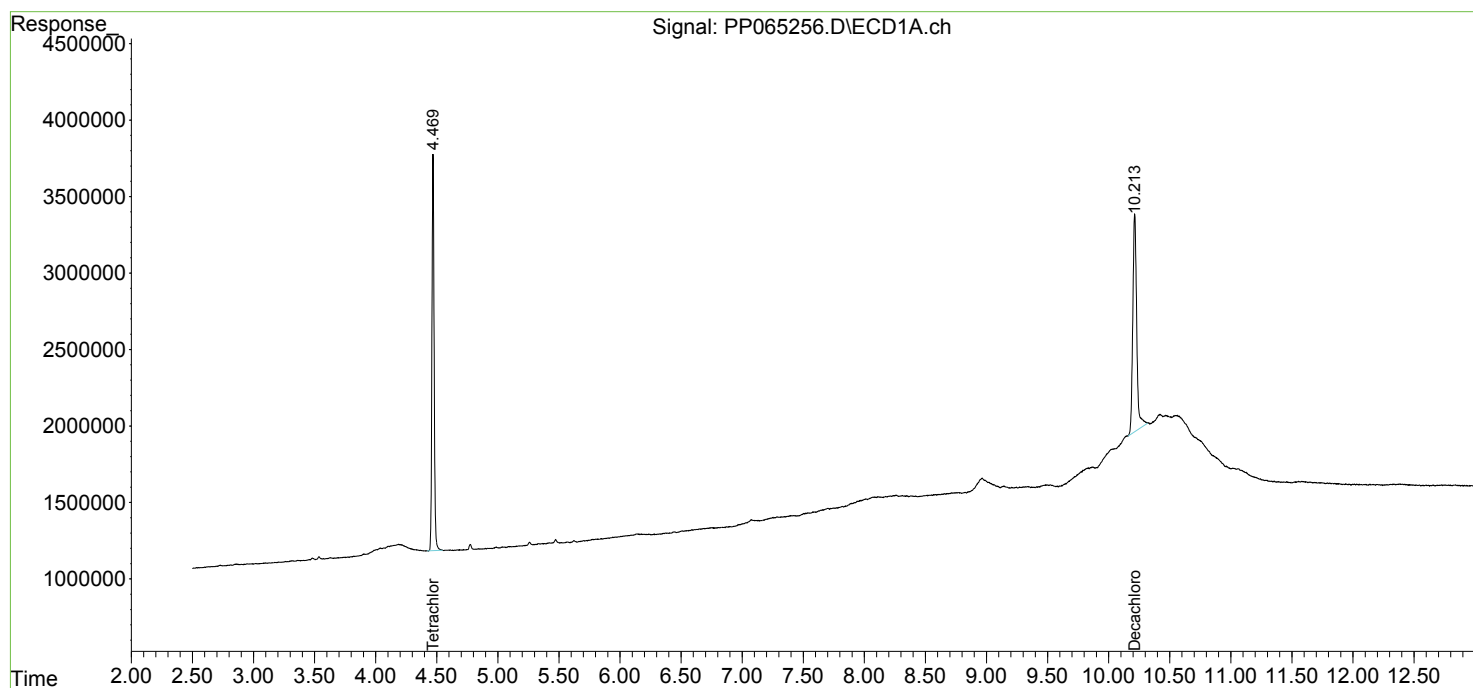

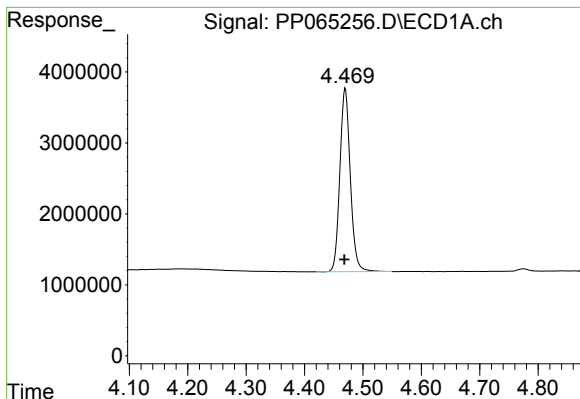


#1 Tetrachloro-m-xylene

R.T.: 4.470 min
Delta R.T.: 0.002 min
Response: 32104373
Conc: 20.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161152BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2024
Supervised By :Ankita Jodhani 05/29/2024

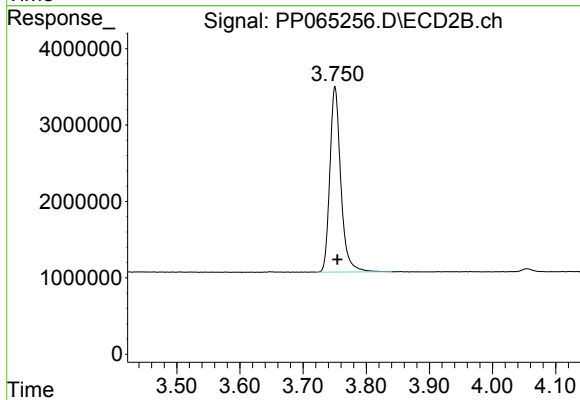


#1 Tetrachloro-m-xylene

R.T.: 3.751 min
Delta R.T.: -0.004 min
Response: 29190529
Conc: 19.23 ng/ml

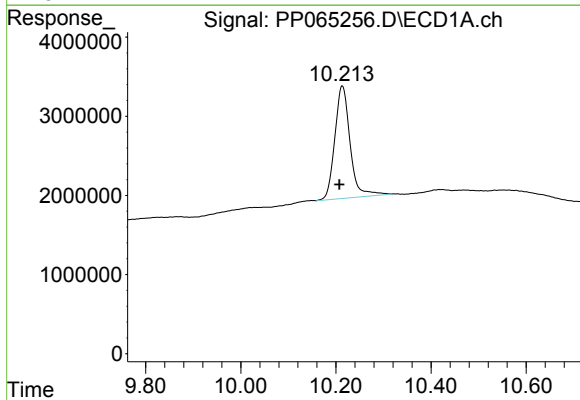

#2 Decachlorobiphenyl

R.T.: 10.213 min
Delta R.T.: 0.005 min
Response: 31718937
Conc: 24.39 ng/ml m

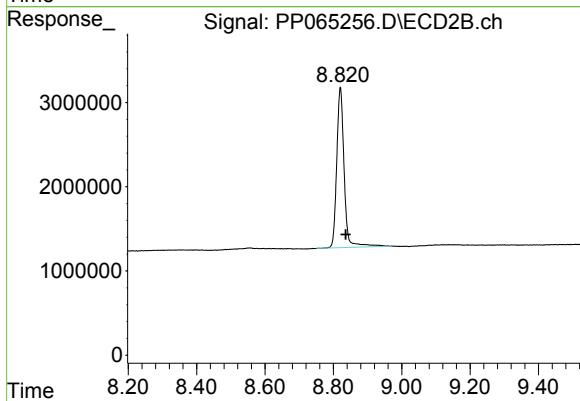

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.016 min
Response: 28654334
Conc: 21.74 ng/ml