

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052825\
 Data File : PP072416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2025 17:59
 Operator : YP\AJ
 Sample : Q2131-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CAM-40626

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/29/2025
 Supervised By :mohammad ahmed 05/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:11:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.504	3.807	28643178	34628720	14.245m	21.665 #
2) SA Decachlor...	10.202	8.814	27550824	21715843	16.911	20.514

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052825\
Data File : PP072416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2025 17:59
Operator : YP\AJ
Sample : Q2131-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CAM-40626


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2025
Supervised By :mohammad ahmed 05/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:11:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

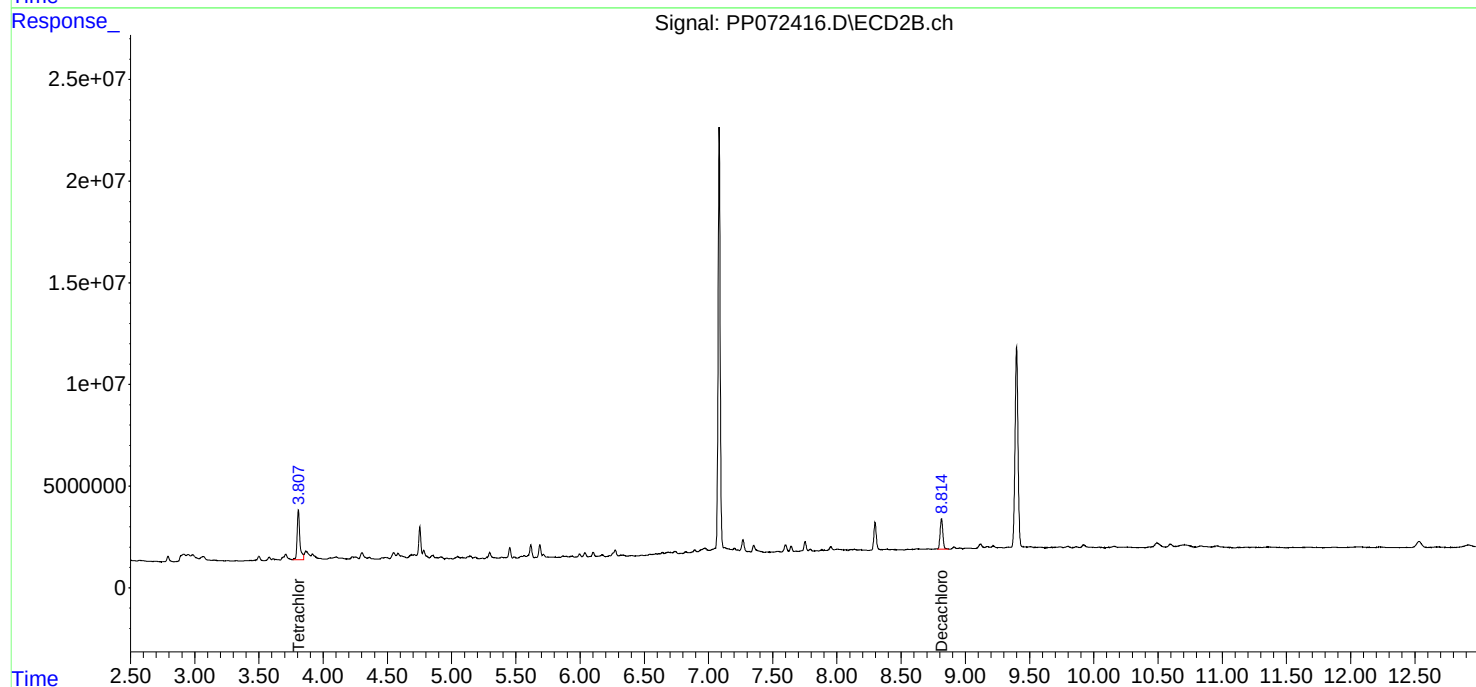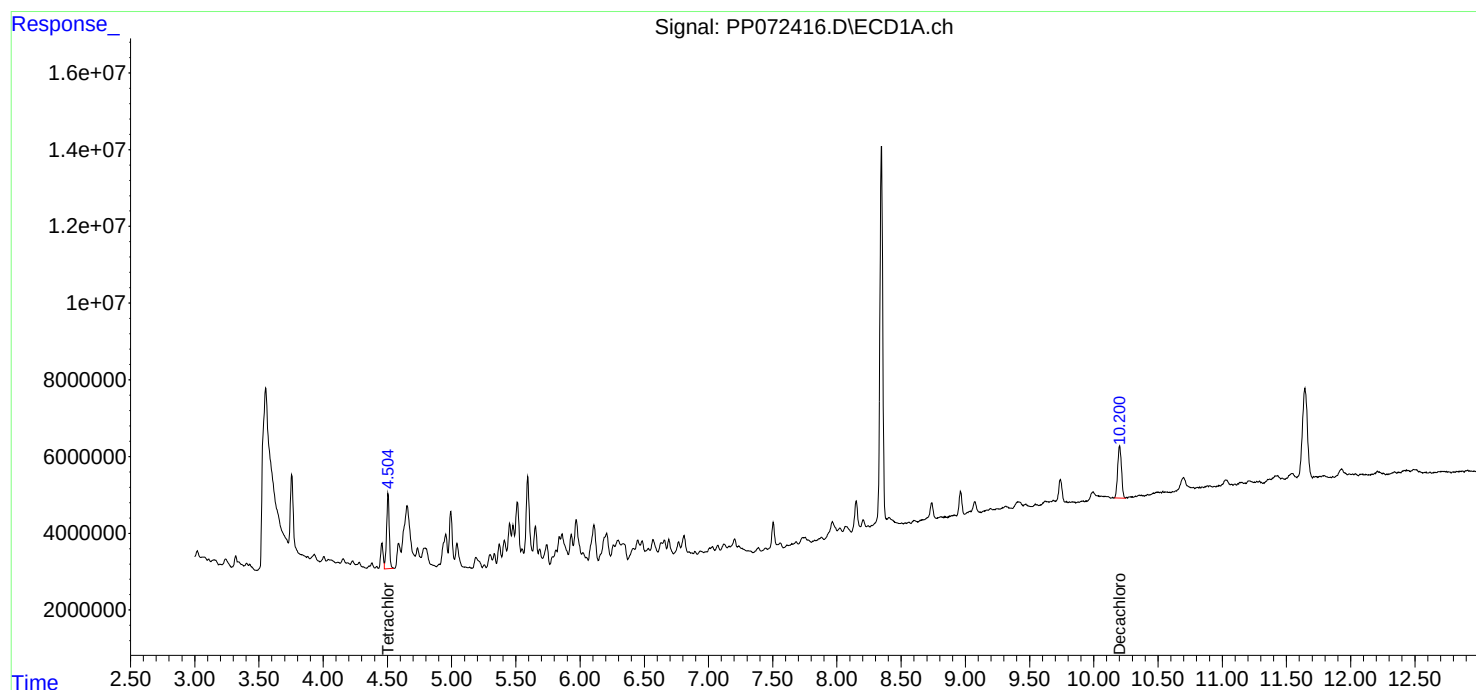

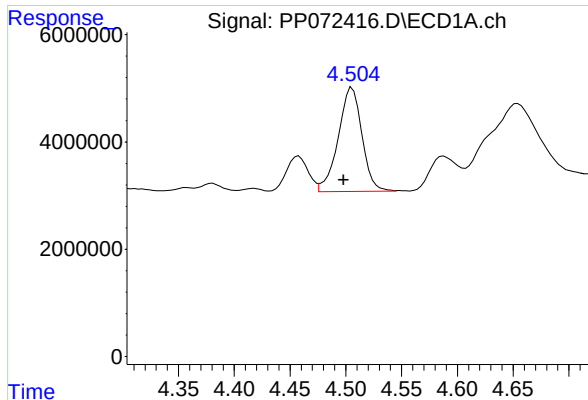


#1 Tetrachloro-m-xylene

R.T.: 4.504 min
Delta R.T.: 0.006 min
Response: 28643178
Conc: 14.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
CAM-40626


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2025
Supervised By :mohammad ahmed 05/30/2025

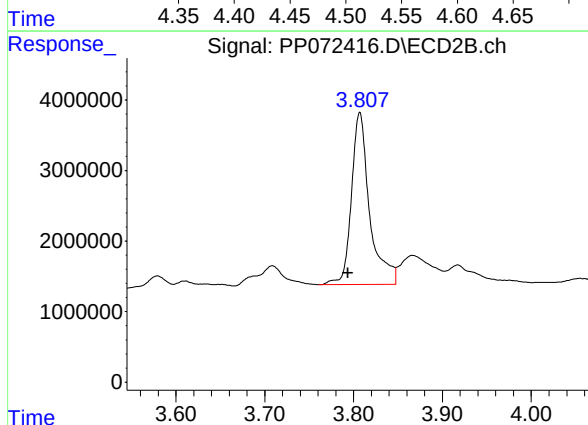


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.014 min
Response: 34628720
Conc: 21.67 ng/ml

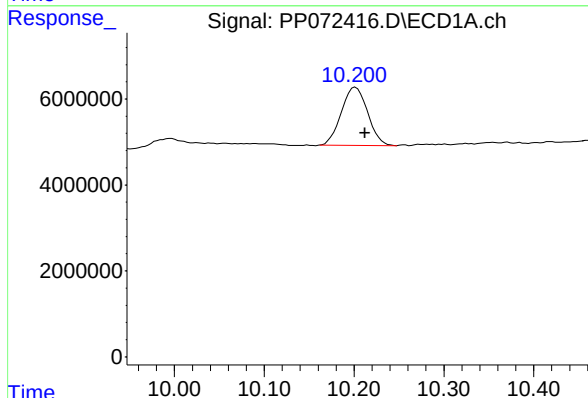

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: -0.010 min
Response: 27550824
Conc: 16.91 ng/ml

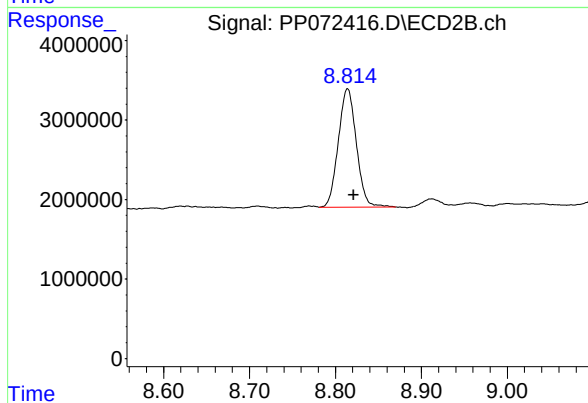

#2 Decachlorobiphenyl

R.T.: 8.814 min
Delta R.T.: -0.007 min
Response: 21715843
Conc: 20.51 ng/ml