

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052924\
 Data File : PP065335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2024 23:33
 Operator : YP\AJ
 Sample : P2651-02 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KEA125F-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

05/30/2024
 Supervised By :Ankita
 Jodhani

05/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 03:26:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.467	3.749	2634154	2935026	1.669m	1.933m
2) SA Decachlor...	10.205	8.815	2940200	2411593	2.261	1.830m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052924\
Data File : PP065335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2024 23:33
Operator : YP\AJ
Sample : P2651-02 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KEA125F-END-1-2

Manual Integrations
APPROVED



Reviewed By :Yogesh
Patel


05/30/2024
Supervised By :Ankita
Jodhani

05/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 03:26:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

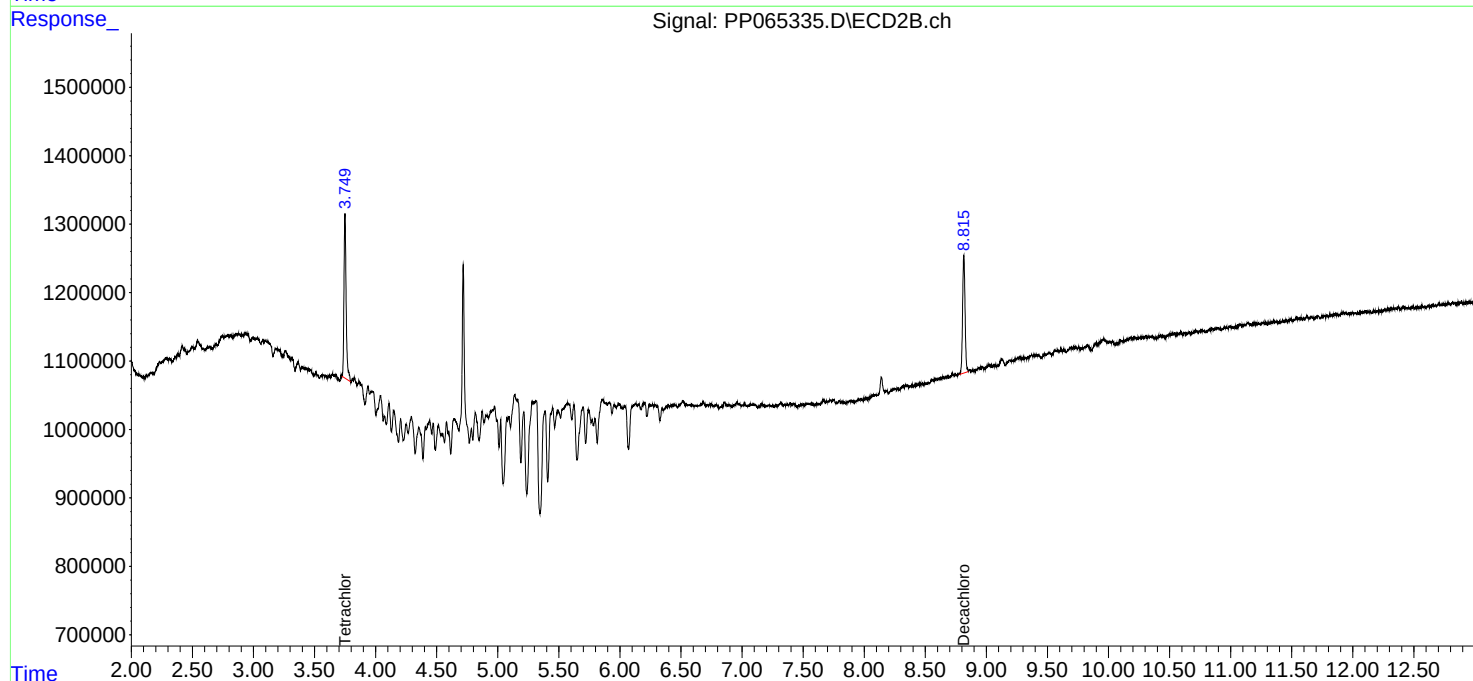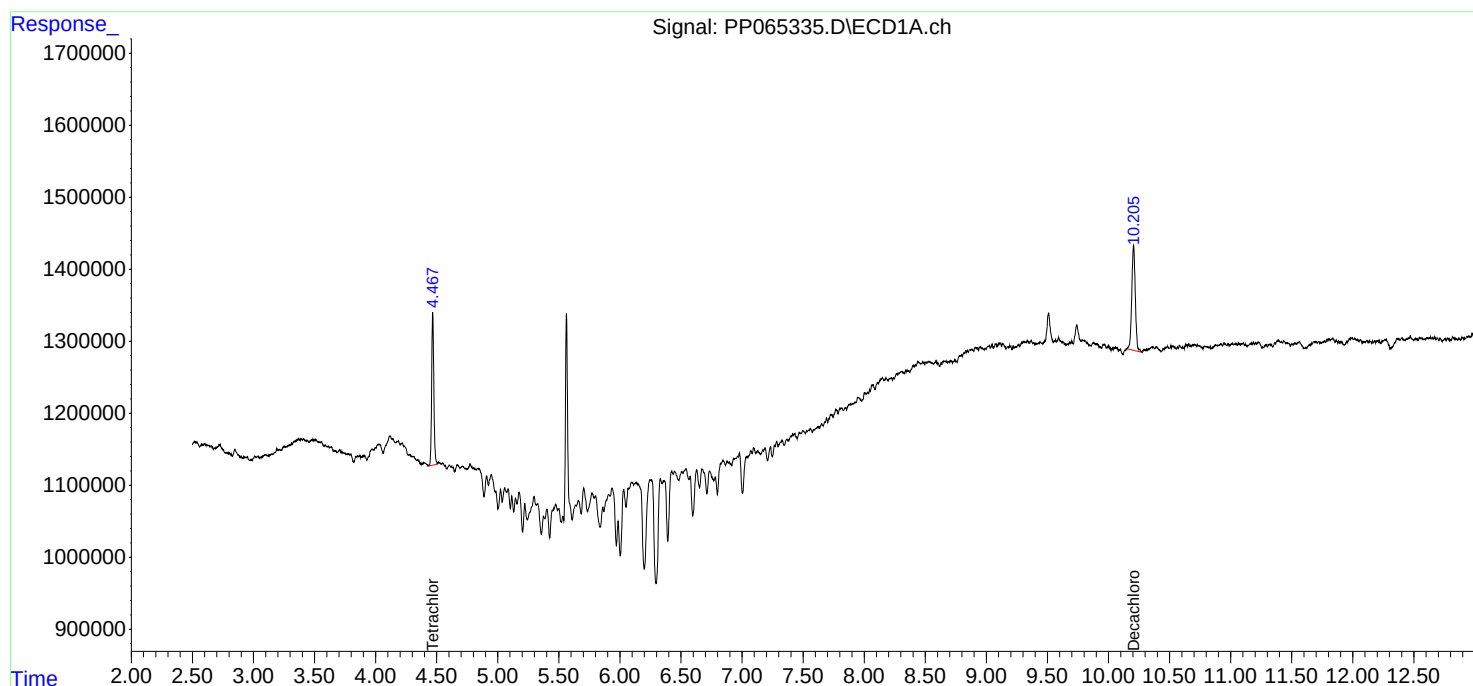

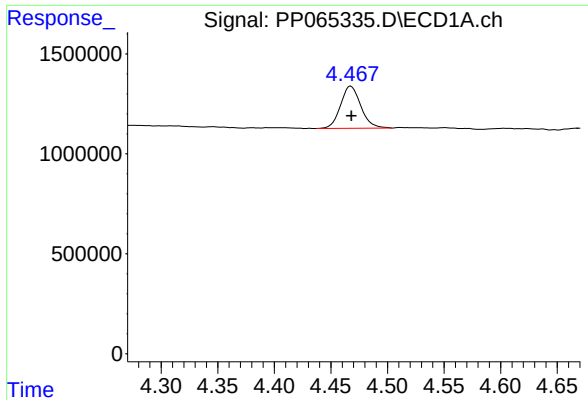

#1 Tetrachloro-m-xylene

R.T.: 4.467 min
Delta R.T.: -0.001 min
Response: 2634154
Conc: 1.67 ng/ml


Instrument :
ECD_P
ClientSampleId :
KEA125F-END-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel


05/30/2024
Supervised By :Ankita
Jodhani

05/30/2024

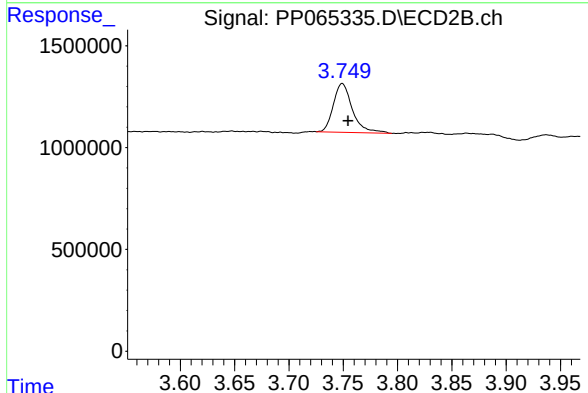


#1 Tetrachloro-m-xylene

R.T.: 3.749 min
Delta R.T.: -0.006 min
Response: 2935026
Conc: 1.93 ng/ml m

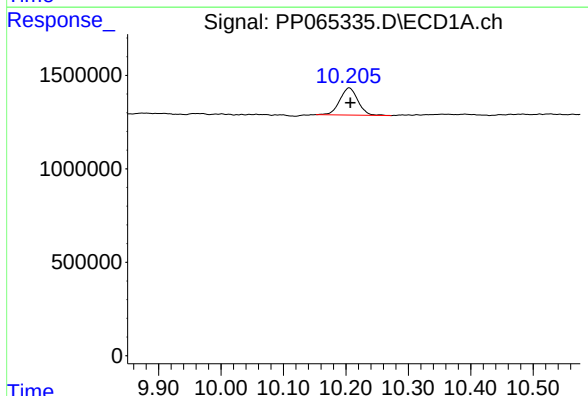

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.002 min
Response: 2940200
Conc: 2.26 ng/ml

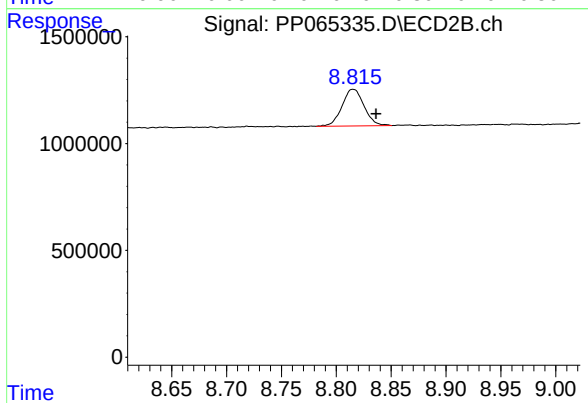

#2 Decachlorobiphenyl

R.T.: 8.815 min
Delta R.T.: -0.021 min
Response: 2411593
Conc: 1.83 ng/ml m