

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
 Data File : PP072438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2025 14:02
 Operator : YP\AJ
 Sample : Q2137-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-25-0151

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2025
 Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 04:23:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.794	81320253	1884661	40.442m	1.179m#
2) SA Decachlor...	10.193	8.811	2343267	1742040	1.438m	1.646

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
Data File : PP072438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2025 14:02
Operator : YP\AJ
Sample : Q2137-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-25-0151


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 04:23:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

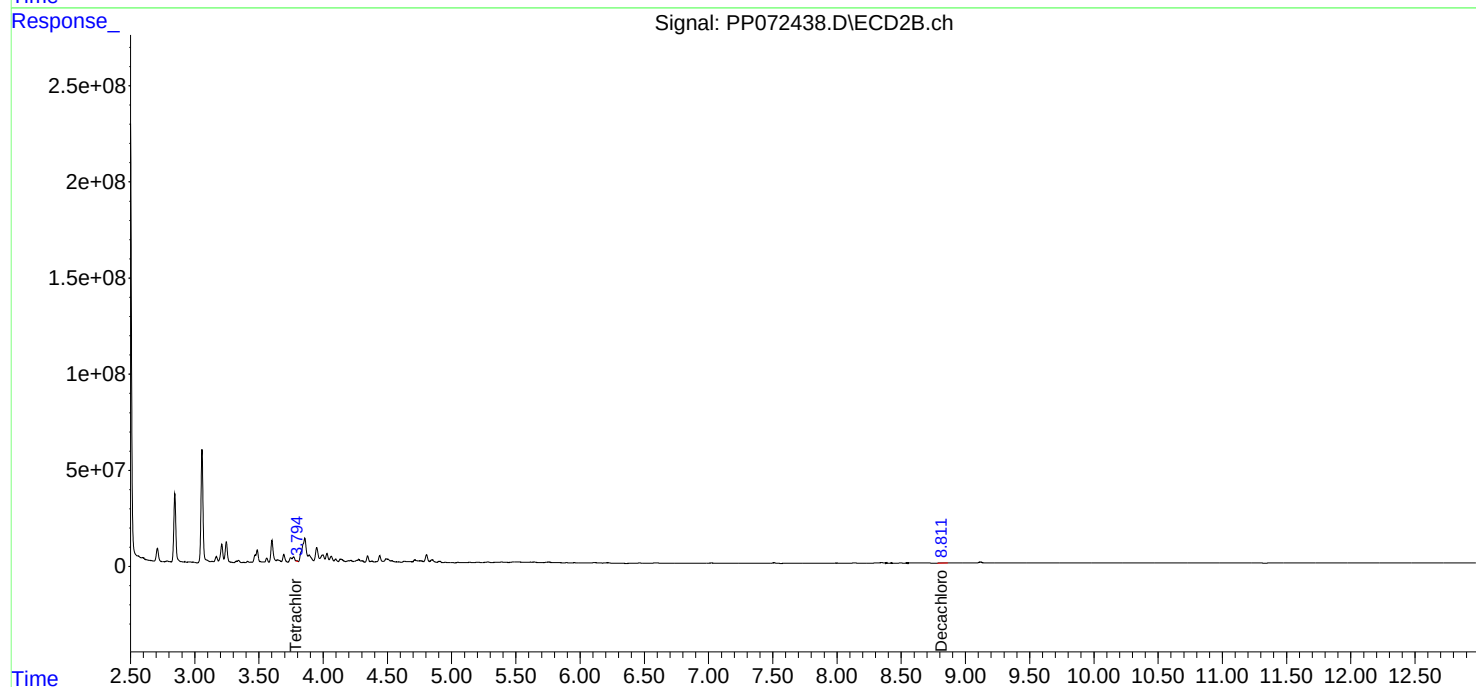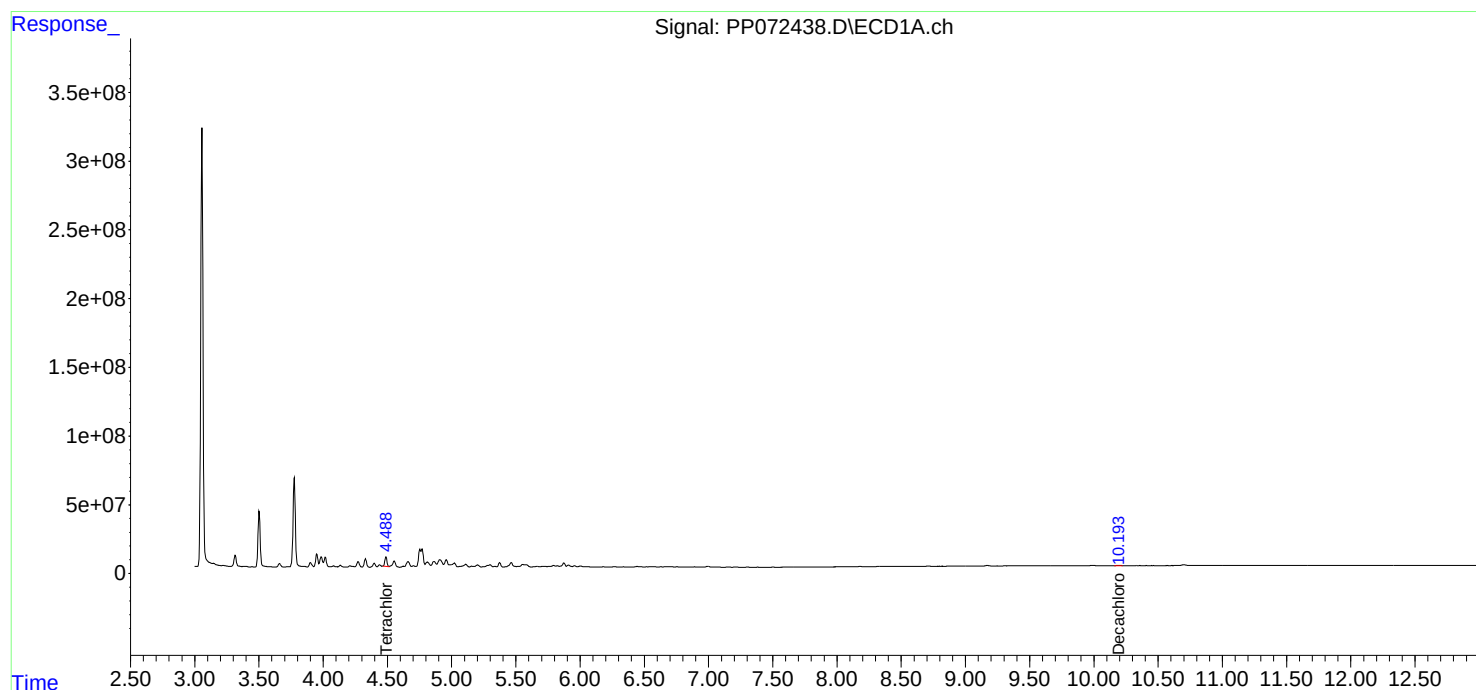

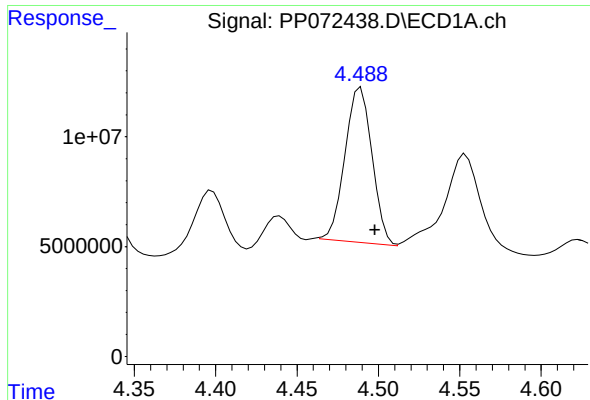


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.010 min
Response: 81320253
Conc: 40.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-25-0151


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

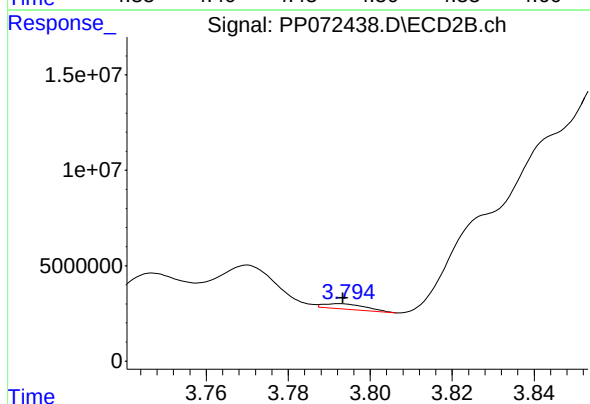


#1 Tetrachloro-m-xylene

R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 1884661
Conc: 1.18 ng/ml

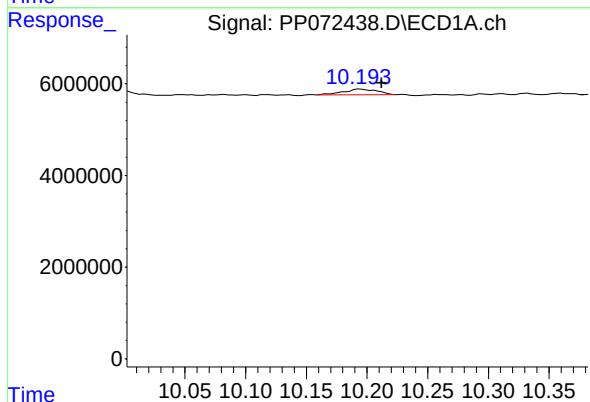

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.019 min
Response: 2343267
Conc: 1.44 ng/ml

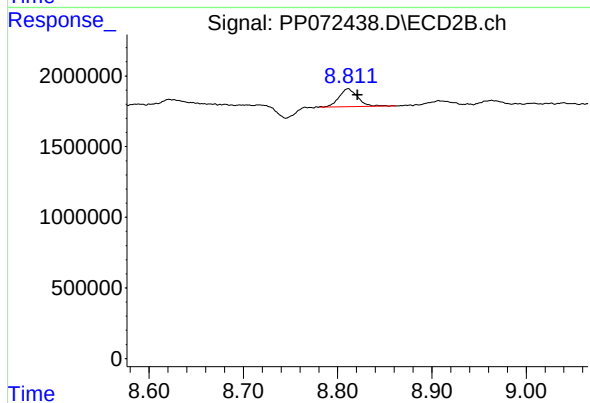

#2 Decachlorobiphenyl

R.T.: 8.811 min
Delta R.T.: -0.010 min
Response: 1742040
Conc: 1.65 ng/ml