

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
 Data File : PP072449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2025 19:15
 Operator : YP\AJ
 Sample : Q2154-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271336-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2025
 Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 04:24:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.500	3.795	2790099	2459724	1.388	1.539
2) SA Decachlor...	10.202	8.813	2418092	1829024	1.484	1.728m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
Data File : PP072449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2025 19:15
Operator : YP\AJ
Sample : Q2154-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC271336-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 04:24:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

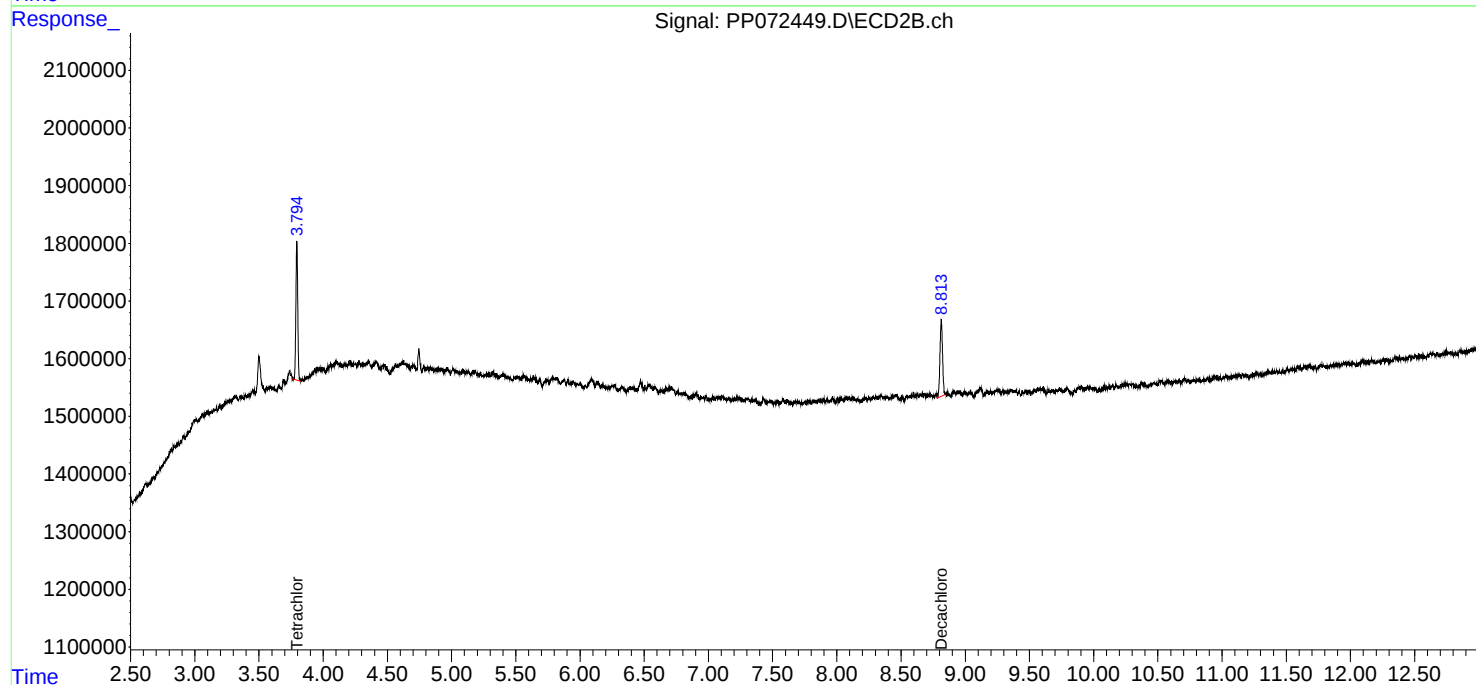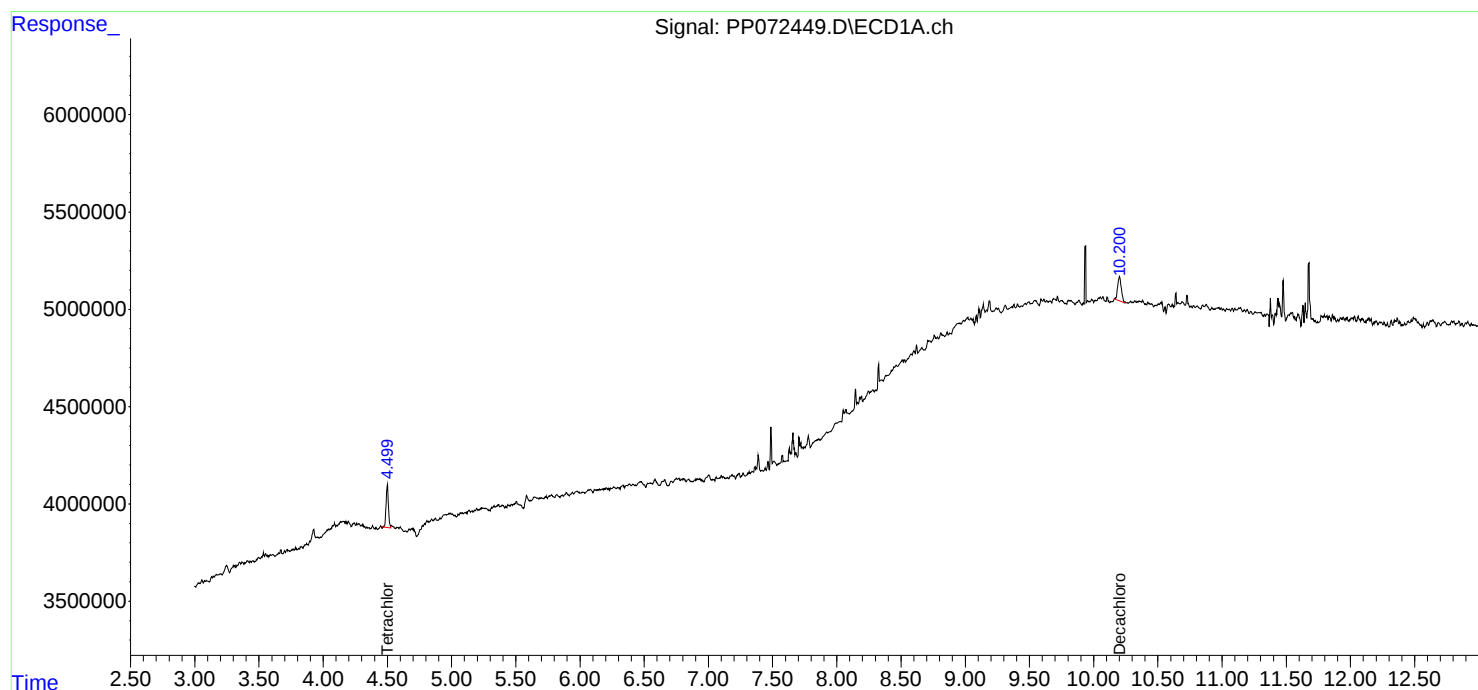

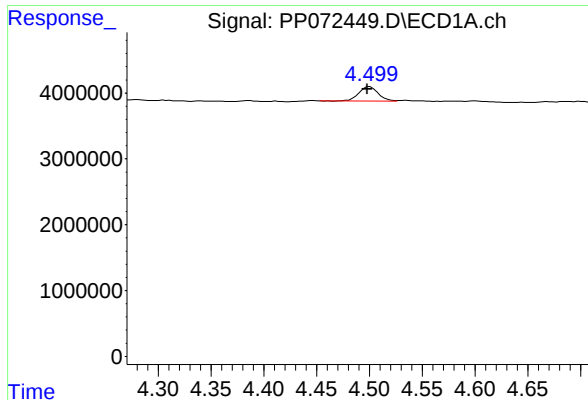


#1 Tetrachloro-m-xylene

R.T.: 4.500 min
Delta R.T.: 0.002 min
Response: 2790099
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271336-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

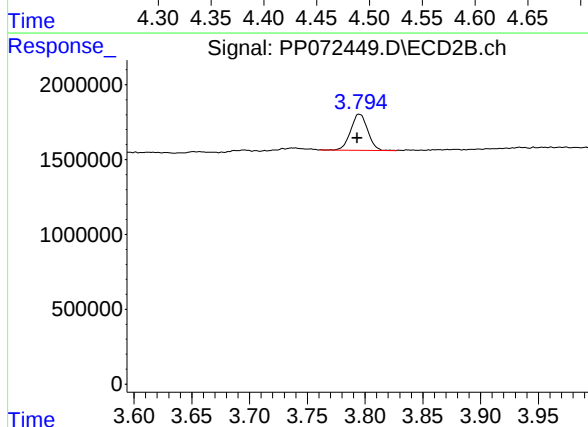


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: 0.002 min
Response: 2459724
Conc: 1.54 ng/ml

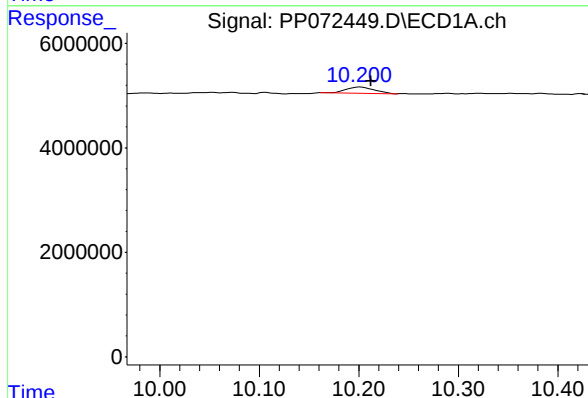

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: -0.010 min
Response: 2418092
Conc: 1.48 ng/ml

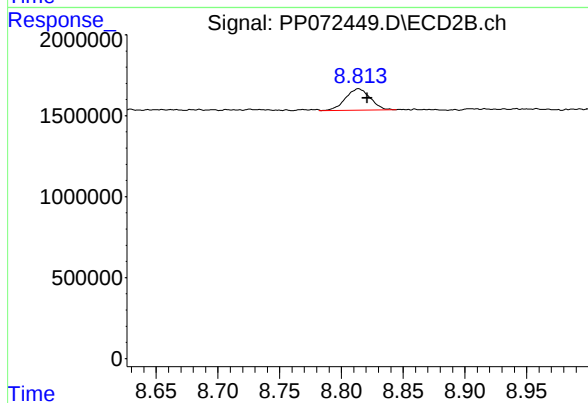

#2 Decachlorobiphenyl

R.T.: 8.813 min
Delta R.T.: -0.008 min
Response: 1829024
Conc: 1.73 ng/ml m