

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
 Data File : PP072459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2025 23:24
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2025
 Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 23:54:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.499	3.796	35543715	30647281	17.676	19.174
2) SA Decachlor...	10.200	8.814	31650775	23802688	19.428m	22.485

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052925\
Data File : PP072459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2025 23:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 23:54:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

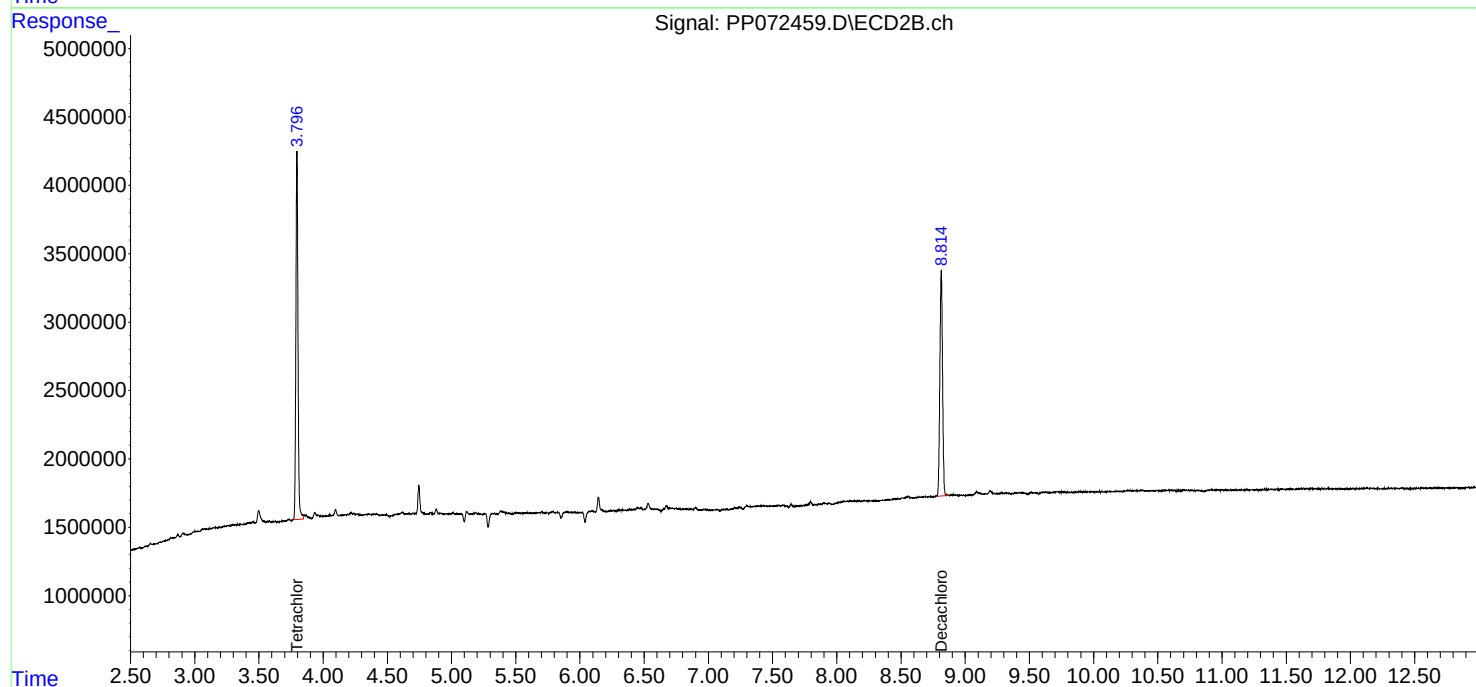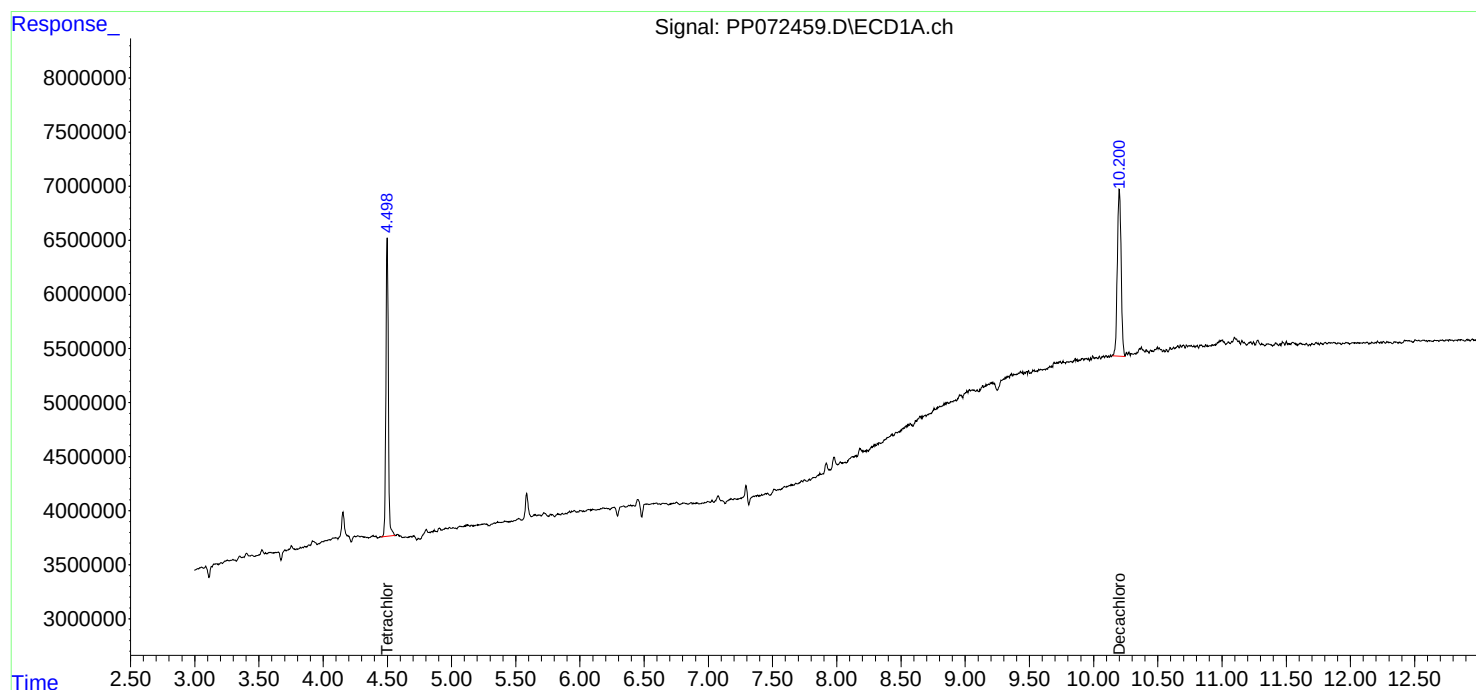

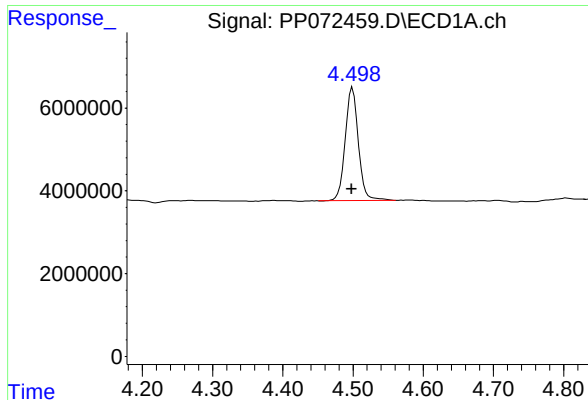


#1 Tetrachloro-m-xylene

R.T.: 4.499 min
Delta R.T.: 0.001 min
Response: 35543715
Conc: 17.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2025
Supervised By :mohammad ahmed 06/03/2025

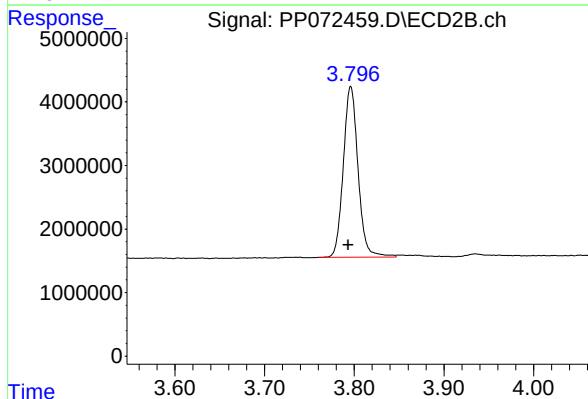


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: 0.003 min
Response: 30647281
Conc: 19.17 ng/ml

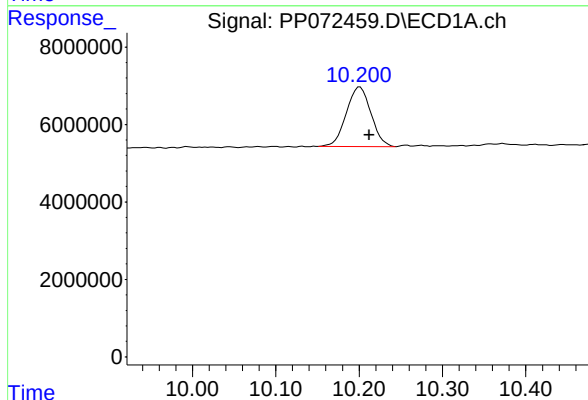

#2 Decachlorobiphenyl

R.T.: 10.200 min
Delta R.T.: -0.012 min
Response: 31650775
Conc: 19.43 ng/ml m

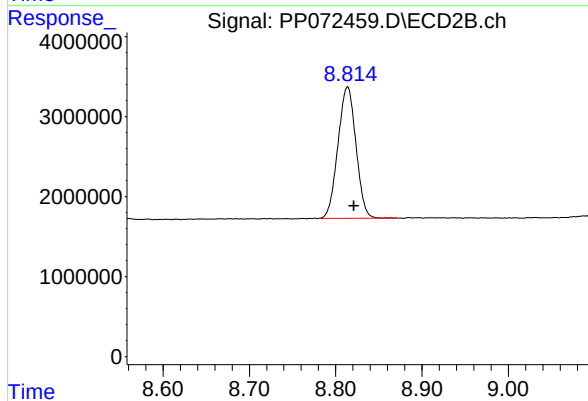

#2 Decachlorobiphenyl

R.T.: 8.814 min
Delta R.T.: -0.007 min
Response: 23802688
Conc: 22.49 ng/ml