

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053024\Not review data\
 Data File : PP065344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 10:15
 Operator : YP\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 09:04:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
2) SA Decachlor...	10.201	0.000	764524	0	0.588	N.D. #
Target Compounds						
24) L5 AR-1248-4	6.490f	0.000	155378	0	2.838	N.D. #
26) L6 AR-1254-1	6.490	0.000	155378	0	2.517	N.D. #
28) L6 AR-1254-3	7.070	0.000	134437	0	1.445	N.D. #
29) L6 AR-1254-4	7.334f	0.000	143311	0	2.364	N.D. #
30) L6 AR-1254-5	7.764	0.000	28985	0	0.413	N.D. #
32) L7 AR-1260-2	7.498	0.000	370398	0	4.796	N.D. #
33) L7 AR-1260-3	7.854	0.000	103372	0	1.727	N.D. #
34) L7 AR-1260-4	8.070	0.000	140189	0	2.082	N.D. #
36) L8 AR-1262-1	7.907	0.000	26476	0	0.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053024\Not review data\
Data File : PP065344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 10:15
Operator : YP\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 09:04:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

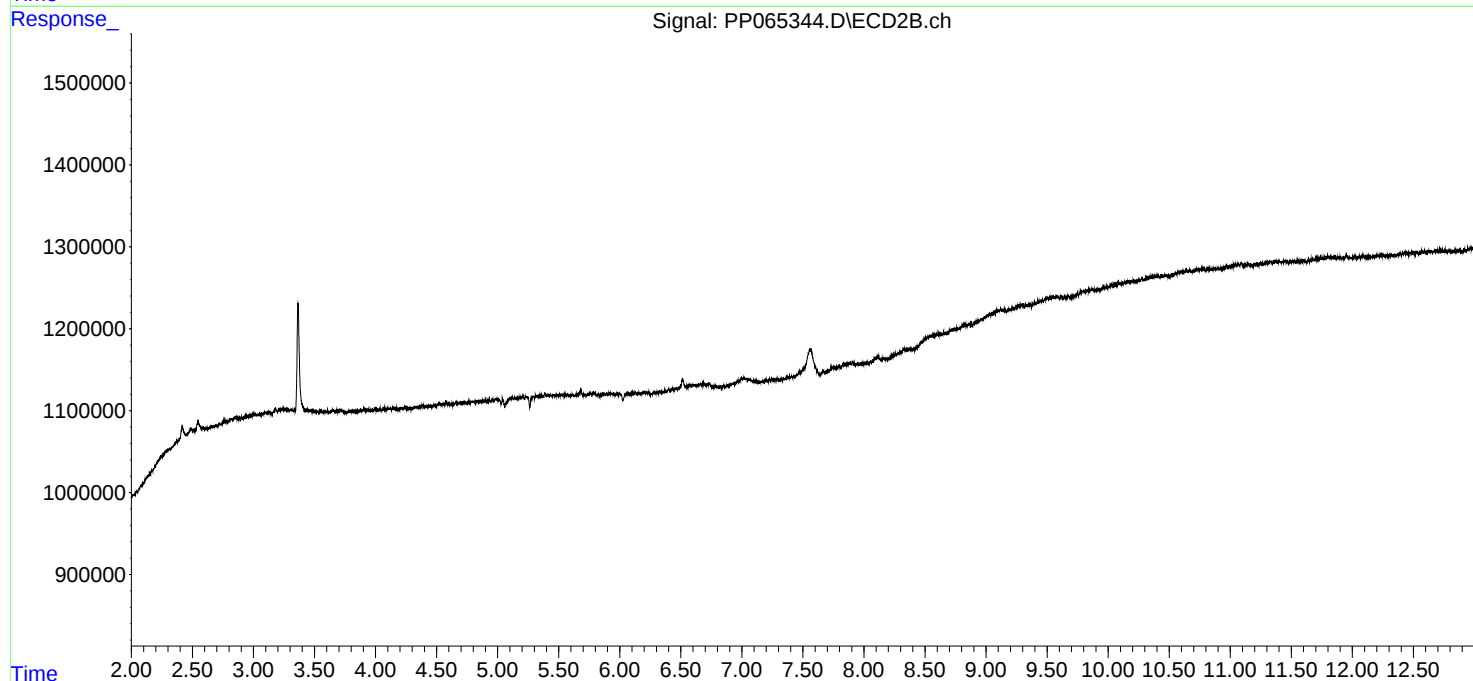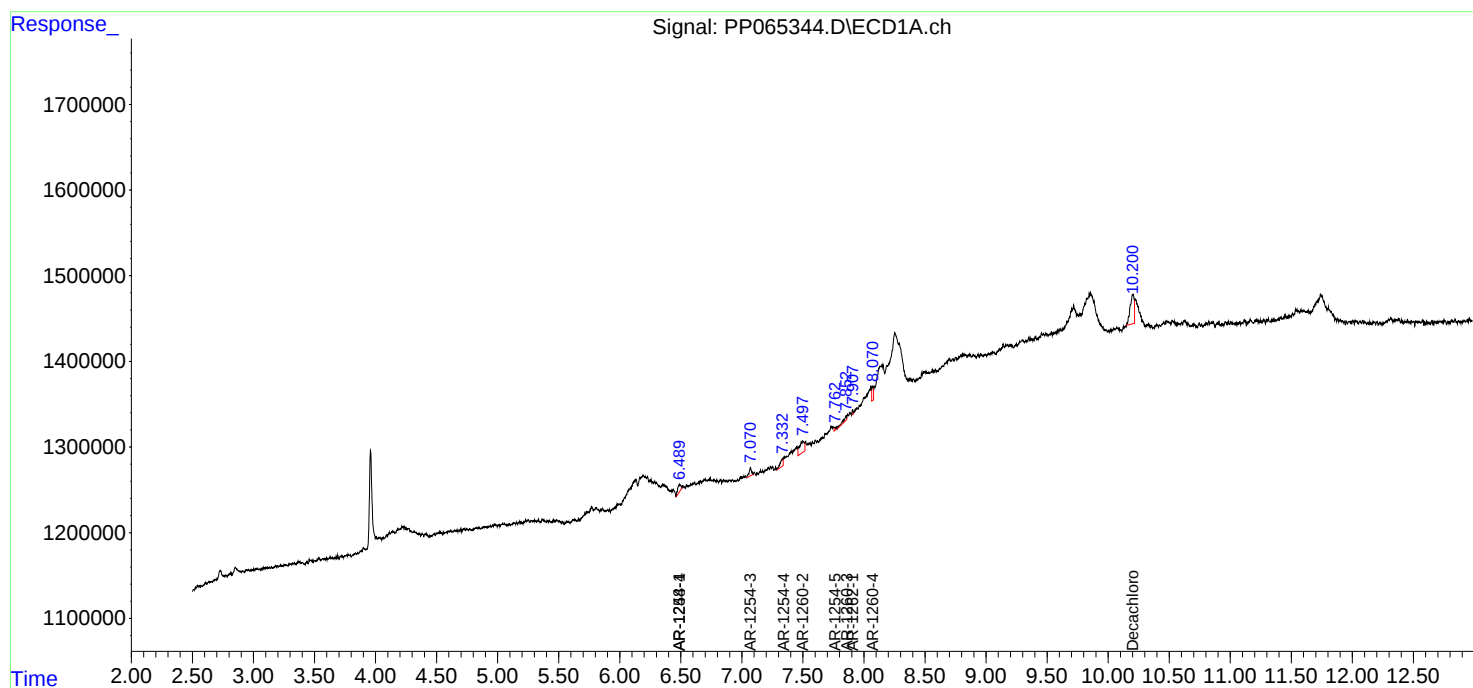

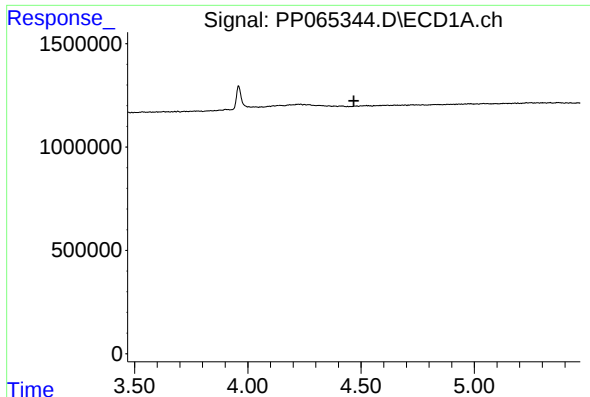

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.754 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 10.201 min
Delta R.T.: -0.007 min
Response: 764524
Conc: 0.59 ng/ml

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.836 min
Response: 0
Conc: N.D.

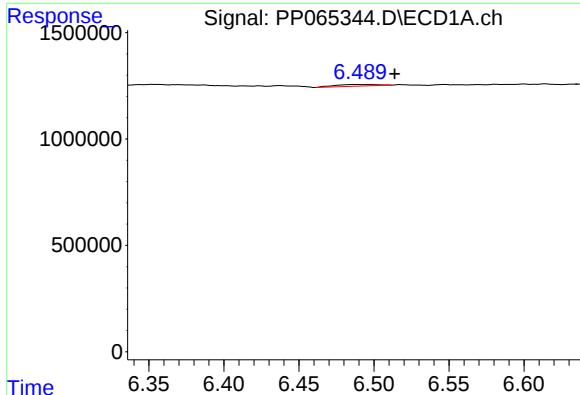

#24 AR-1248-4


R.T.: 6.490 min
Delta R.T.: -0.024 min
Response: 155378
Conc: 2.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

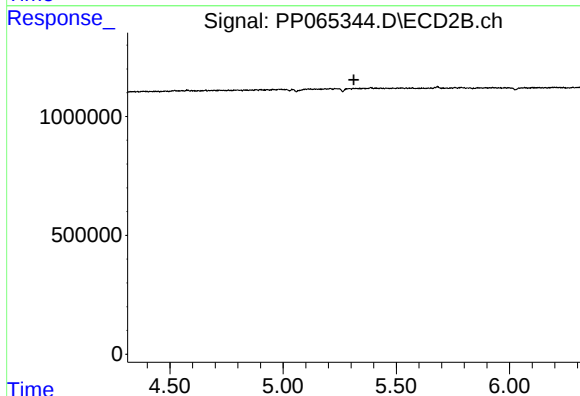


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.313 min
Response: 0
Conc: N.D.

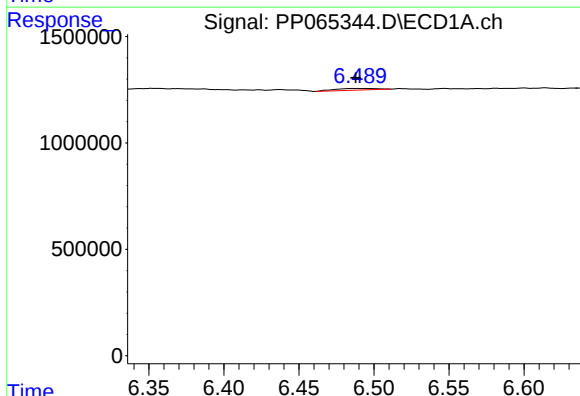


#26 AR-1254-1

R.T.: 6.490 min
Delta R.T.: 0.002 min
Response: 155378
Conc: 2.52 ng/ml

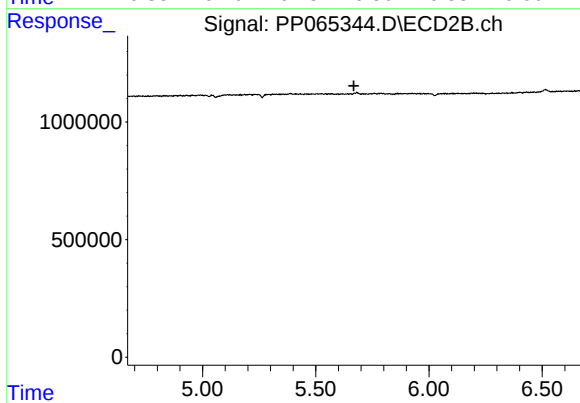

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

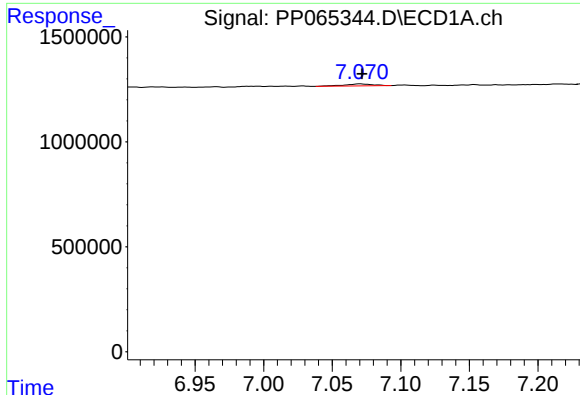

#28 AR-1254-3


R.T.: 7.070 min
Delta R.T.: -0.002 min
Response: 134437
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

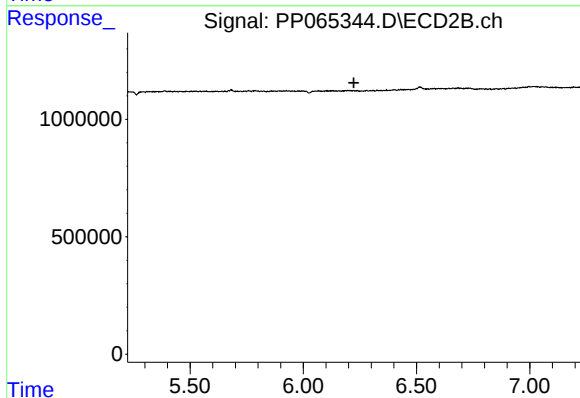


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.223 min
Response: 0
Conc: N.D.

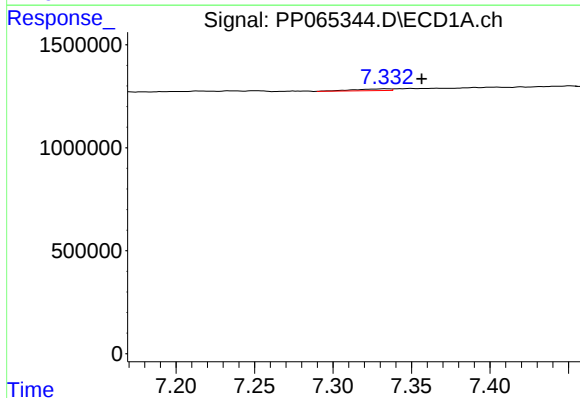


#29 AR-1254-4

R.T.: 7.334 min
Delta R.T.: -0.023 min
Response: 143311
Conc: 2.36 ng/ml

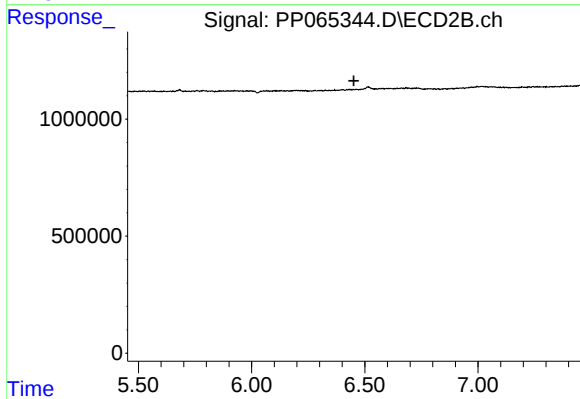

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

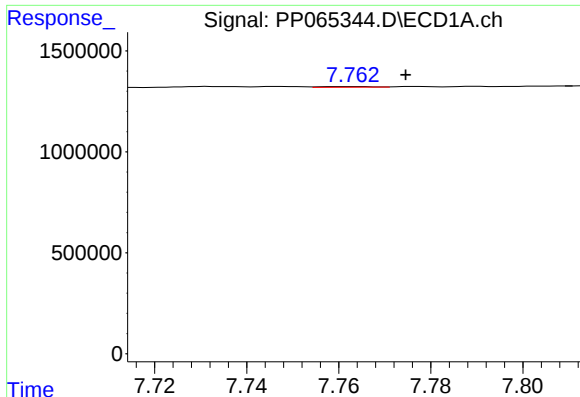

#30 AR-1254-5


R.T.: 7.764 min
Delta R.T.: -0.011 min
Response: 28985
Conc: 0.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

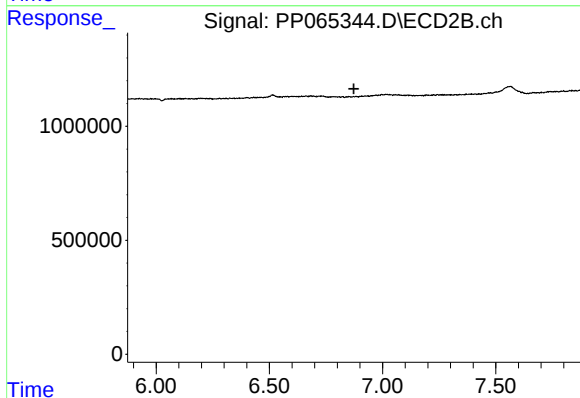


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.873 min
Response: 0
Conc: N.D.

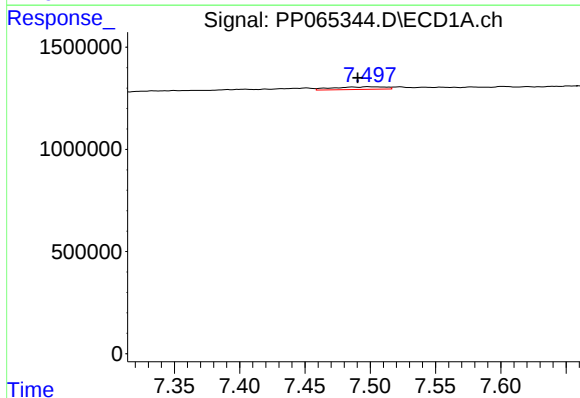


#32 AR-1260-2

R.T.: 7.498 min
Delta R.T.: 0.008 min
Response: 370398
Conc: 4.80 ng/ml

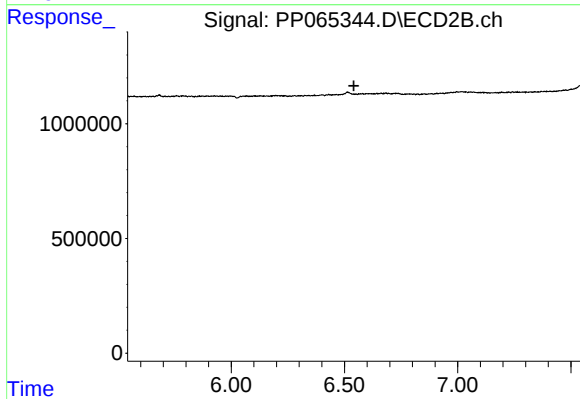

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

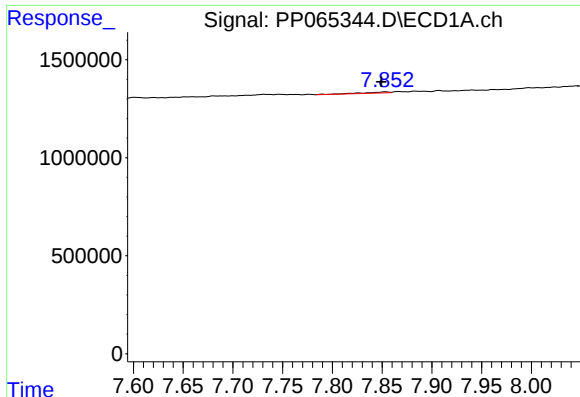

#33 AR-1260-3


R.T.: 7.854 min
Delta R.T.: 0.004 min
Response: 103372
Conc: 1.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

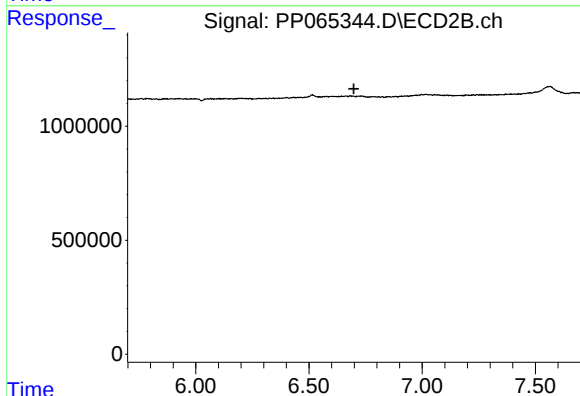


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.699 min
Response: 0
Conc: N.D.

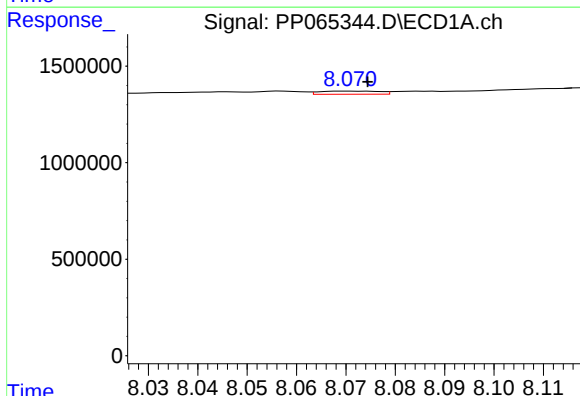


#34 AR-1260-4

R.T.: 8.070 min
Delta R.T.: -0.004 min
Response: 140189
Conc: 2.08 ng/ml

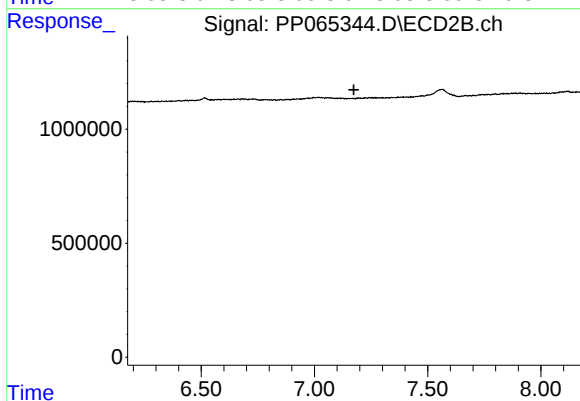

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.174 min
Response: 0
Conc: N.D.

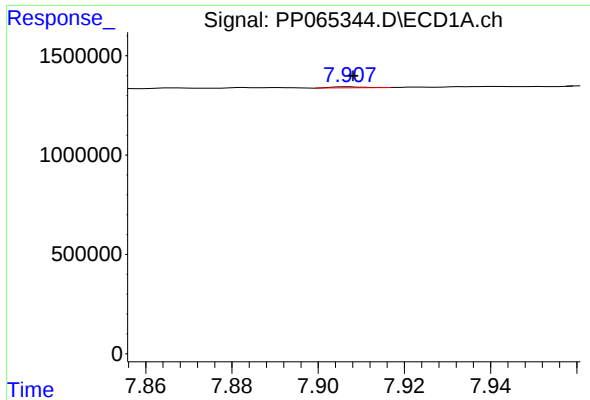

#36 AR-1262-1

R.T.: 7.907 min
Delta R.T.: -0.001 min
Response: 26476
Conc: 0.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

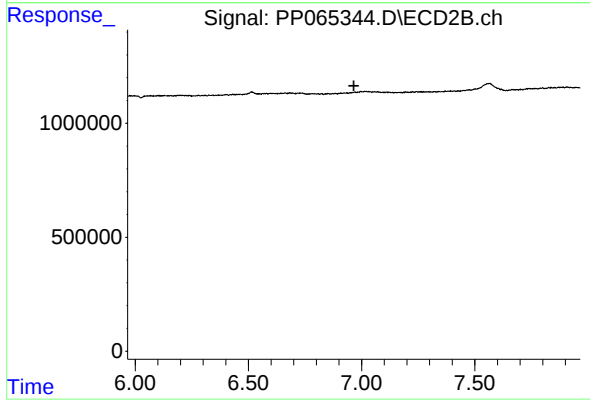

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.966 min
Response: 0
Conc: N.D.