

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053025\
 Data File : PP072475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2025 15:26
 Operator : YP\AJ
 Sample : Q2150-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-50

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/02/2025
 Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 16:54:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.500	3.797	36131864	32392944	17.969m	20.266
2) SA Decachlor...	10.209	8.817	27566306	18859144	16.921	17.815

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053025\
Data File : PP072475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2025 15:26
Operator : YP\AJ
Sample : Q2150-06
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-50


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2025
Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 16:54:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

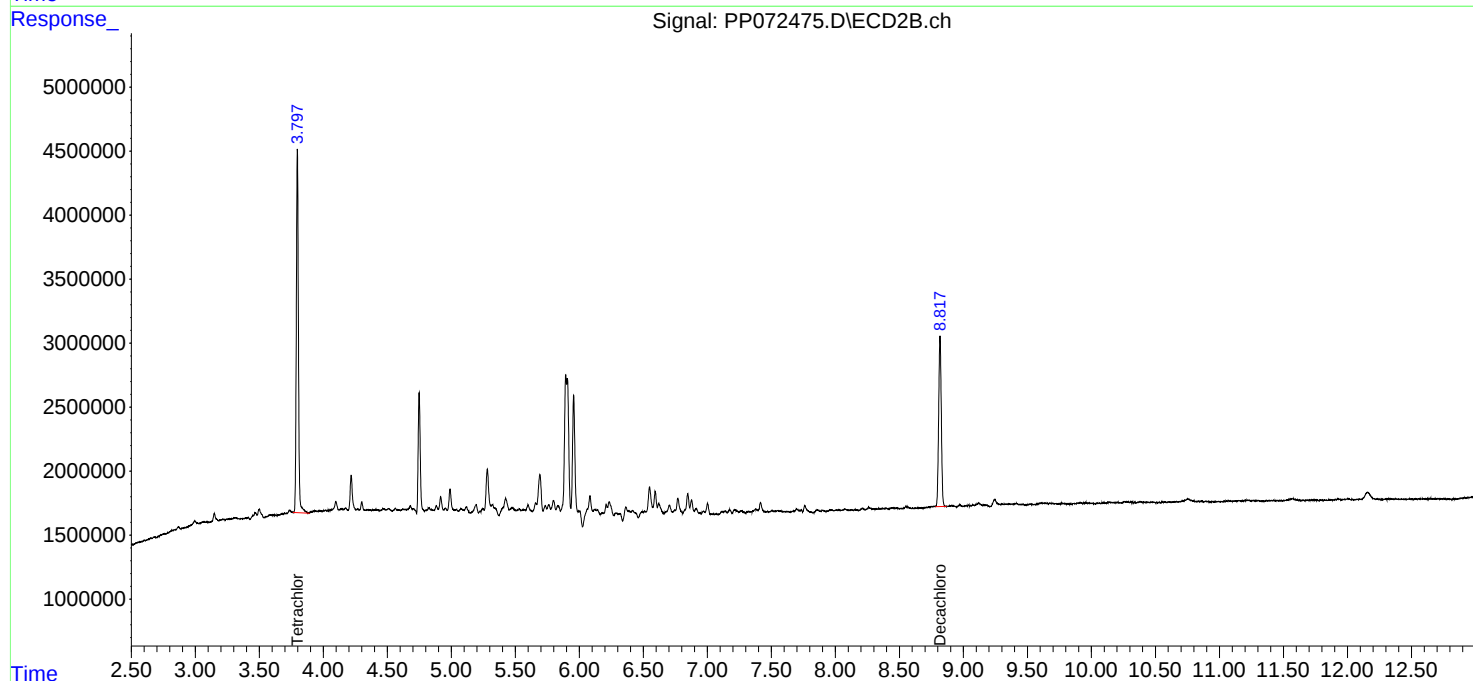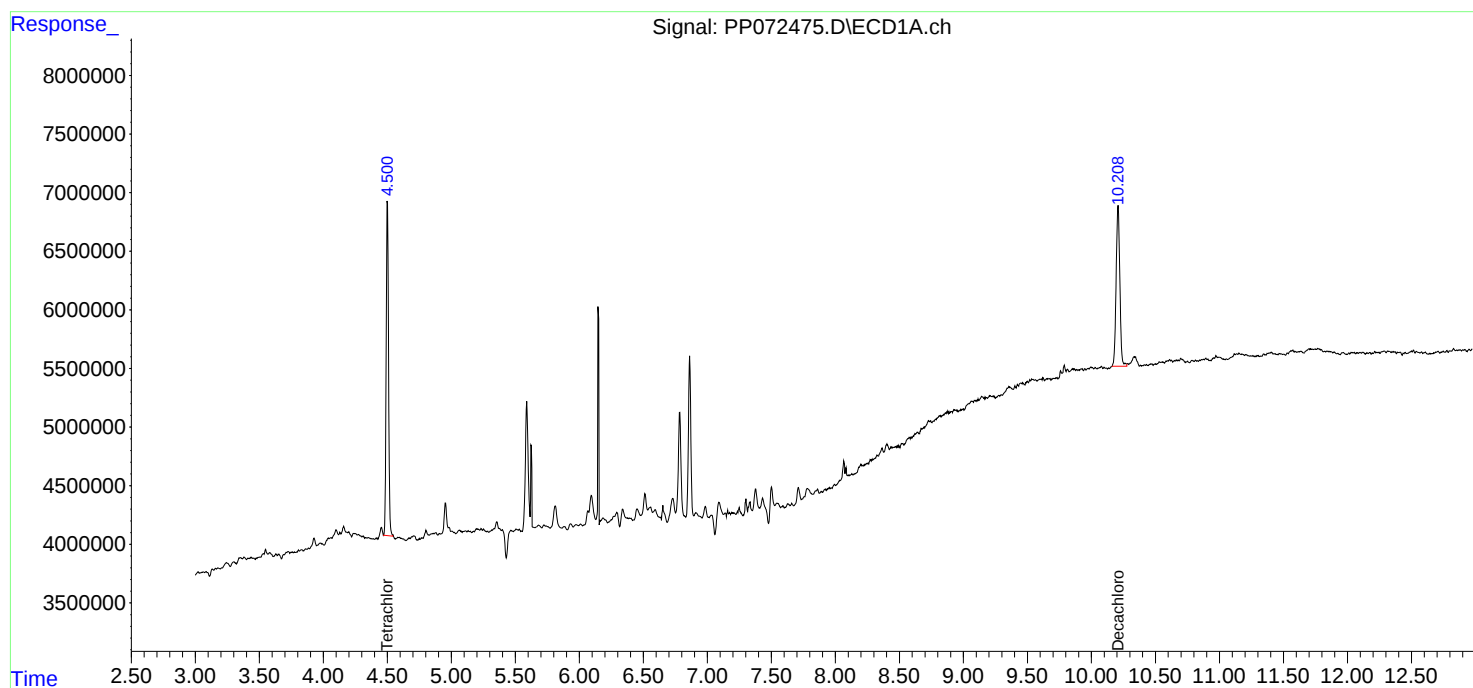

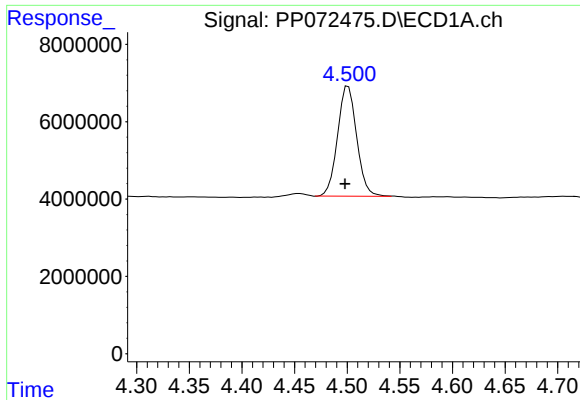


#1 Tetrachloro-m-xylene

R.T.: 4.500 min
Delta R.T.: 0.002 min
Response: 36131864
Conc: 17.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-50


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2025
Supervised By :mohammad ahmed 06/03/2025

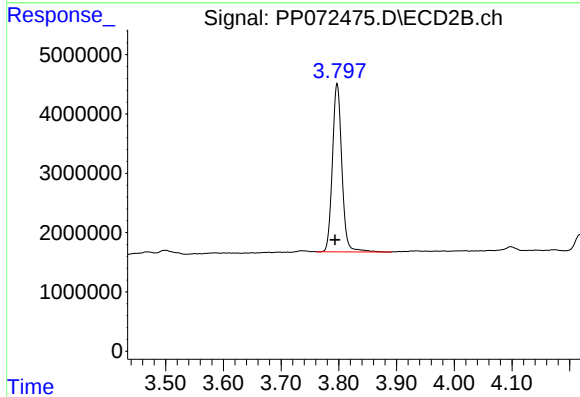


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: 0.004 min
Response: 32392944
Conc: 20.27 ng/ml

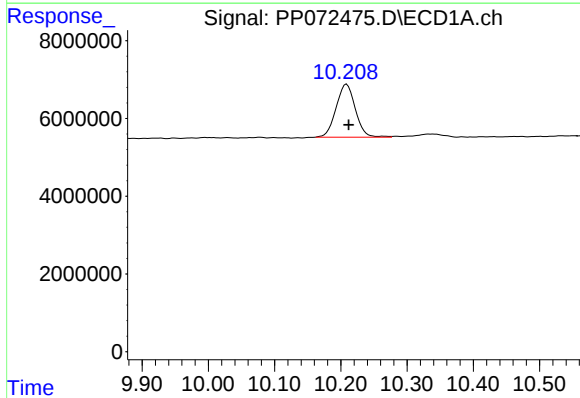

#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.003 min
Response: 27566306
Conc: 16.92 ng/ml

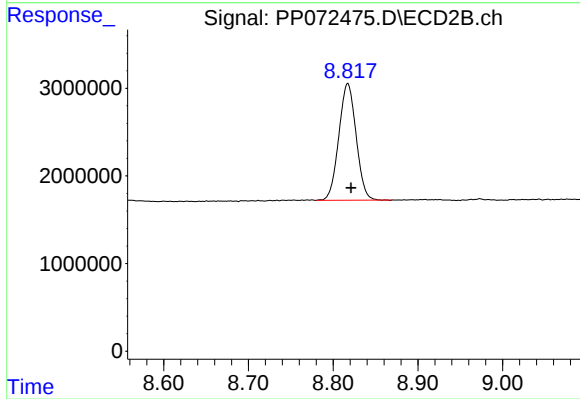

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: -0.004 min
Response: 18859144
Conc: 17.82 ng/ml