

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053025\
 Data File : PP072487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2025 19:15
 Operator : YP\AJ
 Sample : Q2153-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-04-0592025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/02/2025
 Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 22:56:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.501	3.796	33318470	30548102	16.570m	19.112
2) SA Decachlor...	10.211	8.818	23252100	16422859	14.273	15.514

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053025\
Data File : PP072487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2025 19:15
Operator : YP\AJ
Sample : Q2153-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-04-0592025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2025
Supervised By :mohammad ahmed 06/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 22:56:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

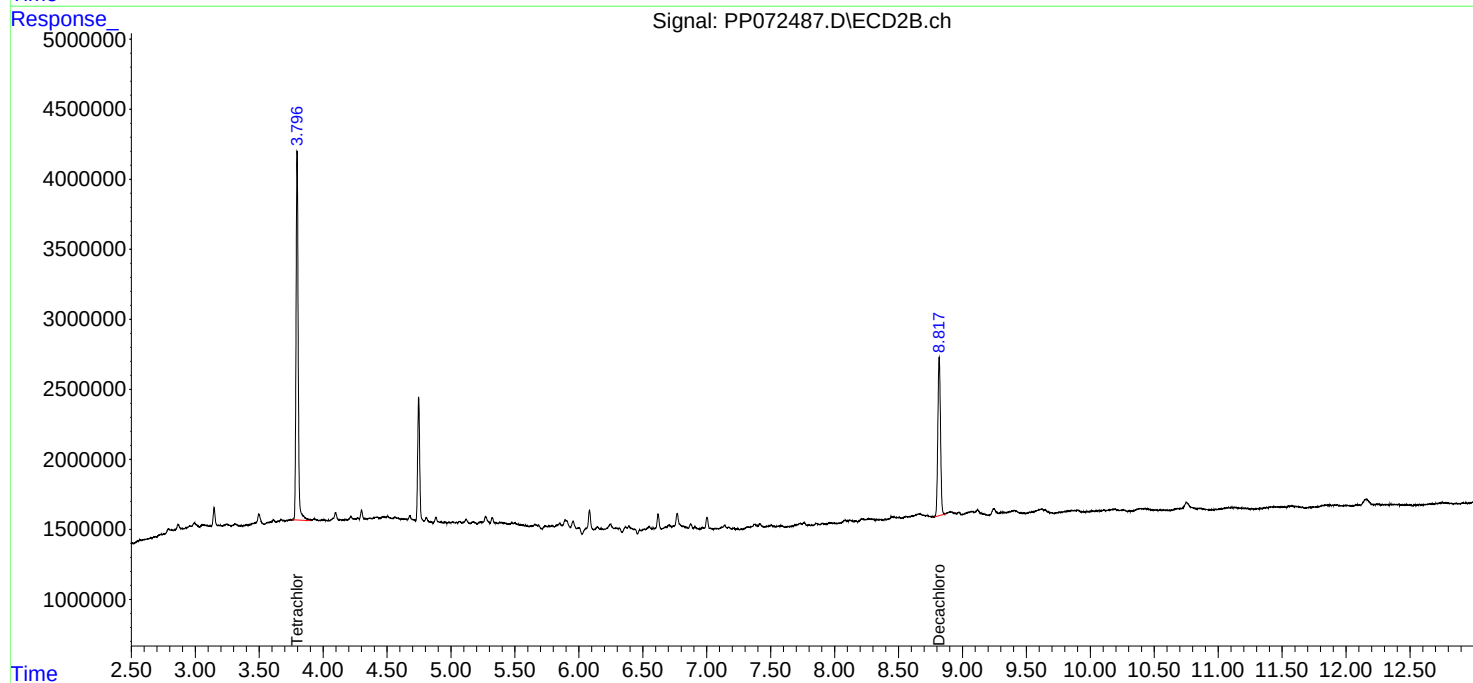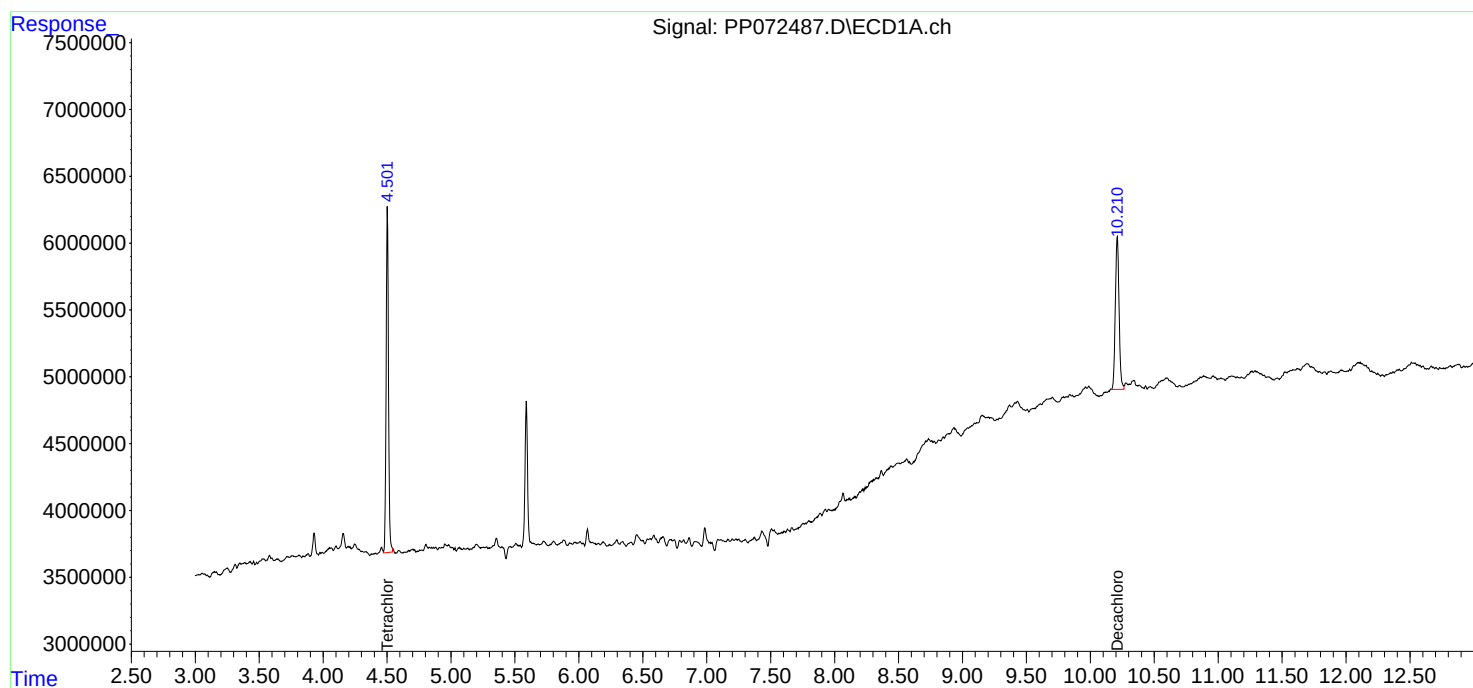

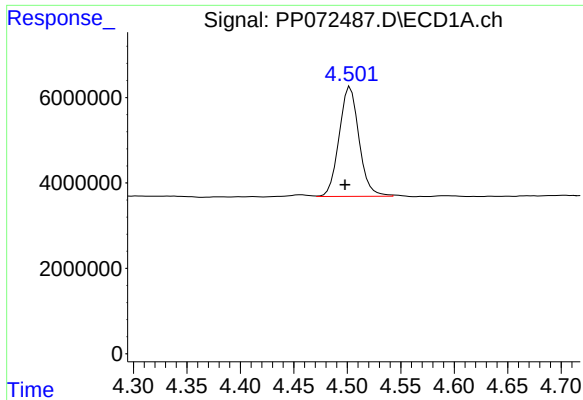


#1 Tetrachloro-m-xylene

R.T.: 4.501 min
Delta R.T.: 0.003 min
Response: 33318470
Conc: 16.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-04-0592025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2025
Supervised By :mohammad ahmed 06/03/2025

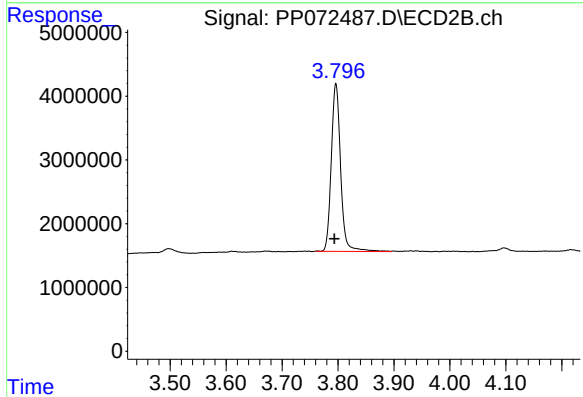


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: 0.003 min
Response: 30548102
Conc: 19.11 ng/ml

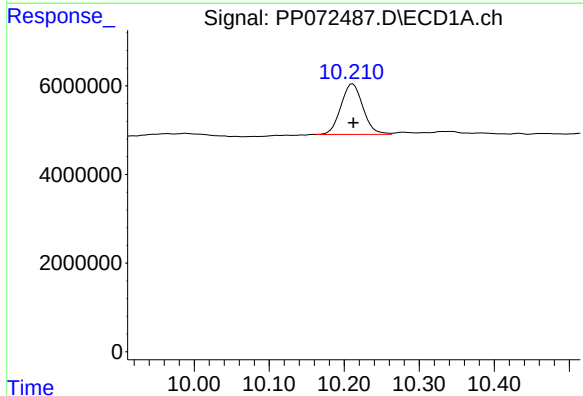

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.000 min
Response: 23252100
Conc: 14.27 ng/ml

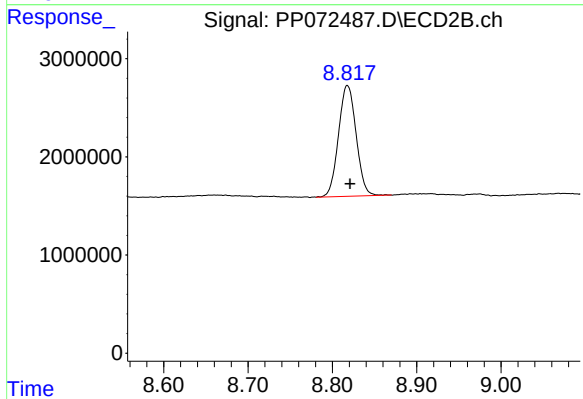

#2 Decachlorobiphenyl

R.T.: 8.818 min
Delta R.T.: -0.003 min
Response: 16422859
Conc: 15.51 ng/ml