

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053122\
 Data File : PP048212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 09:16
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/01/2022
 Supervised By :Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 16:02:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 27 23:53:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.037	3.218	59064909	46462674	25.222m	23.576
2) SA Decachlor...	10.392	8.652	36786990	39549199	18.927m	24.466 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP053122\
Data File : PP048212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 09:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/01/2022
Supervised By :Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 16:02:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 27 23:53:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

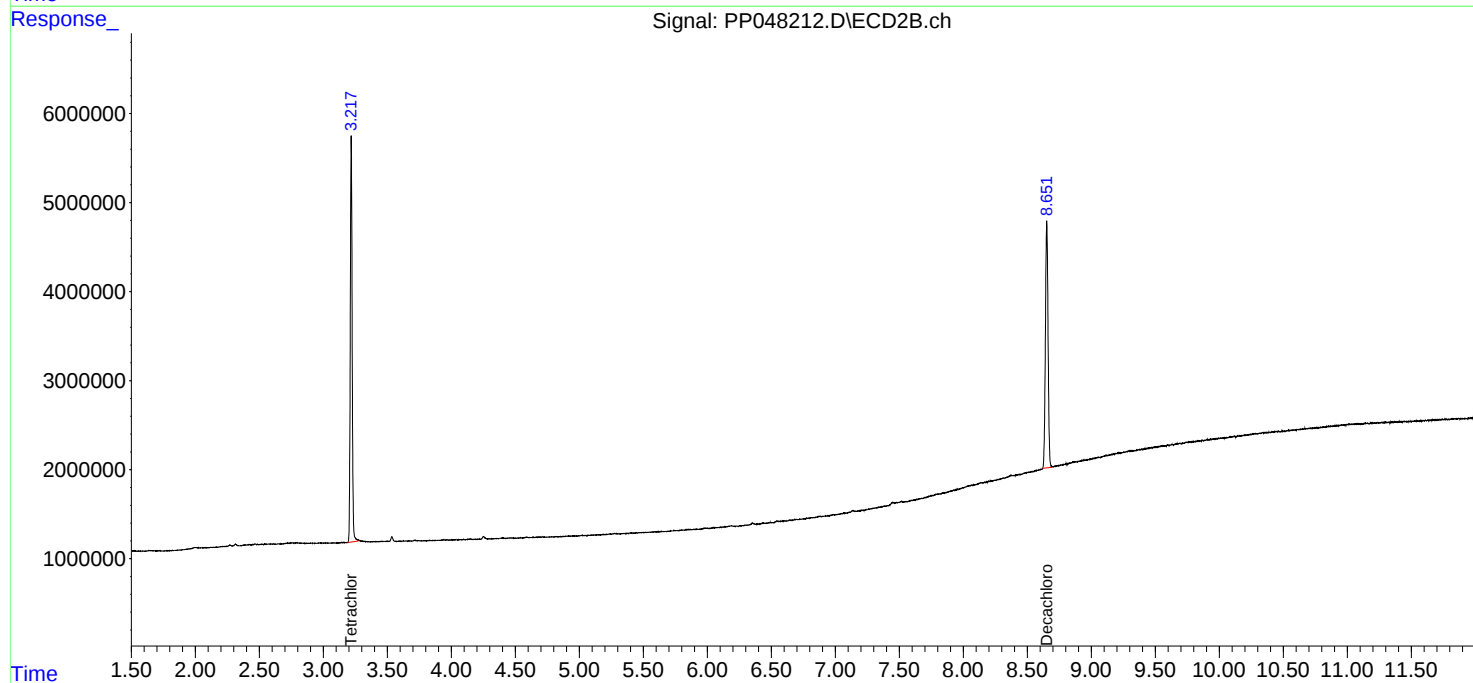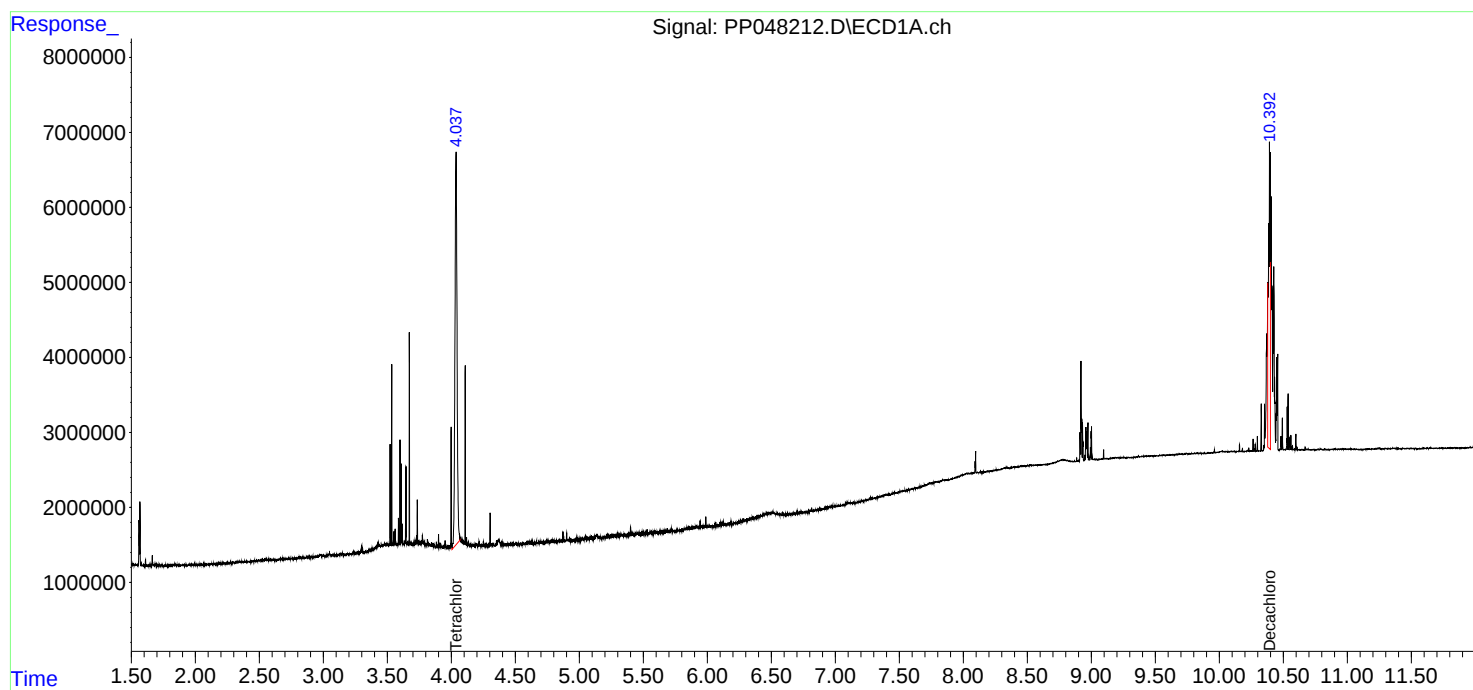

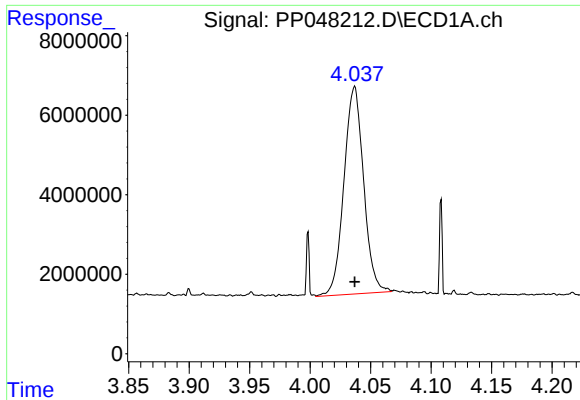


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 59064909
Conc: 25.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/01/2022
Supervised By :Ankita Jodhani 06/01/2022

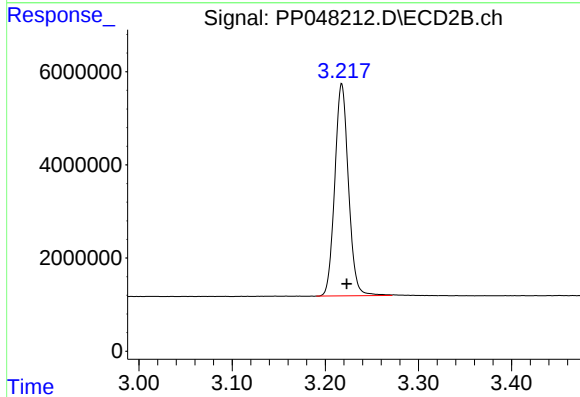


#1 Tetrachloro-m-xylene

R.T.: 3.218 min
Delta R.T.: -0.005 min
Response: 46462674
Conc: 23.58 ng/ml

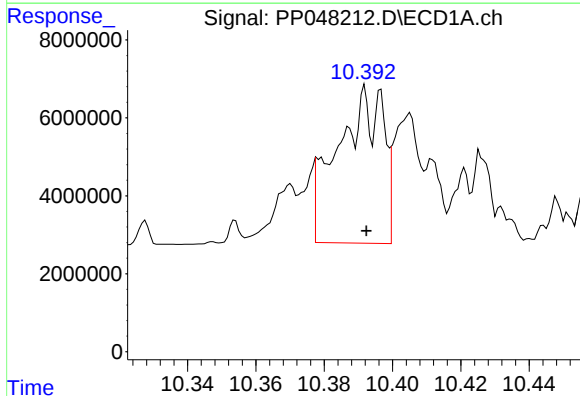

#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 36786990
Conc: 18.93 ng/ml m

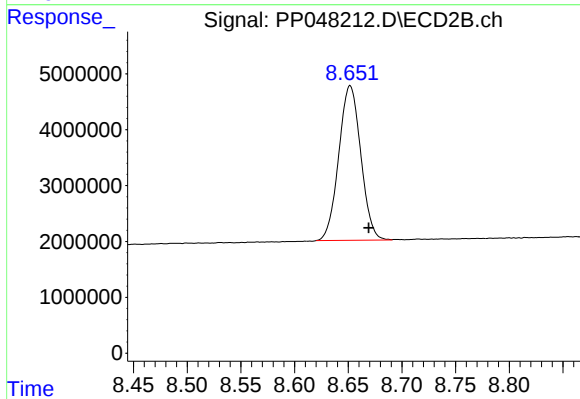

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.017 min
Response: 39549199
Conc: 24.47 ng/ml