

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060123\
 Data File : PP058139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2023 20:03
 Operator : YP\AJ
 Sample : 02985-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PLYMOUTH-XRDS-001

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/02/2023
 Supervised By :Ankita Jodhani 06/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 21:26:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.620	45201903	48112524	20.604	21.211
2) SA Decachlor...	10.201	8.677	23506682	25767432	20.743	16.415

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060123\
Data File : PP058139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2023 20:03
Operator : YP\AJ
Sample : 02985-02
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PLYMOUTH-XRDS-001


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2023
Supervised By :Ankita Jodhani 06/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 21:26:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

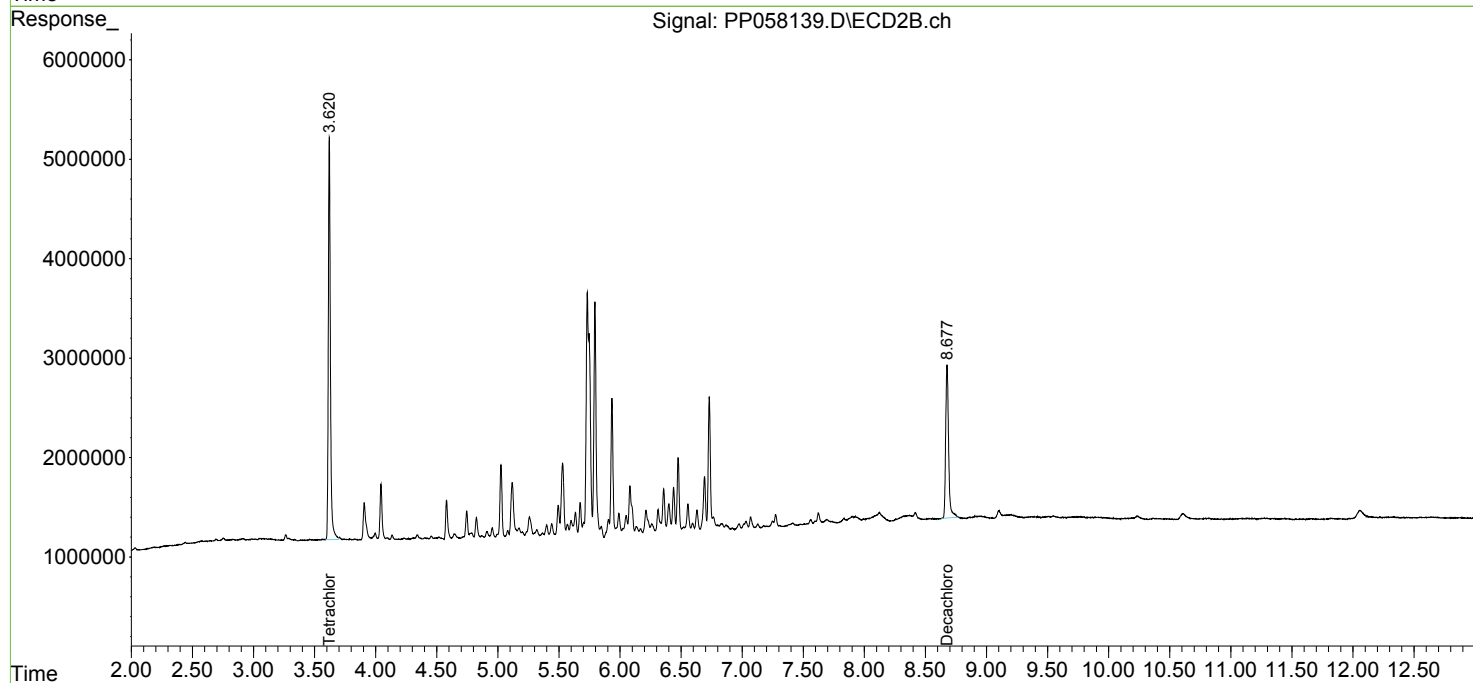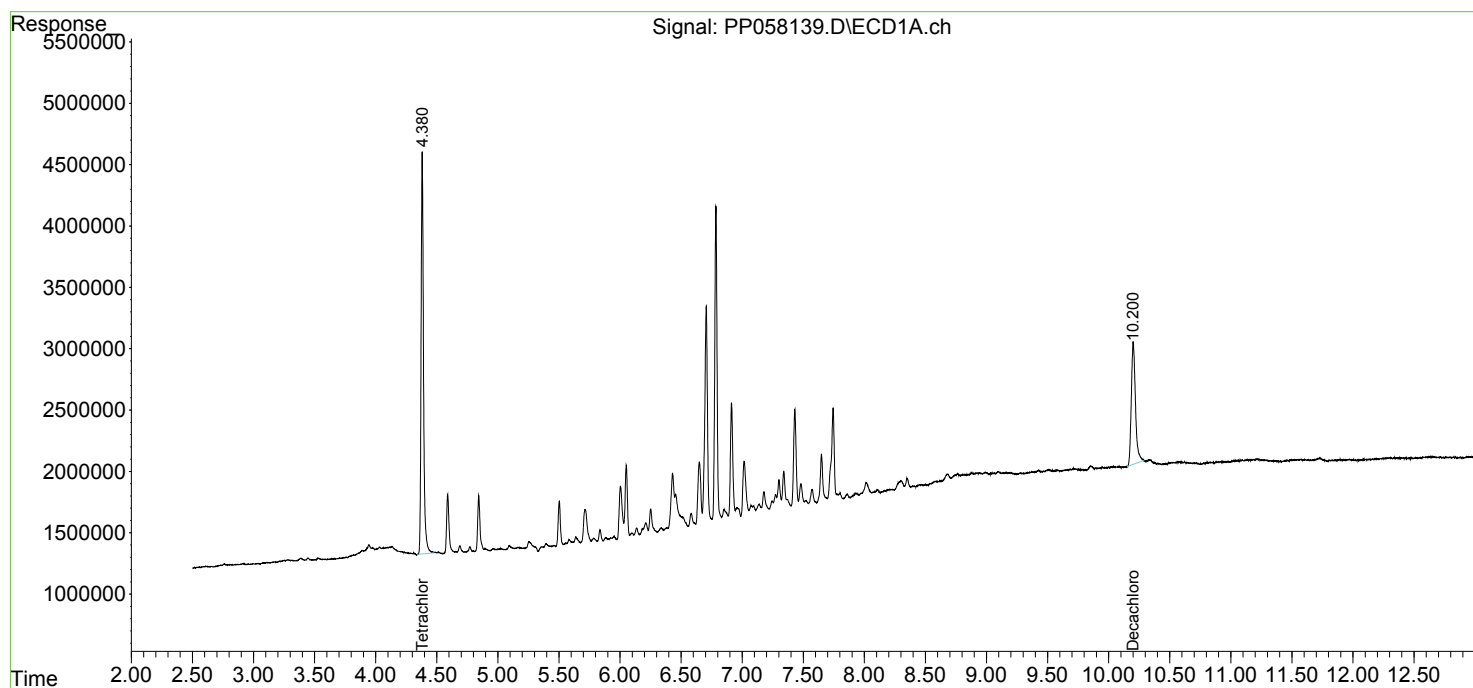

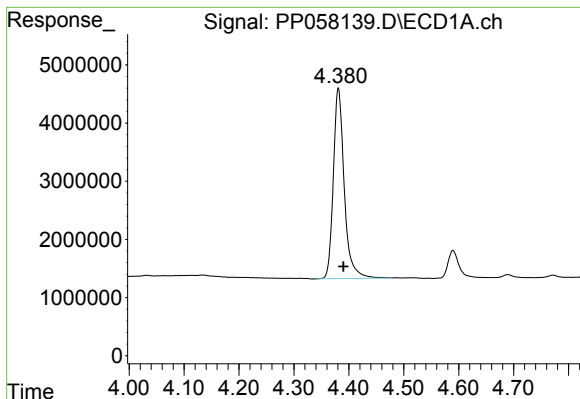


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: -0.009 min
Response: 45201903
Conc: 20.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLYMOUTH-XRDS-001


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/02/2023
Supervised By :Ankita Jodhani 06/02/2023

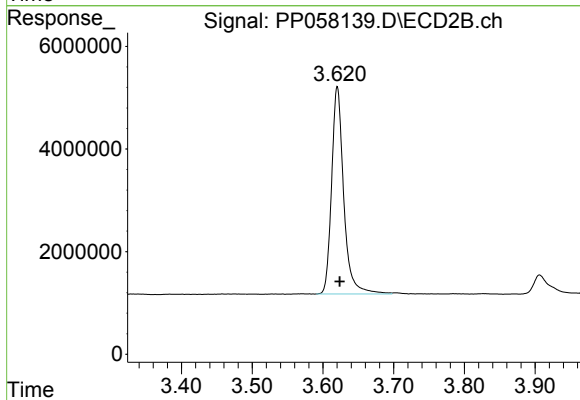


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.003 min
Response: 48112524
Conc: 21.21 ng/ml

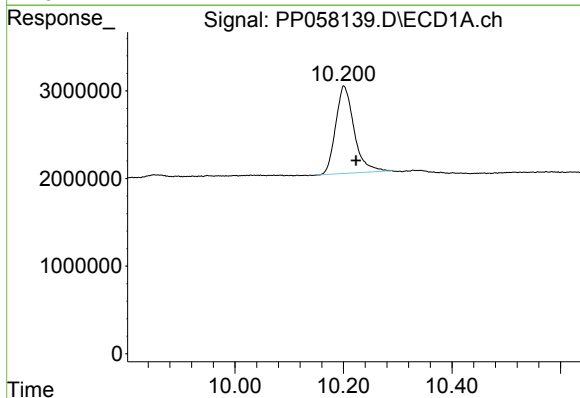

#2 Decachlorobiphenyl

R.T.: 10.201 min
Delta R.T.: -0.023 min
Response: 23506682
Conc: 20.74 ng/ml

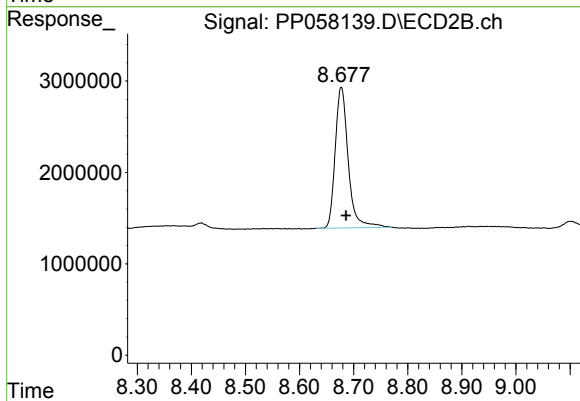

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.009 min
Response: 25767432
Conc: 16.42 ng/ml