

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060324\
 Data File : PP065433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 06:44
 Operator : YP\AJ
 Sample : P2687-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 72-11998

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/04/2024
 Supervised By :Ankita Jodhani 06/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 07:29:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 04 04:29:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.749	32830691	31120936	19.725	20.784
2) SA Decachlor...	10.207	8.810	32411626	29945281	19.651m	20.468

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060324\
Data File : PP065433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 06:44
Operator : YP\AJ
Sample : P2687-07
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
72-11998


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/04/2024
Supervised By :Ankita Jodhani 06/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:29:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 04 04:29:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

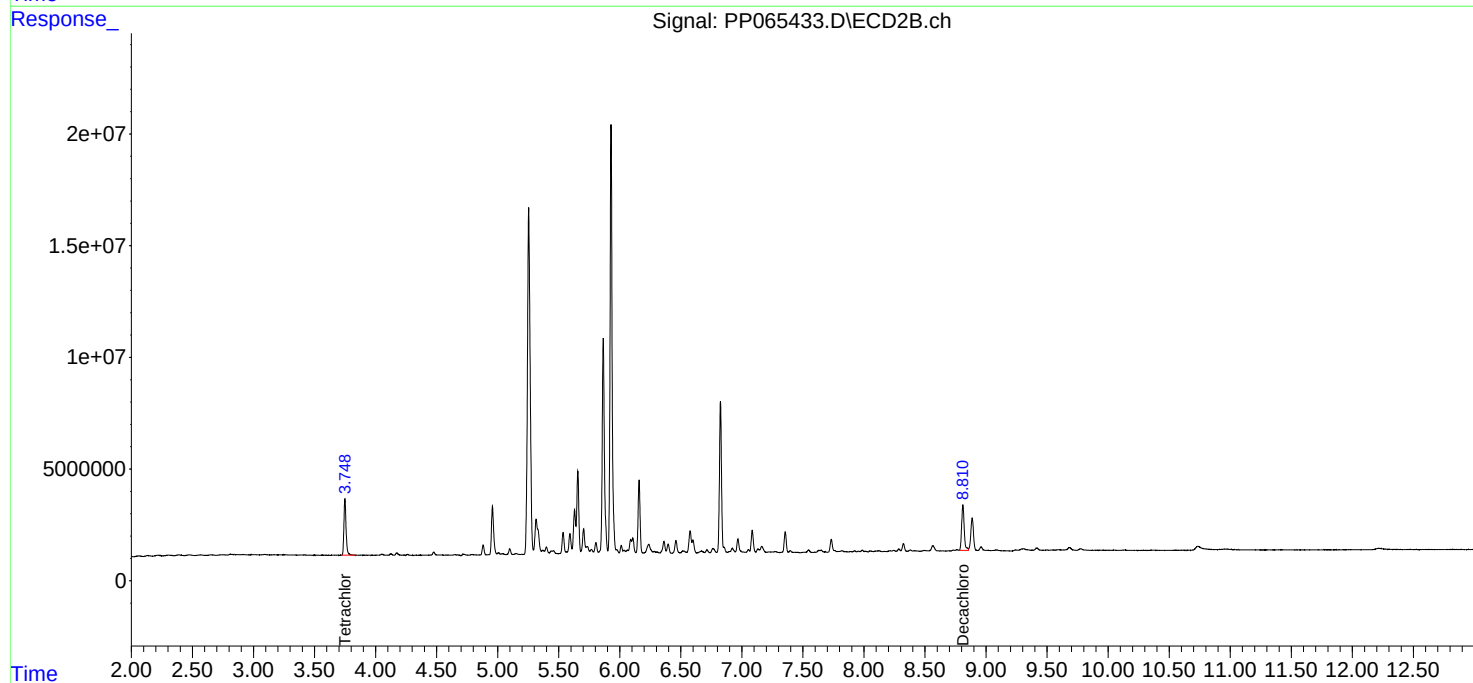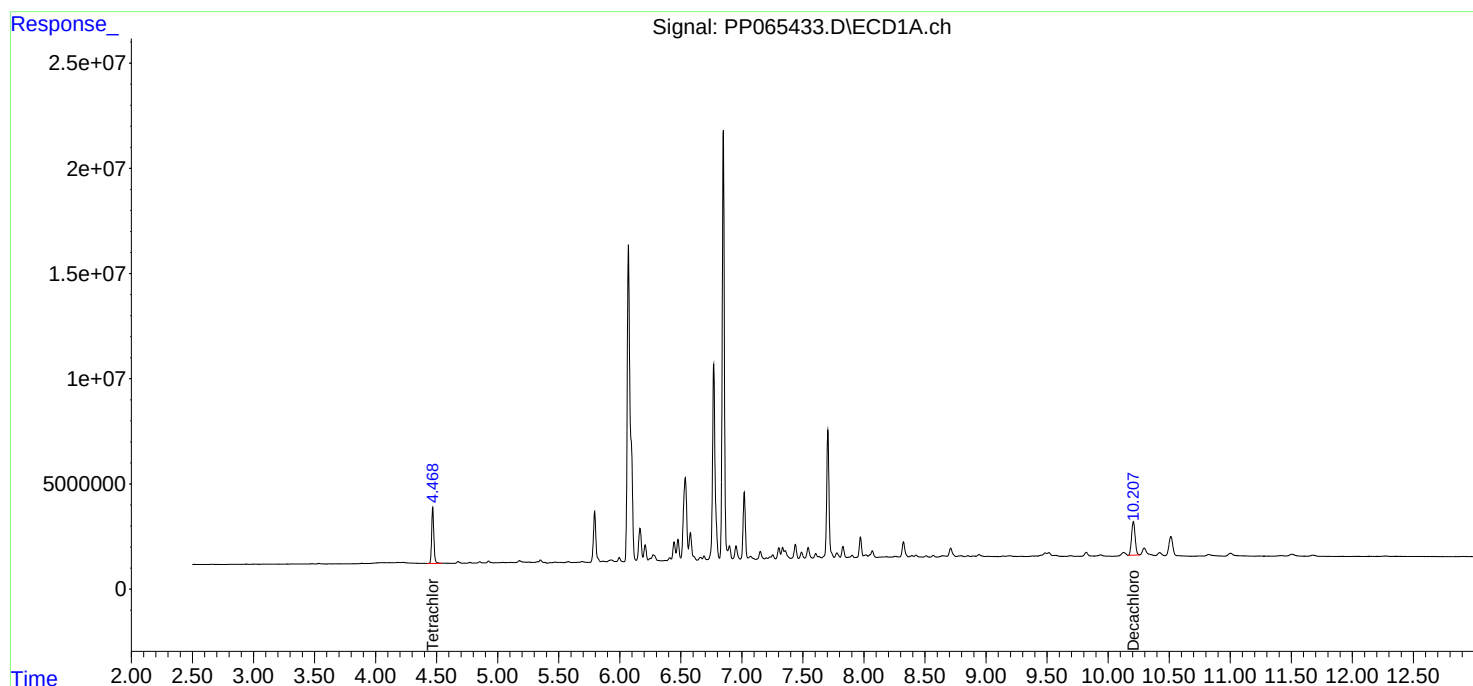

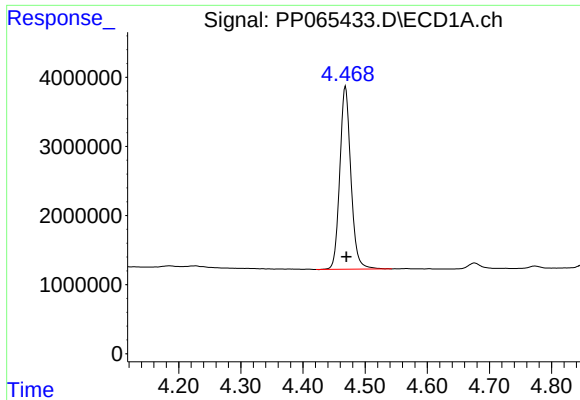


#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: -0.002 min
Response: 32830691
Conc: 19.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
72-11998


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/04/2024
Supervised By :Ankita Jodhani 06/04/2024

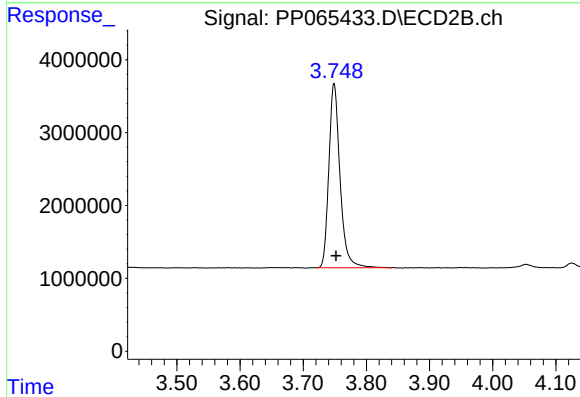


#1 Tetrachloro-m-xylene

R.T.: 3.749 min
Delta R.T.: -0.003 min
Response: 31120936
Conc: 20.78 ng/ml

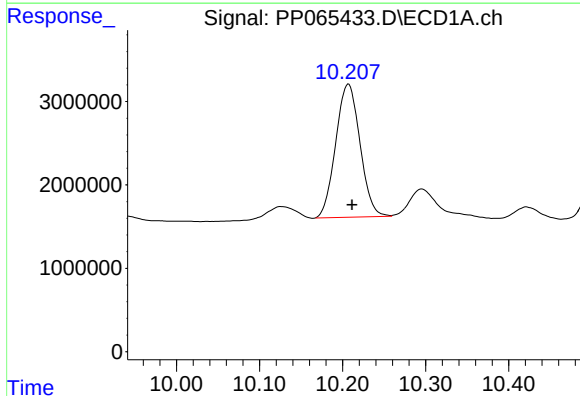

#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: -0.005 min
Response: 32411626
Conc: 19.65 ng/ml m

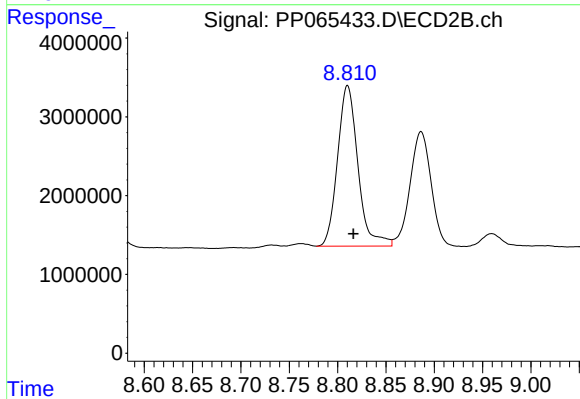

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: -0.006 min
Response: 29945281
Conc: 20.47 ng/ml