

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
 Data File : PP036220.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 10:20
 Operator : DD\AJ
 Sample : M2583-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 39-41S

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:57:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:07:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.962	788399	514413	17.713m	18.432m
2) SA Decachlor...	10.999	9.272	569867	336865	13.334	14.683m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
Data File : PP036220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 10:20
Operator : DD\AJ
Sample : M2583-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
39-41S


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:07:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

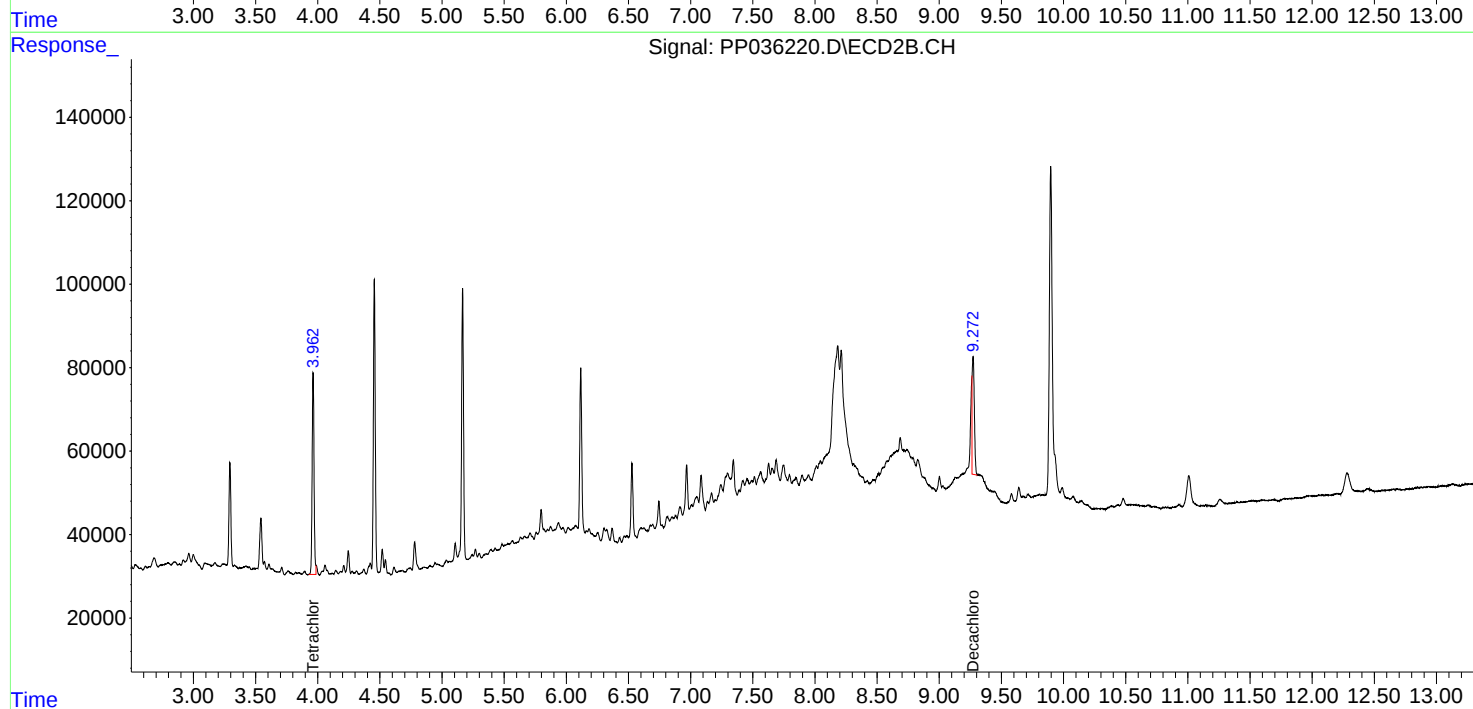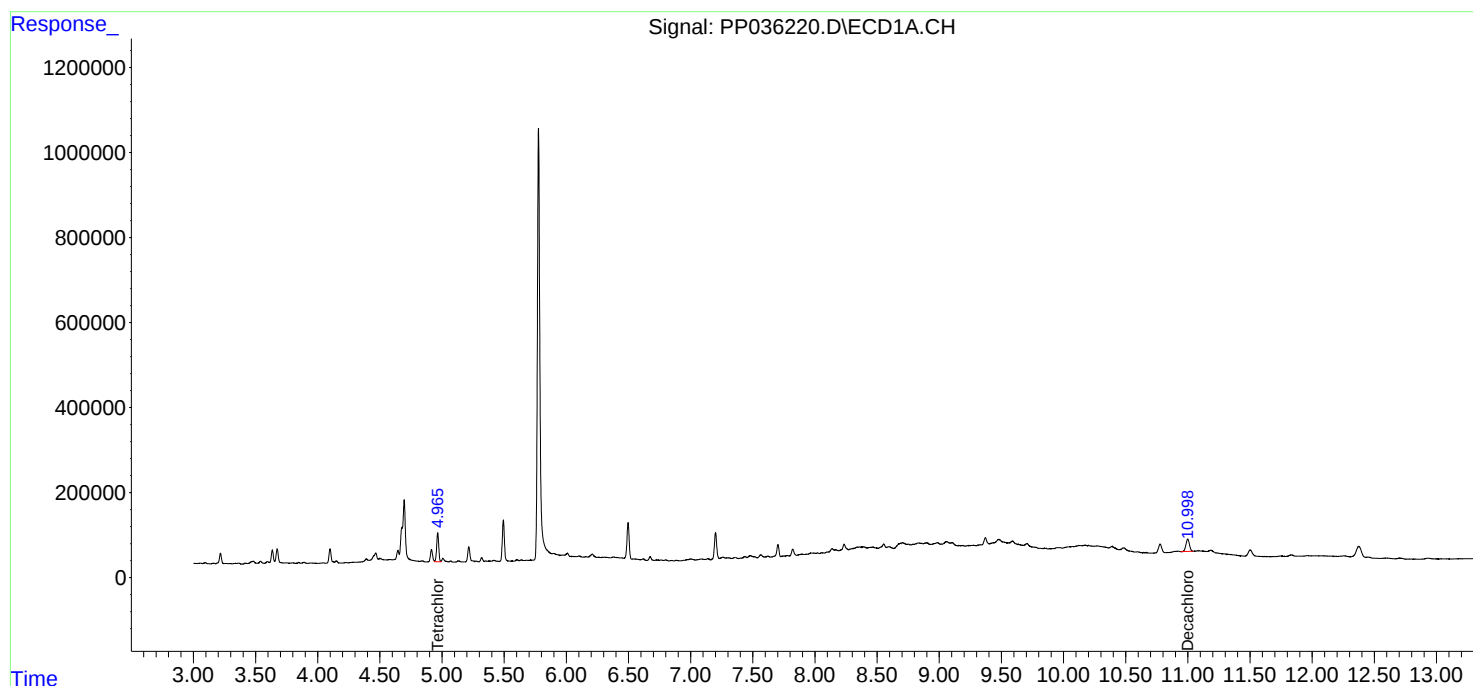

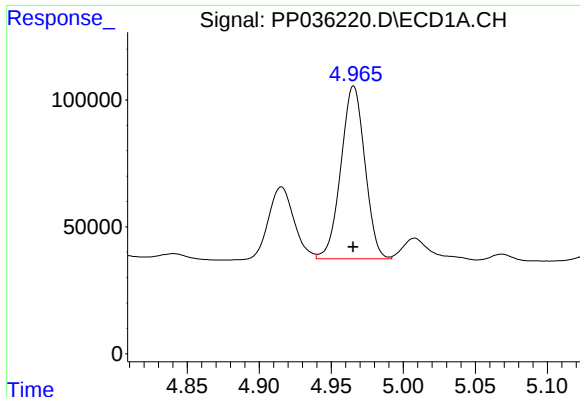


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 788399
Conc: 17.71 ng/ml m

Instrument :
ECD_P
ClientSampleId :
39-41S


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:38 AM

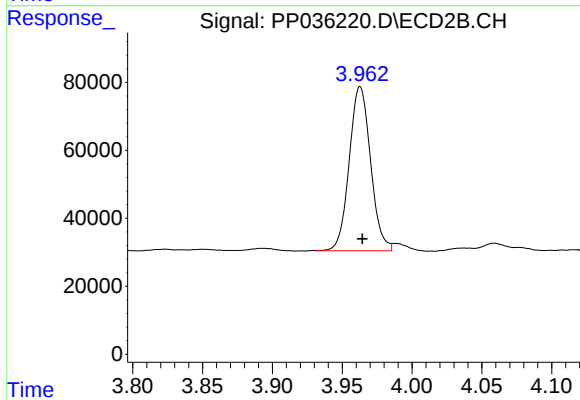


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.002 min
Response: 514413
Conc: 18.43 ng/ml m

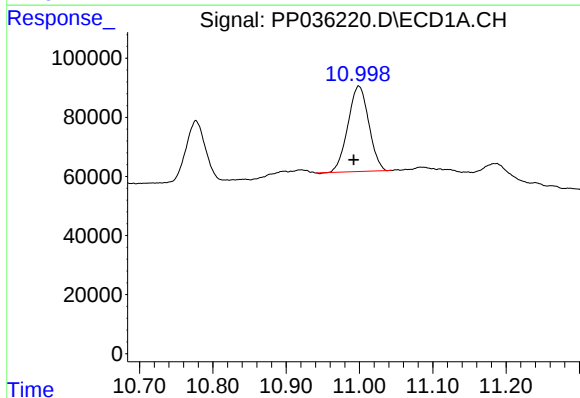

#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.007 min
Response: 569867
Conc: 13.33 ng/ml

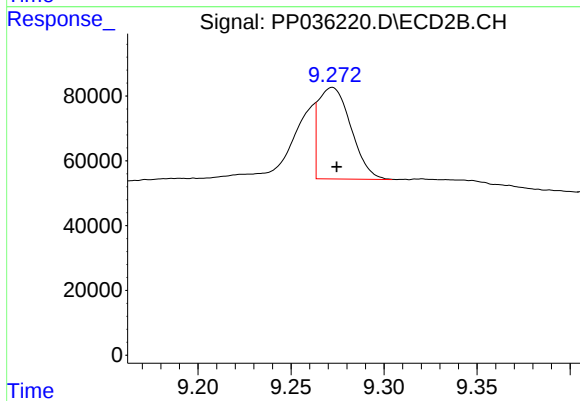

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: -0.003 min
Response: 336865
Conc: 14.68 ng/ml m