

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
 Data File : PP036224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 11:27
 Operator : DD\AJ
 Sample : M2583-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 30785

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:57:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:10:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.951	3.975	838110	829343	18.830m	29.716 #
2) SA Decachlor...	11.030f	9.306f	657273	369933	15.380m	16.125m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
Data File : PP036224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 11:27
Operator : DD\AJ
Sample : M2583-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
30785


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:10:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

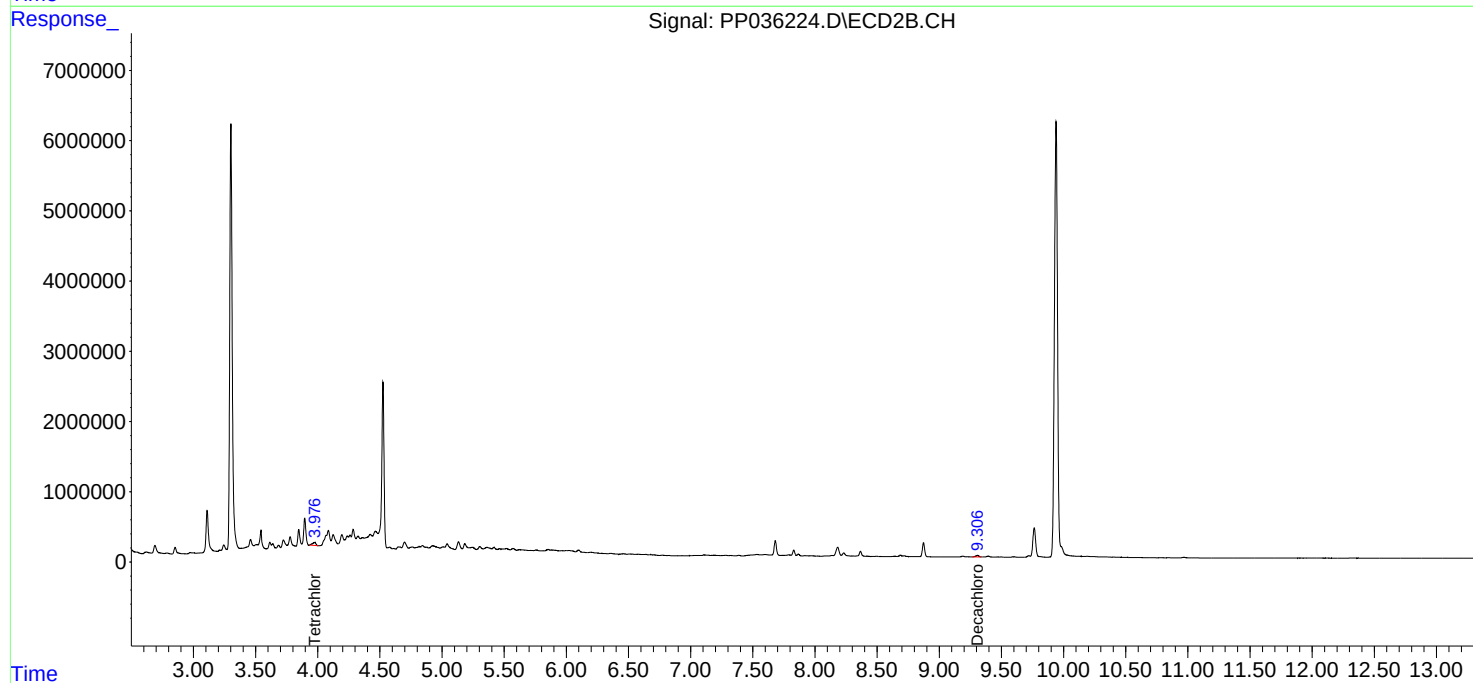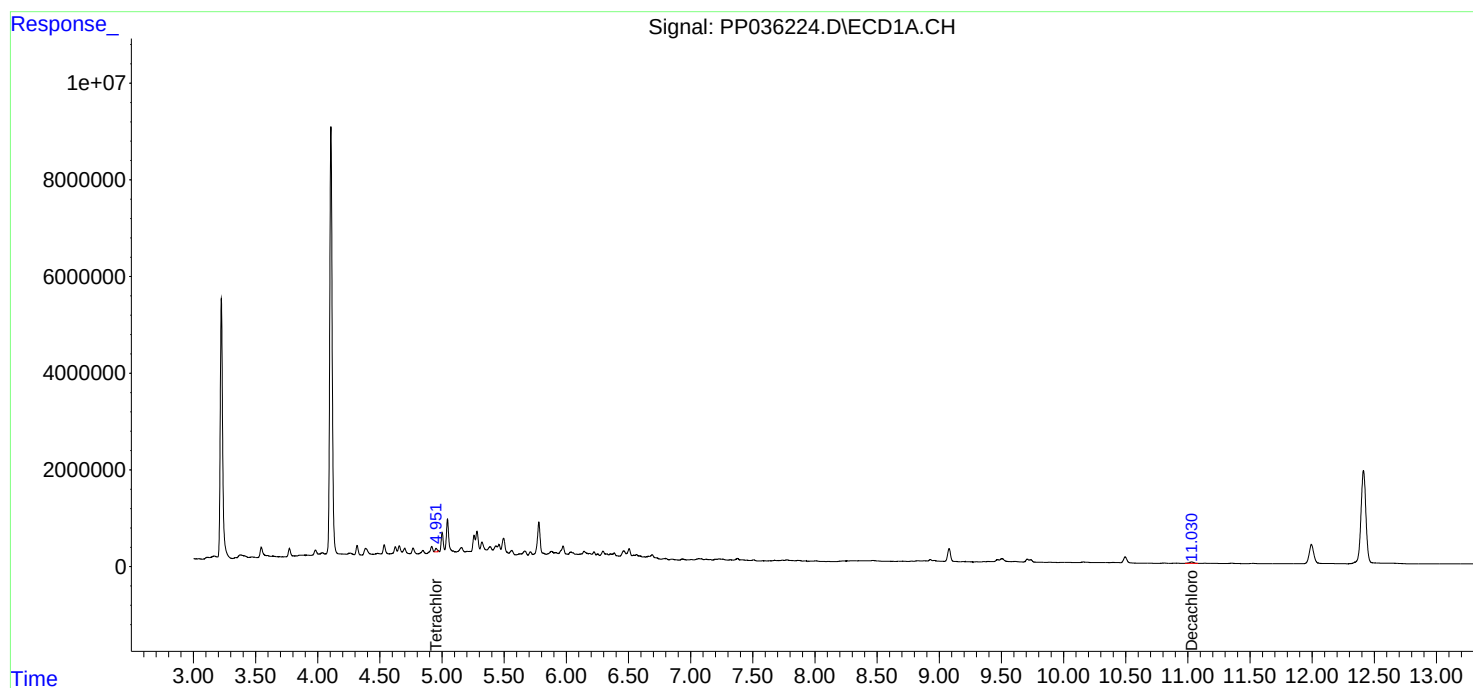

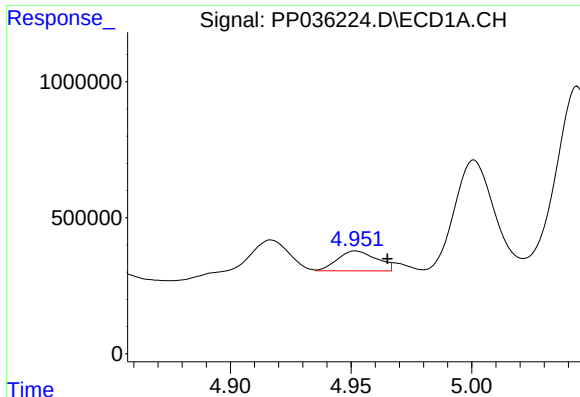


#1 Tetrachloro-m-xylene

R.T.: 4.951 min
Delta R.T.: -0.014 min
Response: 838110
Conc: 18.83 ng/ml m

Instrument :
ECD_P
ClientSampleId :
30785


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:43 AM

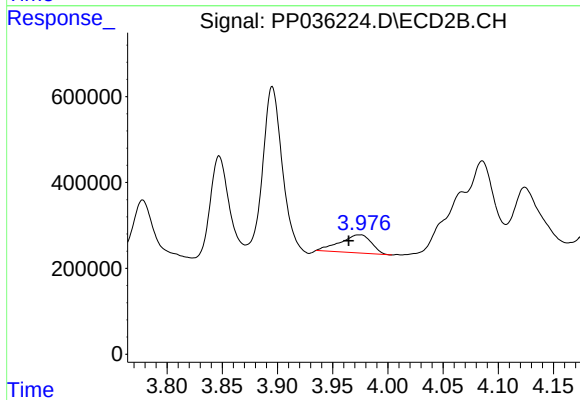


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: 0.010 min
Response: 829343
Conc: 29.72 ng/ml

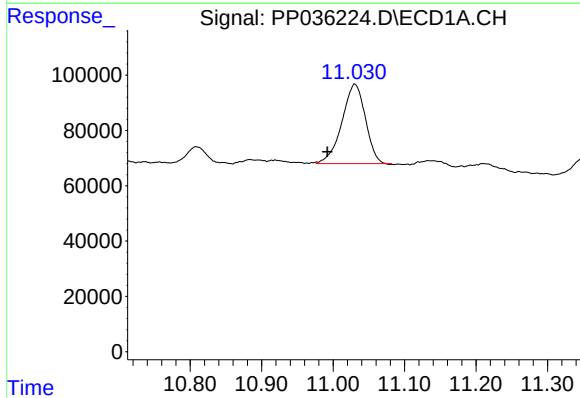

#2 Decachlorobiphenyl

R.T.: 11.030 min
Delta R.T.: 0.037 min
Response: 657273
Conc: 15.38 ng/ml m

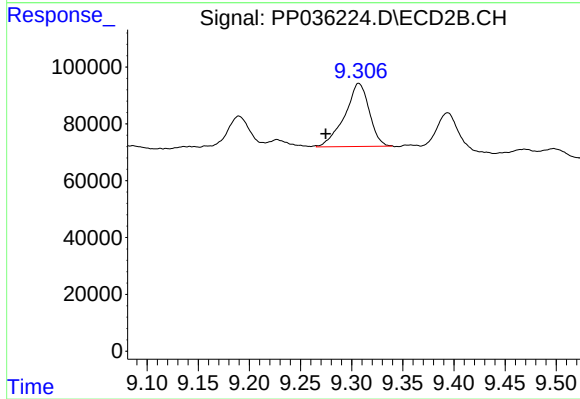

#2 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: 0.032 min
Response: 369933
Conc: 16.12 ng/ml m