

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
 Data File : PP036227.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 14:10
 Operator : DD\AJ
 Sample : M2599-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 339

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:57:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:11:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.970	3.964	1167255	780962	26.225	27.982
2) SA Decachlor...	11.004	9.273	1104042	617089	25.834m	26.898
Target Compounds						
31) L7 AR-1260-1	7.976	6.810	47518	29095	23.457m	23.319m
32) L7 AR-1260-2	8.240	7.007	117514	76332	48.103m	50.653m
33) L7 AR-1260-3	8.606	7.160	41914	48987	22.570m	34.856 #
34) L7 AR-1260-4	8.836	7.647	82497	31347	36.944m	26.812m#
35) L7 AR-1260-5	9.167	7.895	98957	51852	23.176m	18.731m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
Data File : PP036227.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 14:10
Operator : DD\AJ
Sample : M2599-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
339


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:11:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

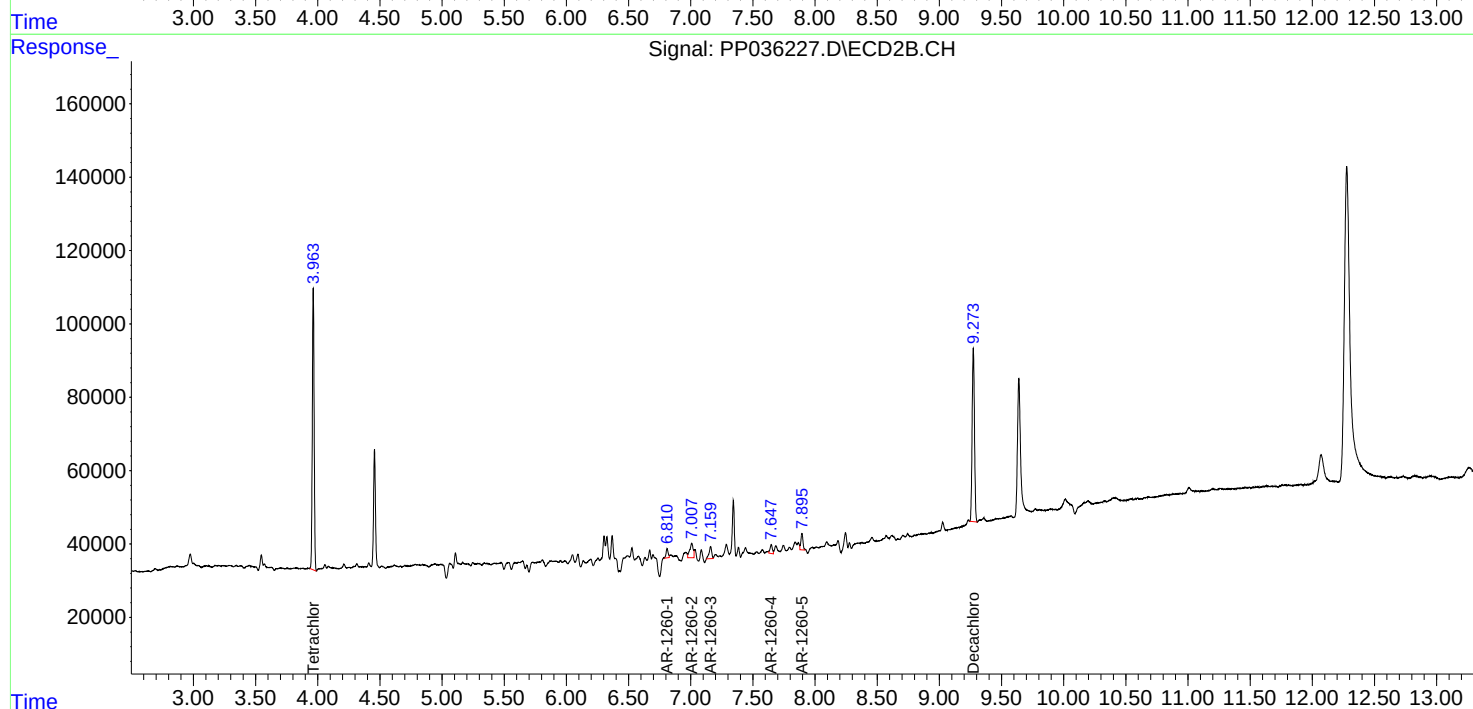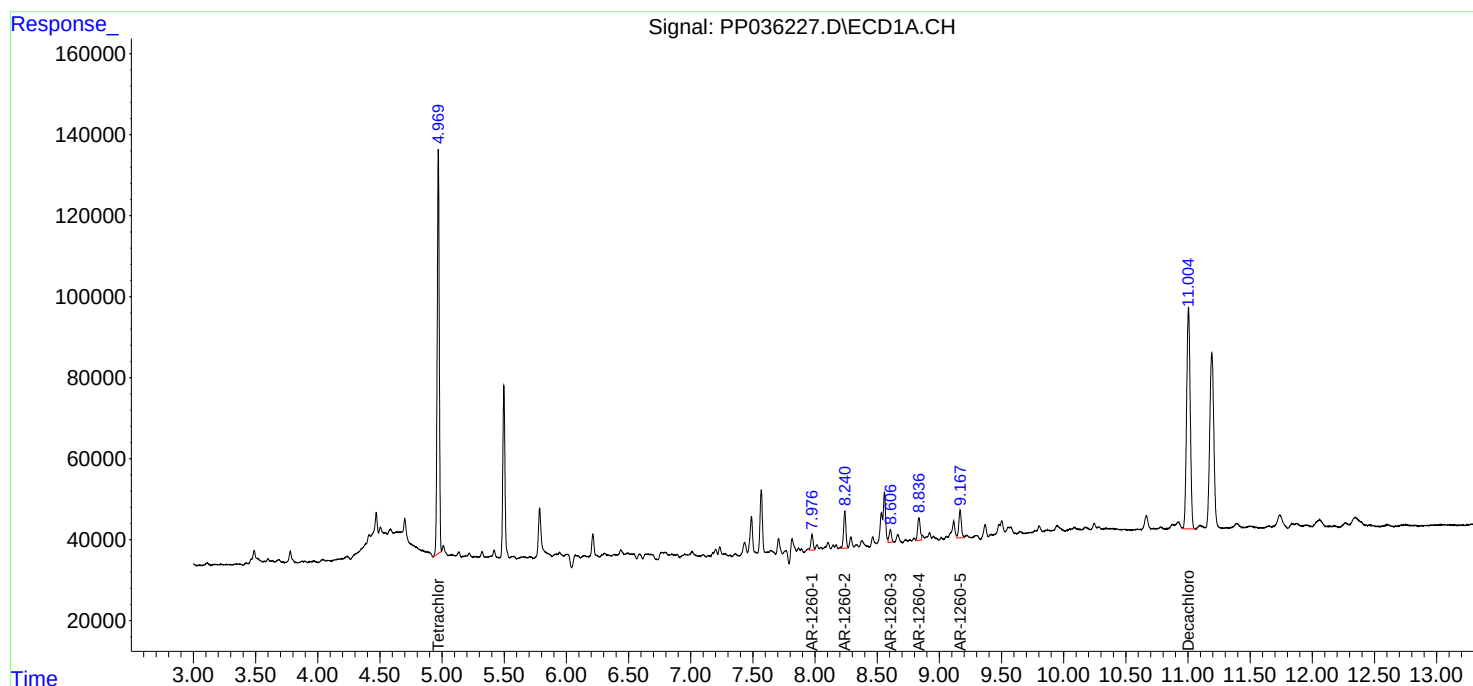

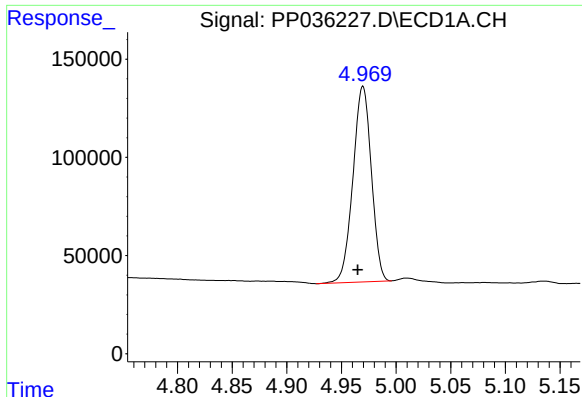


#1 Tetrachloro-m-xylene

R.T.: 4.970 min
Delta R.T.: 0.005 min
Response: 1167255
Conc: 26.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
339


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:46 AM

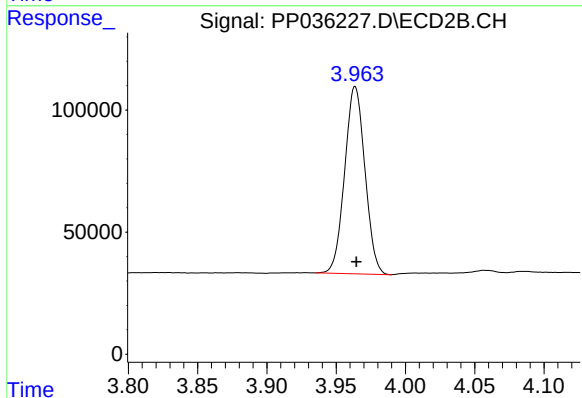


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 780962
Conc: 27.98 ng/ml

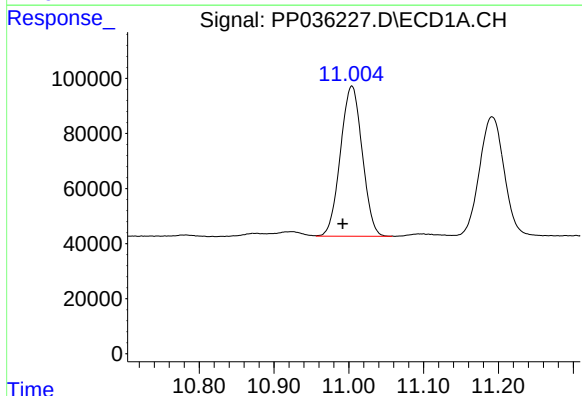


#2 Decachlorobiphenyl

R.T.: 11.004 min
Delta R.T.: 0.011 min
Response: 1104042
Conc: 25.83 ng/ml m

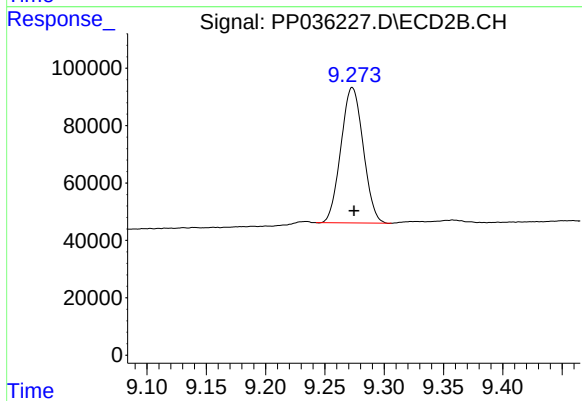

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.001 min
Response: 617089
Conc: 26.90 ng/ml

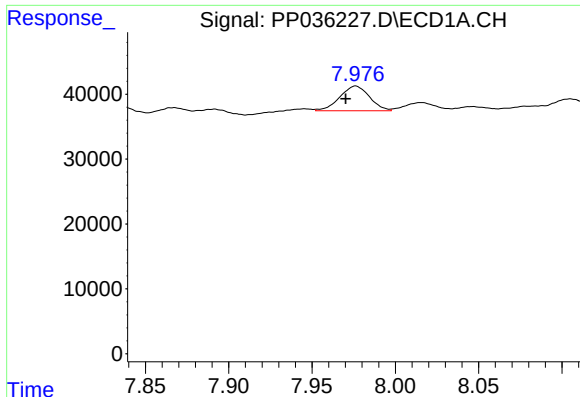


#31 AR-1260-1

R.T.: 7.976 min
Delta R.T.: 0.005 min
Response: 47518
Conc: 23.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
339


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:46 AM

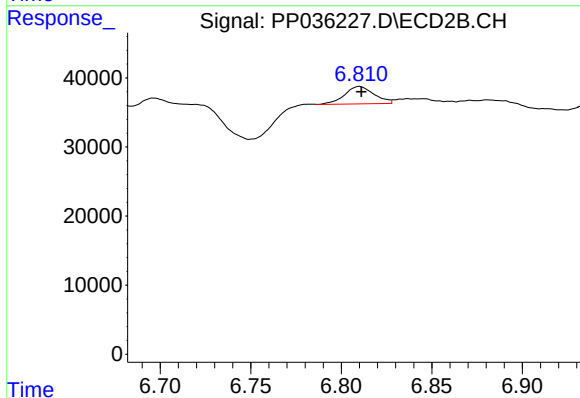


#31 AR-1260-1

R.T.: 6.810 min
Delta R.T.: -0.002 min
Response: 29095
Conc: 23.32 ng/ml m

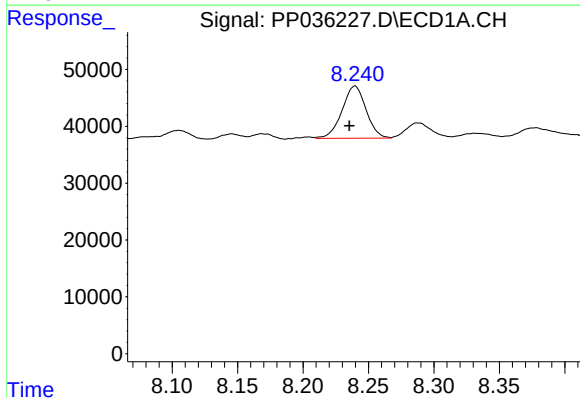


#32 AR-1260-2

R.T.: 8.240 min
Delta R.T.: 0.004 min
Response: 117514
Conc: 48.10 ng/ml m

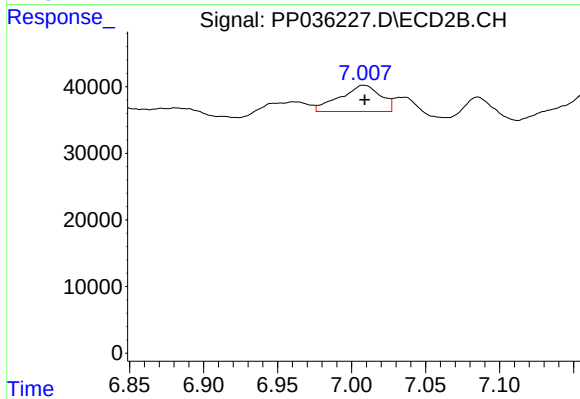

#32 AR-1260-2

R.T.: 7.007 min
Delta R.T.: -0.002 min
Response: 76332
Conc: 50.65 ng/ml m

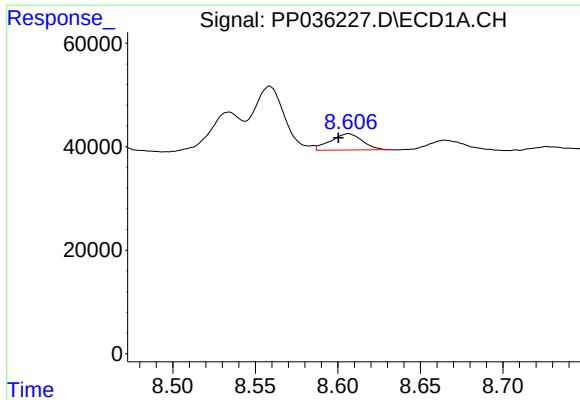


#33 AR-1260-3

R.T.: 8.606 min
Delta R.T.: 0.006 min
Response: 41914
Conc: 22.57 ng/ml m

Instrument :
ECD_P
ClientSampleId :
339


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:46 AM

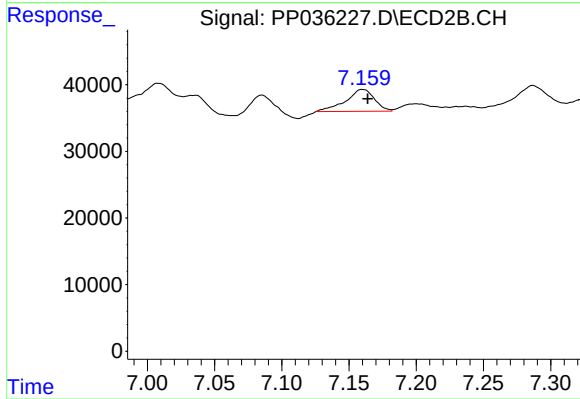


#33 AR-1260-3

R.T.: 7.160 min
Delta R.T.: -0.004 min
Response: 48987
Conc: 34.86 ng/ml

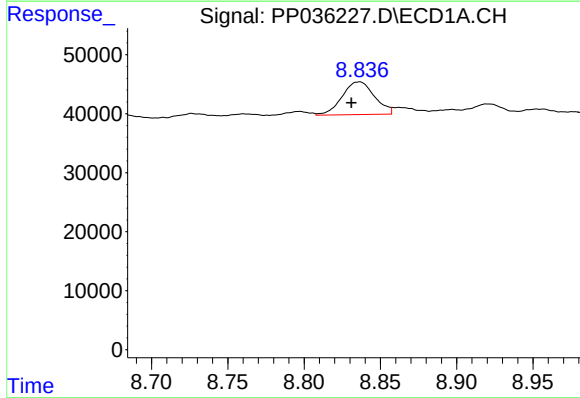


#34 AR-1260-4

R.T.: 8.836 min
Delta R.T.: 0.005 min
Response: 82497
Conc: 36.94 ng/ml m

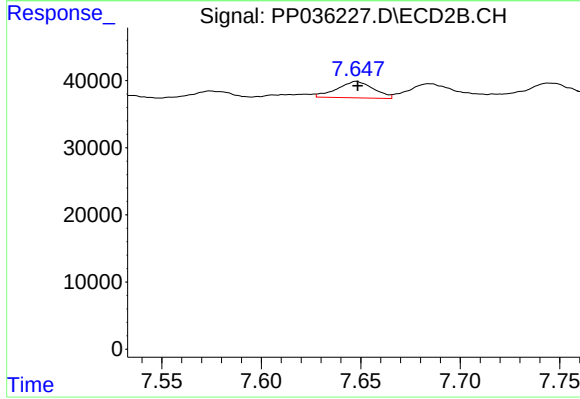

#34 AR-1260-4

R.T.: 7.647 min
Delta R.T.: -0.001 min
Response: 31347
Conc: 26.81 ng/ml m

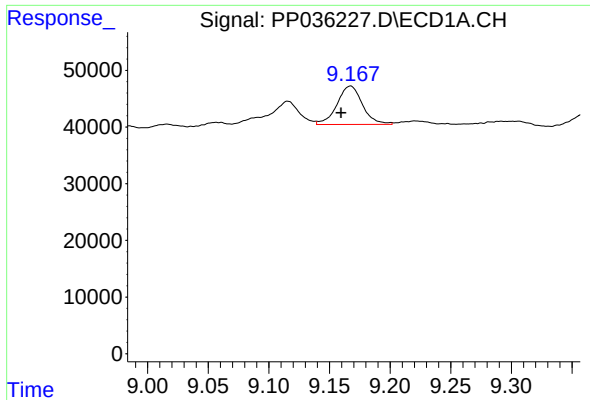


#35 AR-1260-5

R.T.: 9.167 min
Delta R.T.: 0.008 min
Response: 98957
Conc: 23.18 ng/ml m

Instrument :
ECD_P
ClientSampleId :
339

Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:46 AM

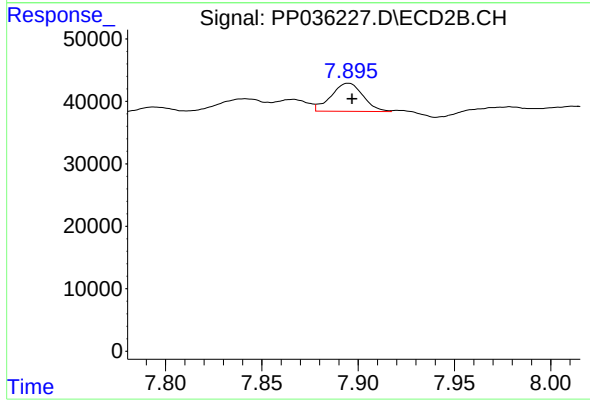

#35 AR-1260-5

R.T.: 7.895 min
Delta R.T.: -0.002 min
Response: 51852
Conc: 18.73 ng/ml m