

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
 Data File : PP036232.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 15:34
 Operator : DD\AJ
 Sample : M2601-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-VNJ-212

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:57:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:14:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.967	3.963	737347	450789	16.566	16.152
2) SA Decachlor...	11.001	9.272	924948	506774	21.643m	22.090
Target Compounds						
31) L7 AR-1260-1	7.974	6.810	266175	164803	131.398	132.086
32) L7 AR-1260-2	8.239	7.007	494372	271099	202.365	179.899
33) L7 AR-1260-3	8.605	7.162	421247	185601	226.837	132.061 #
34) L7 AR-1260-4	8.832	7.647	626755	196033	280.672	167.675 #
35) L7 AR-1260-5	9.165	7.894	699780	449414	163.893	162.351

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060421\
Data File : PP036232.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 15:34
Operator : DD\AJ
Sample : M2601-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

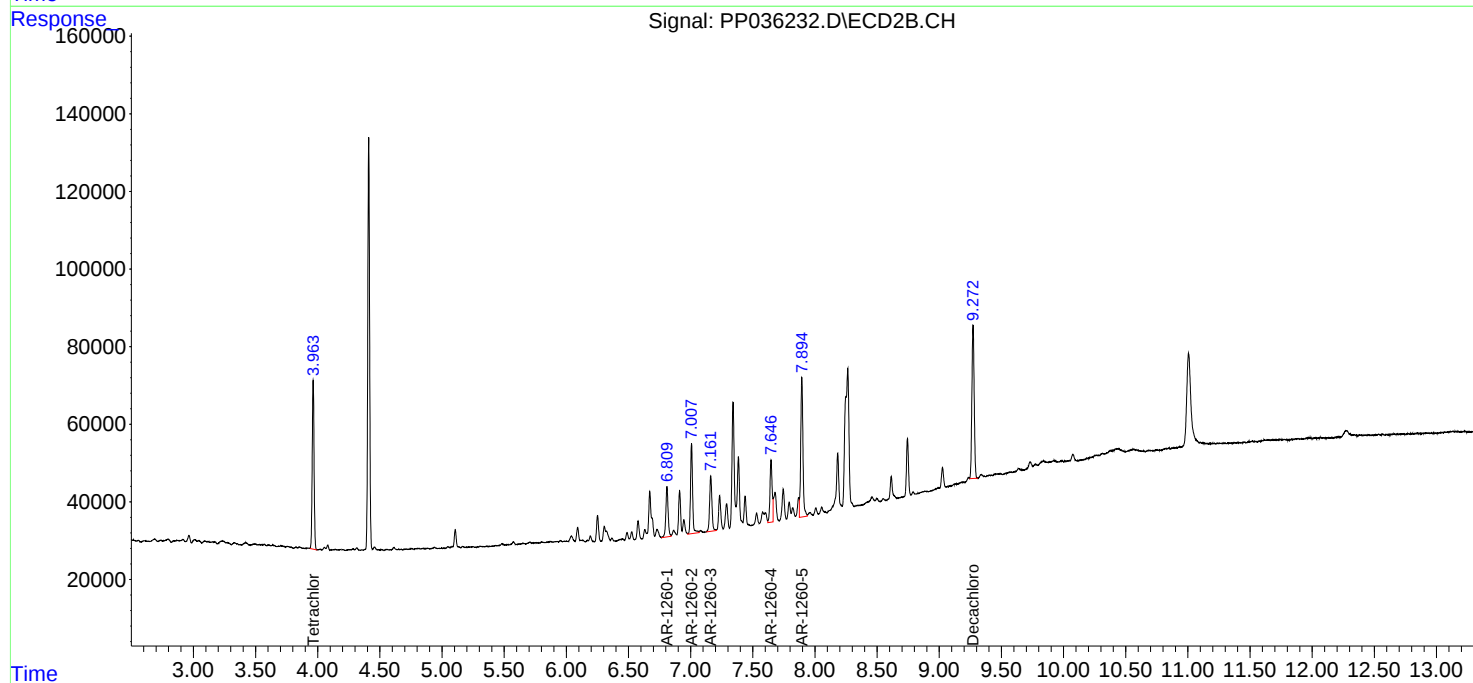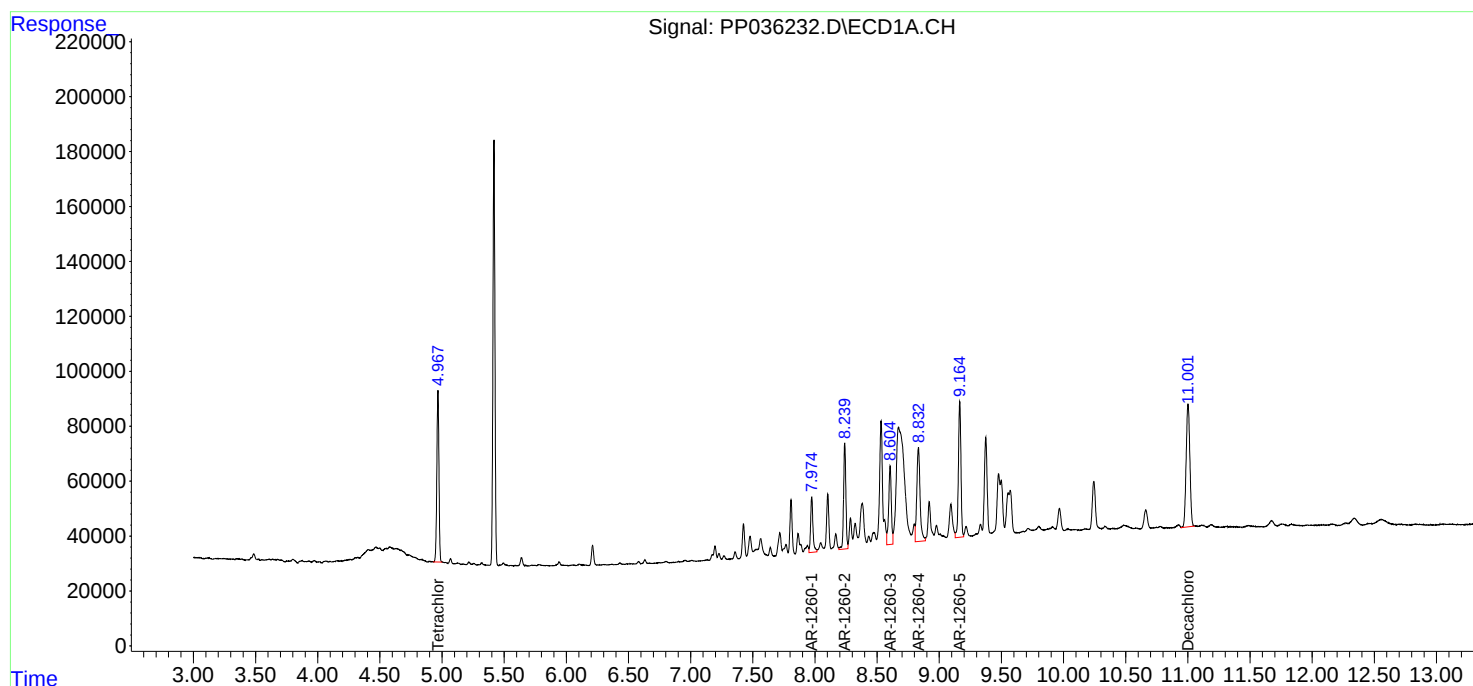

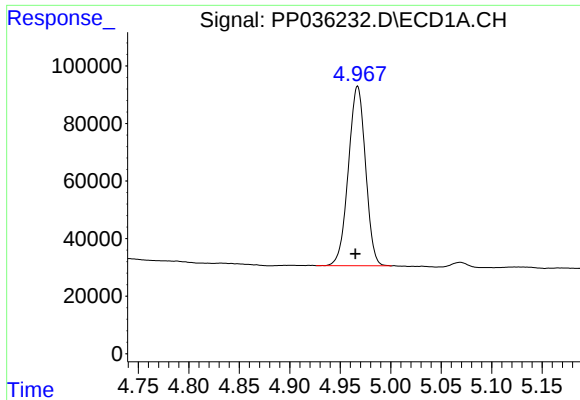


#1 Tetrachloro-m-xylene

R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 737347
Conc: 16.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:47 AM

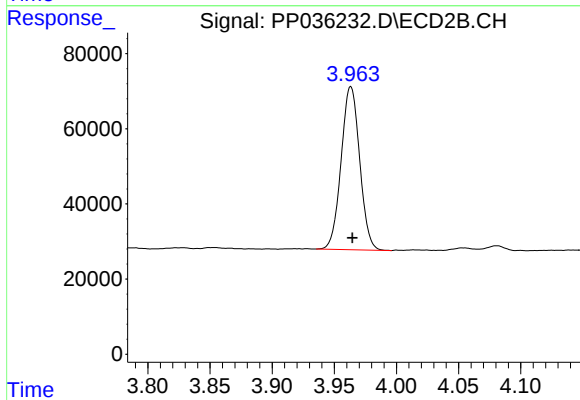


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.001 min
Response: 450789
Conc: 16.15 ng/ml

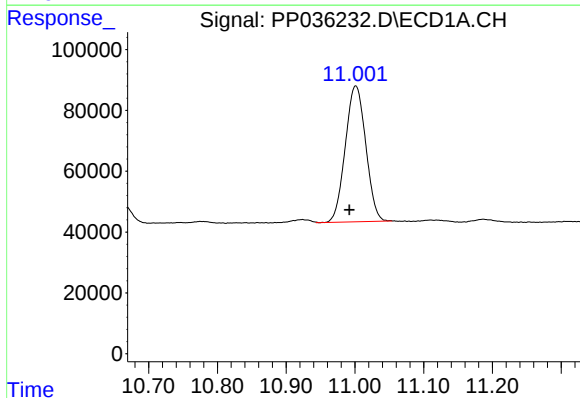


#2 Decachlorobiphenyl

R.T.: 11.001 min
Delta R.T.: 0.009 min
Response: 924948
Conc: 21.64 ng/ml m

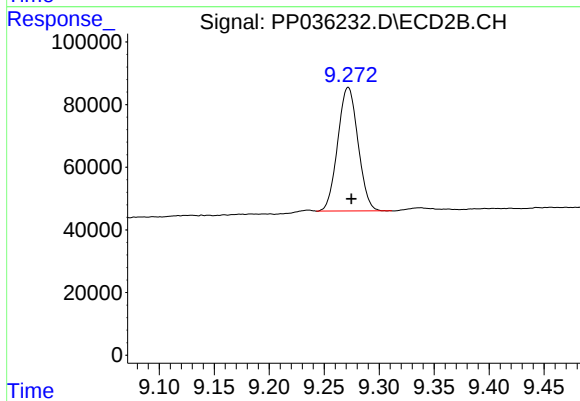

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: -0.003 min
Response: 506774
Conc: 22.09 ng/ml

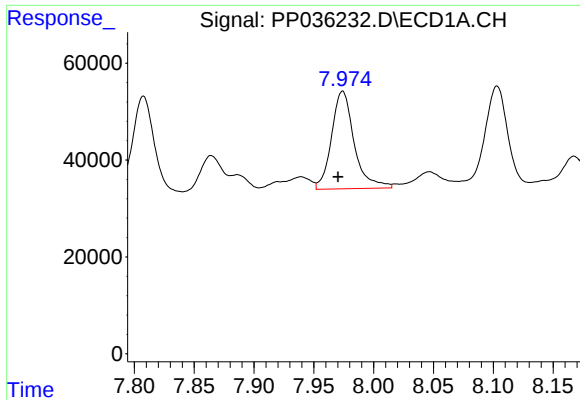


#31 AR-1260-1

R.T.: 7.974 min
Delta R.T.: 0.004 min
Response: 266175
Conc: 131.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:47 AM

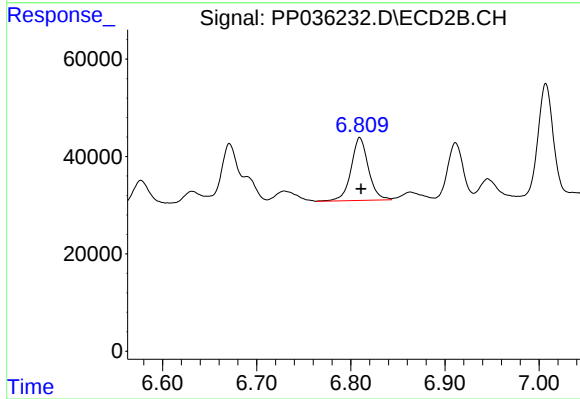


#31 AR-1260-1

R.T.: 6.810 min
Delta R.T.: -0.002 min
Response: 164803
Conc: 132.09 ng/ml

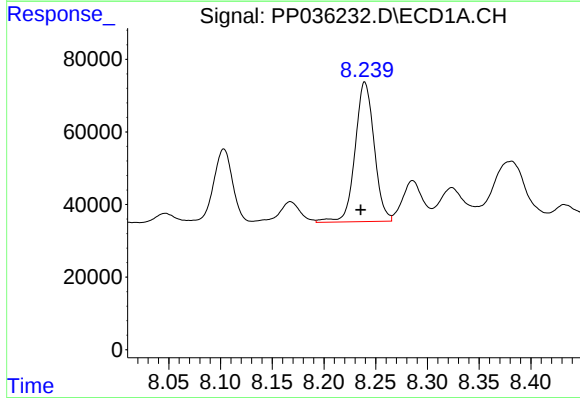


#32 AR-1260-2

R.T.: 8.239 min
Delta R.T.: 0.004 min
Response: 494372
Conc: 202.37 ng/ml

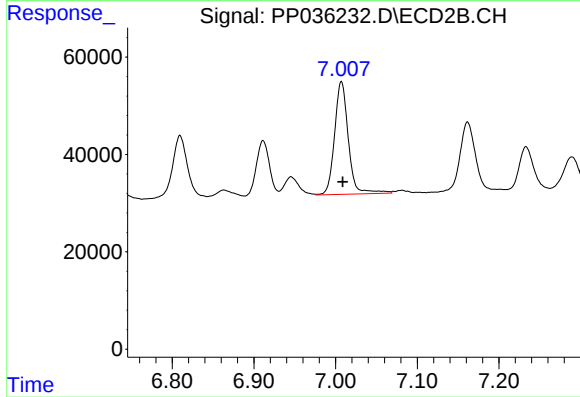

#32 AR-1260-2

R.T.: 7.007 min
Delta R.T.: -0.002 min
Response: 271099
Conc: 179.90 ng/ml

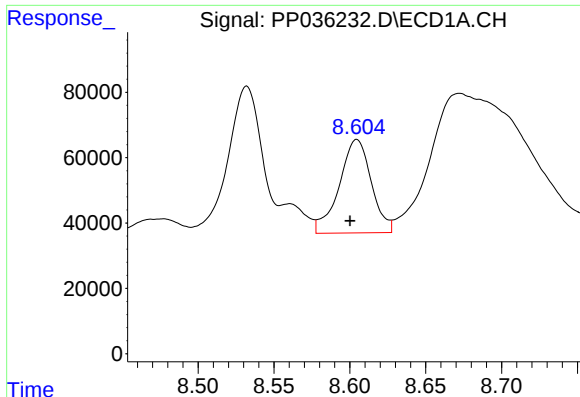


#33 AR-1260-3

R.T.: 8.605 min
Delta R.T.: 0.004 min
Response: 421247
Conc: 226.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:47 AM

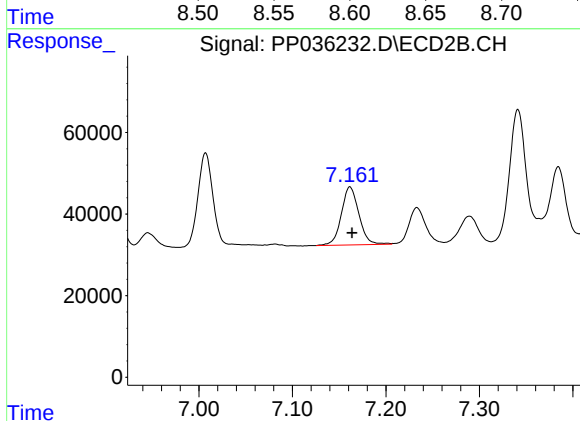


#33 AR-1260-3

R.T.: 7.162 min
Delta R.T.: -0.002 min
Response: 185601
Conc: 132.06 ng/ml

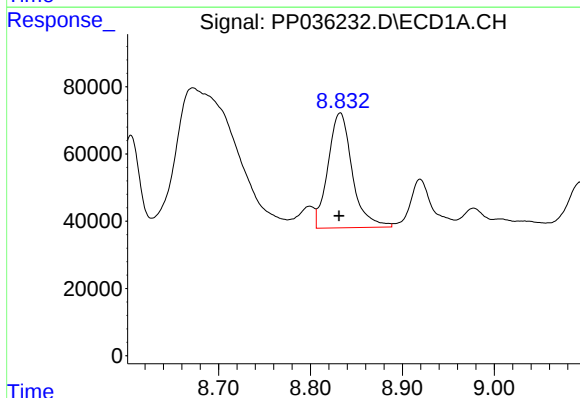


#34 AR-1260-4

R.T.: 8.832 min
Delta R.T.: 0.001 min
Response: 626755
Conc: 280.67 ng/ml

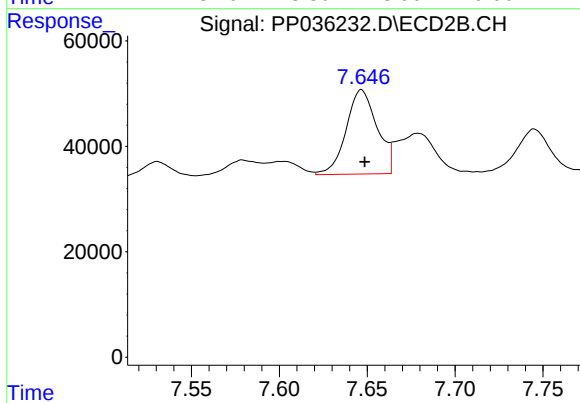

#34 AR-1260-4

R.T.: 7.647 min
Delta R.T.: -0.002 min
Response: 196033
Conc: 167.68 ng/ml

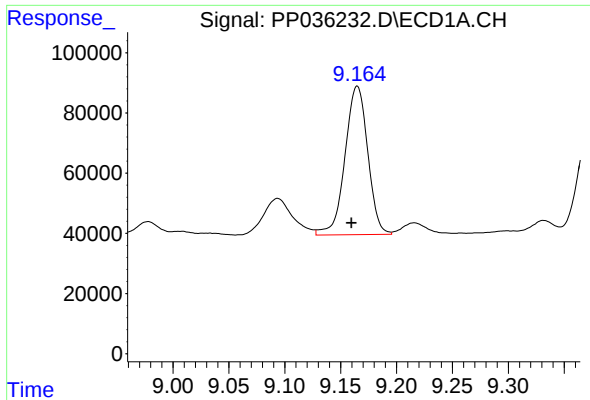


#35 AR-1260-5

R.T.: 9.165 min
Delta R.T.: 0.005 min
Response: 699780
Conc: 163.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-VNJ-212

Manual Integrations
APPROVED

Ankita
6/8/2021 11:57:47 AM

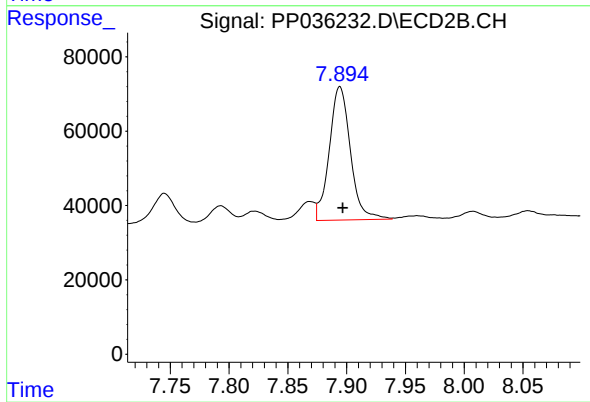

#35 AR-1260-5

R.T.: 7.894 min
Delta R.T.: -0.003 min
Response: 449414
Conc: 162.35 ng/ml