

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060424\
 Data File : PP065448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 11:11
 Operator : YP\AJ
 Sample : P2700-12 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271315-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 12:36:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 04 04:29:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.468	3.748	2493155	2409868	1.498	1.609
2)	SA Decachlor...	10.209	8.810	3666330	2530563	2.223	1.730
Target Compounds							
26)	L6 AR-1254-1	6.485	0.000	172175	0	2.486	N.D. #
30)	L6 AR-1254-5	7.750f	0.000	74245	0	0.837	N.D. #
32)	L7 AR-1260-2	7.490	0.000	67090	0	0.663	N.D. #
33)	L7 AR-1260-3	7.861	0.000	54297	0	0.679	N.D. #
34)	L7 AR-1260-4	8.076	0.000	187525	0	2.120	N.D. #
35)	L7 AR-1260-5	8.377f	0.000	29118	0	0.179	N.D. #
36)	L8 AR-1262-1	7.904	0.000	120898	0	2.499	N.D. #
37)	L8 AR-1262-2	8.377f	0.000	29118	0	0.155	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060424\
Data File : PP065448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 11:11
Operator : YP\AJ
Sample : P2700-12 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 12:36:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 04 04:29:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

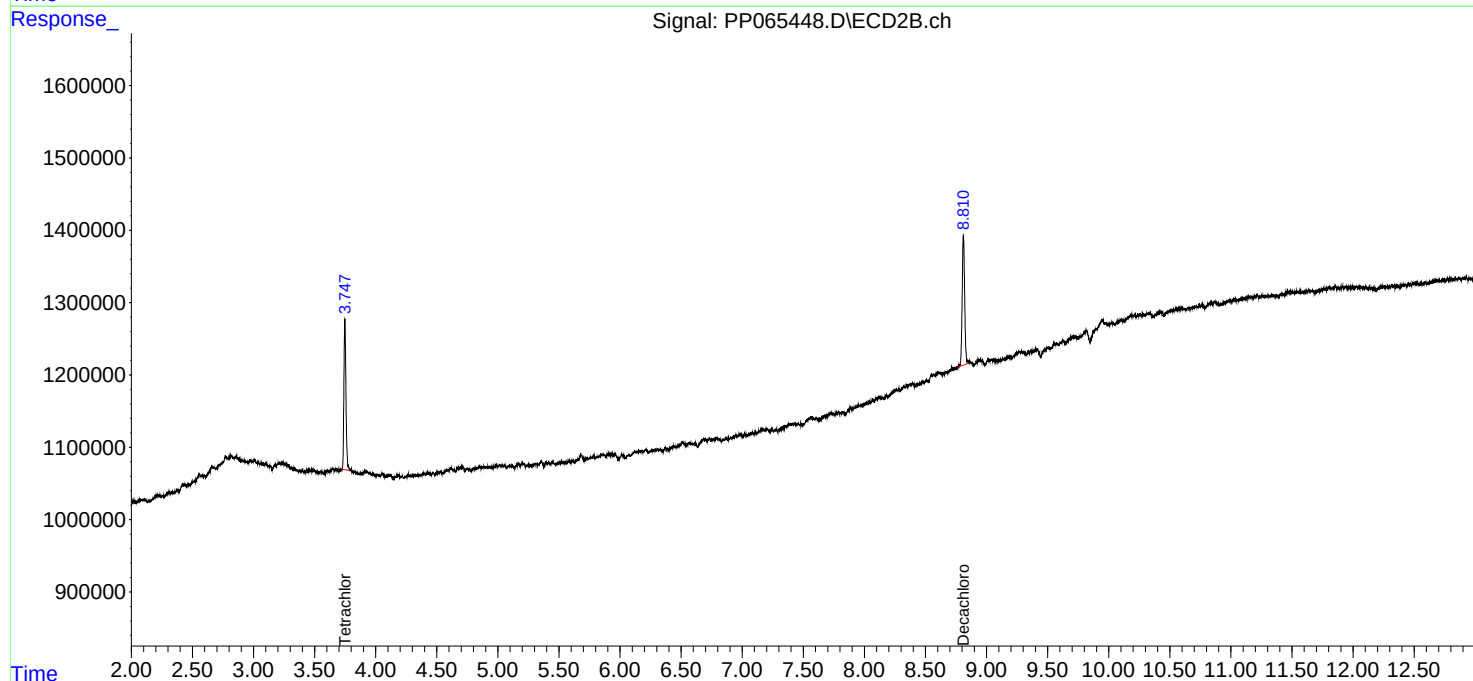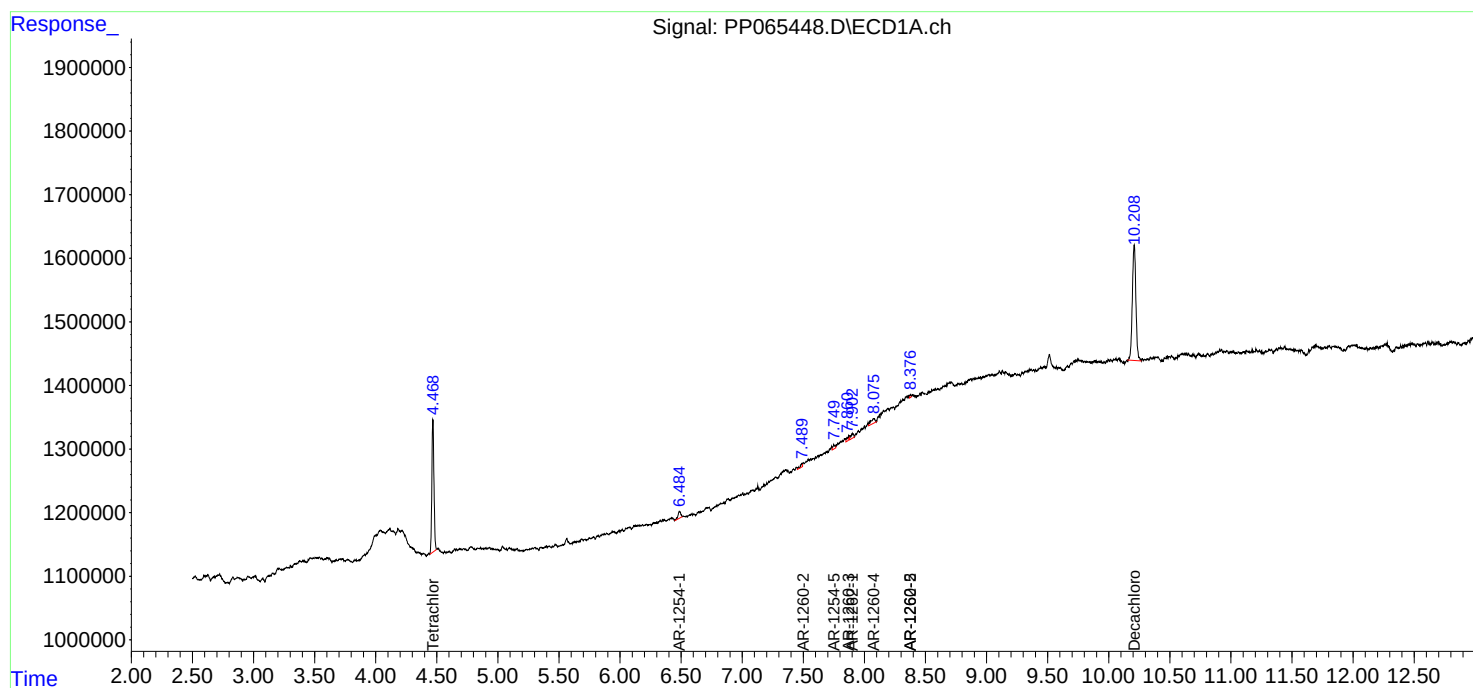


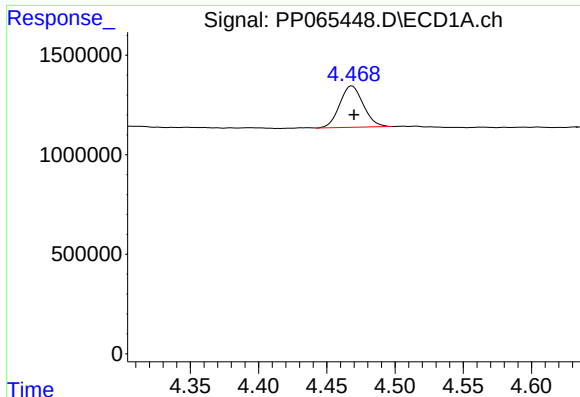

#1 Tetrachloro-m-xylene


R.T.: 4.468 min
Delta R.T.: -0.002 min
Response: 2493155
Conc: 1.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

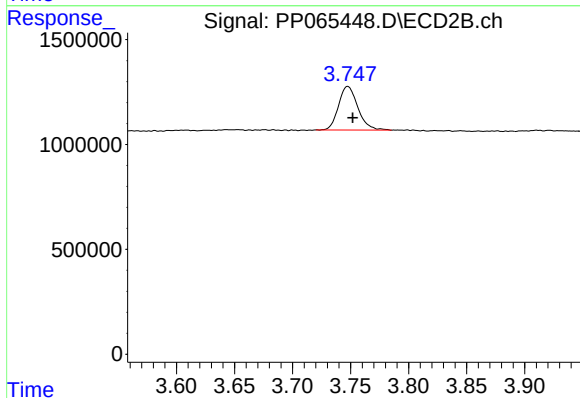


#1 Tetrachloro-m-xylene

R.T.: 3.748 min
Delta R.T.: -0.004 min
Response: 2409868
Conc: 1.61 ng/ml

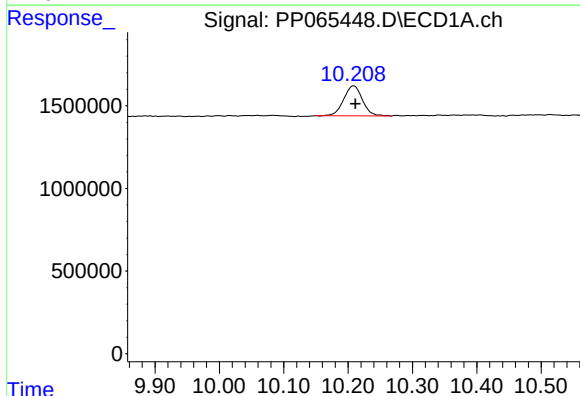


#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.002 min
Response: 3666330
Conc: 2.22 ng/ml

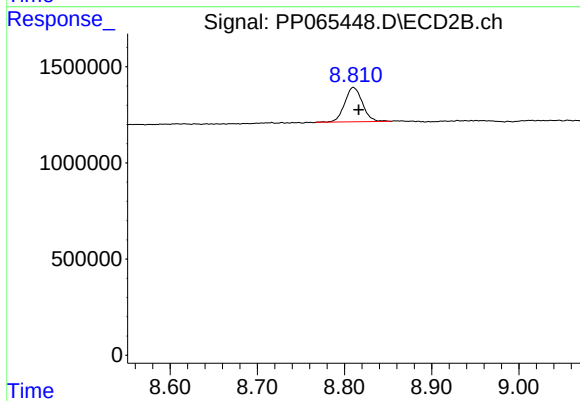

#2 Decachlorobiphenyl


R.T.: 8.810 min
Delta R.T.: -0.006 min
Response: 2530563
Conc: 1.73 ng/ml

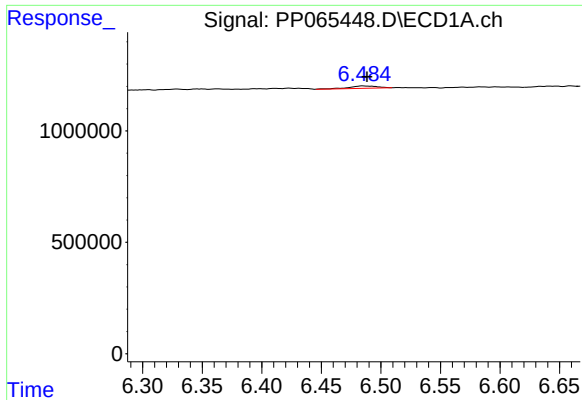

#26 AR-1254-1


R.T.: 6.485 min
Delta R.T.: -0.003 min
Response: 172175
Conc: 2.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

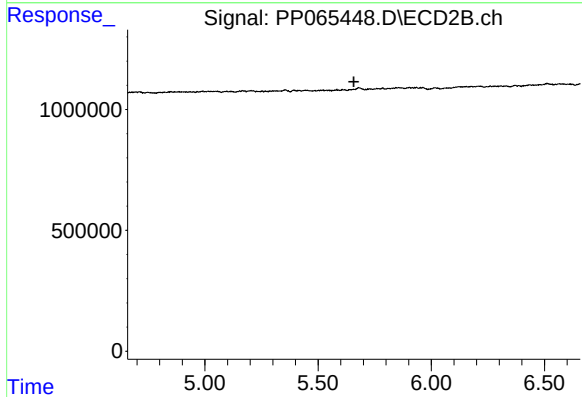


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

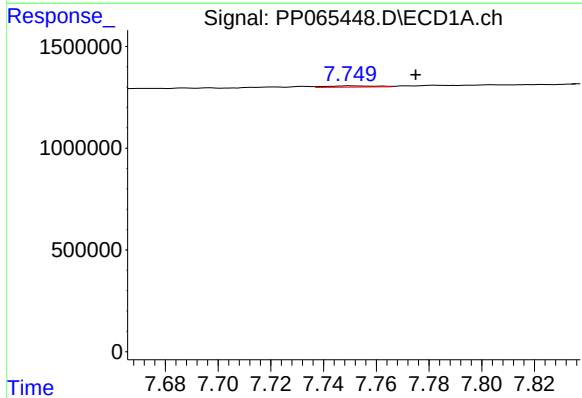


#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: -0.025 min
Response: 74245
Conc: 0.84 ng/ml

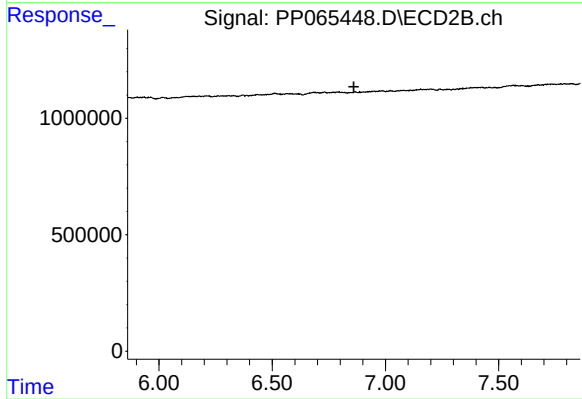

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

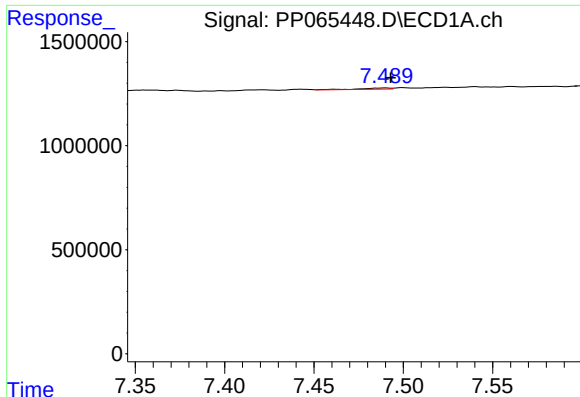

#32 AR-1260-2


R.T.: 7.490 min
Delta R.T.: -0.003 min
Response: 67090
Conc: 0.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

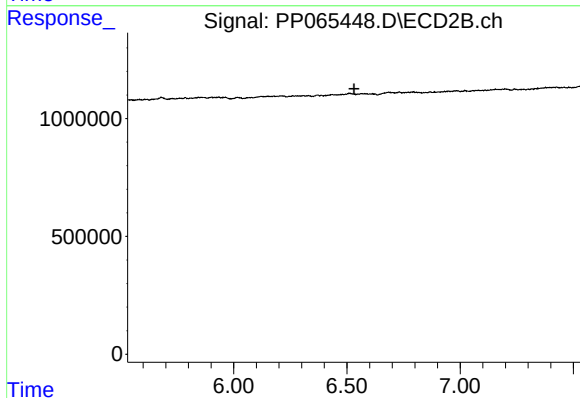


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.531 min
Response: 0
Conc: N.D.

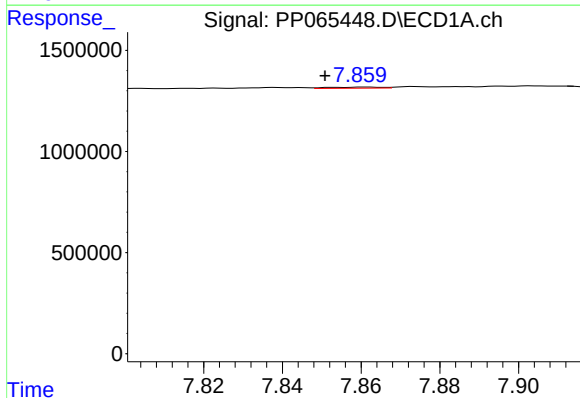


#33 AR-1260-3

R.T.: 7.861 min
Delta R.T.: 0.011 min
Response: 54297
Conc: 0.68 ng/ml

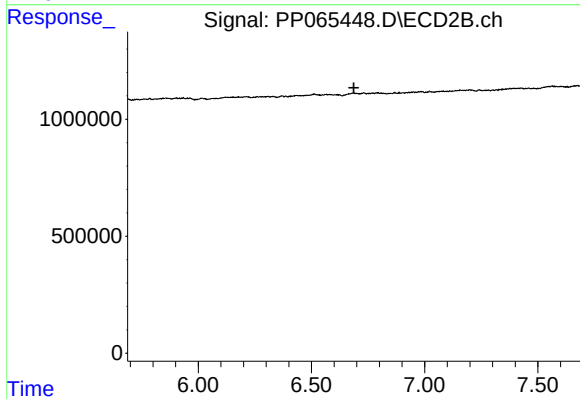

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.688 min
Response: 0
Conc: N.D.

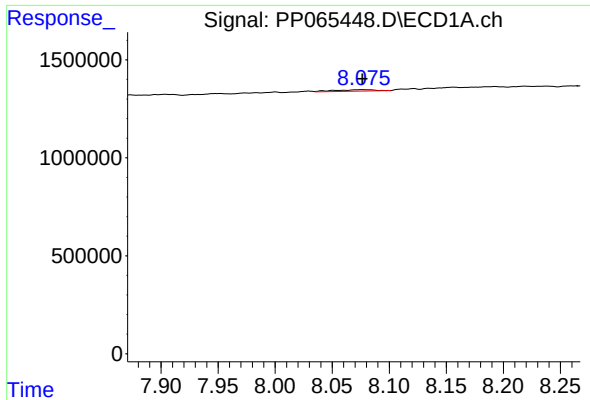

#34 AR-1260-4


R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 187525
Conc: 2.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

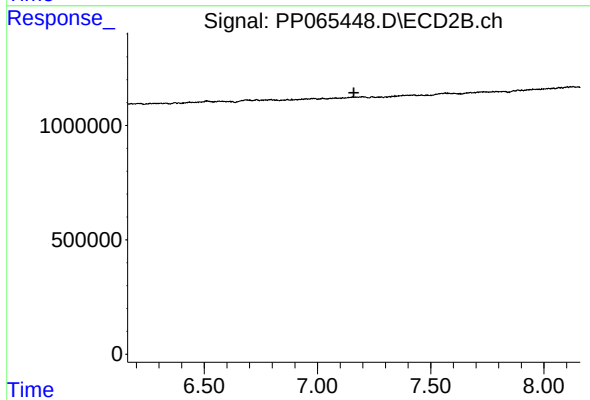


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.161 min
Response: 0
Conc: N.D.

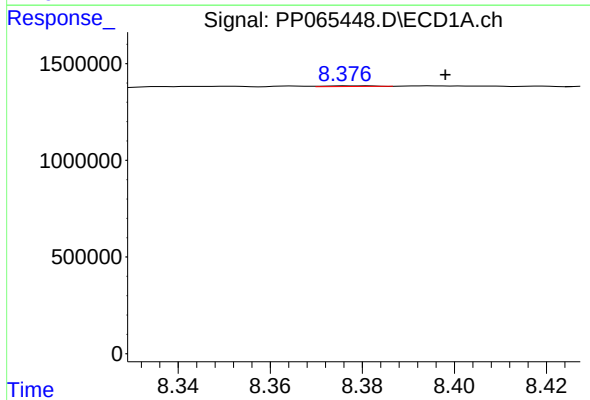


#35 AR-1260-5

R.T.: 8.377 min
Delta R.T.: -0.021 min
Response: 29118
Conc: 0.18 ng/ml

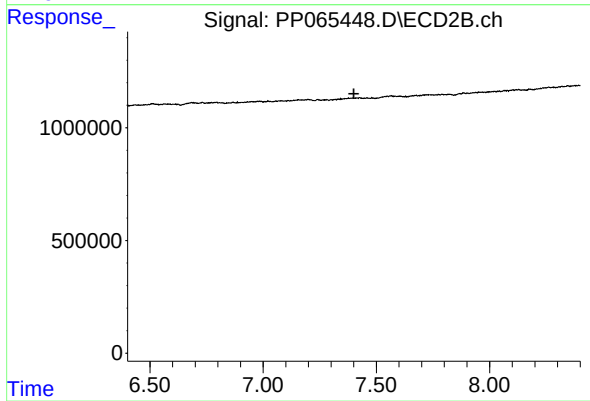

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.400 min
Response: 0
Conc: N.D.

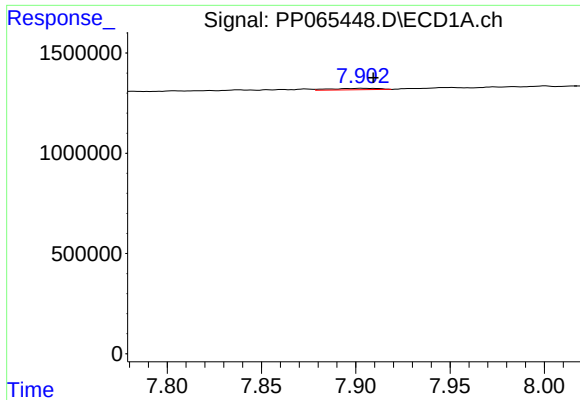

#36 AR-1262-1


R.T.: 7.904 min
Delta R.T.: -0.006 min
Response: 120898
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271315-1-2

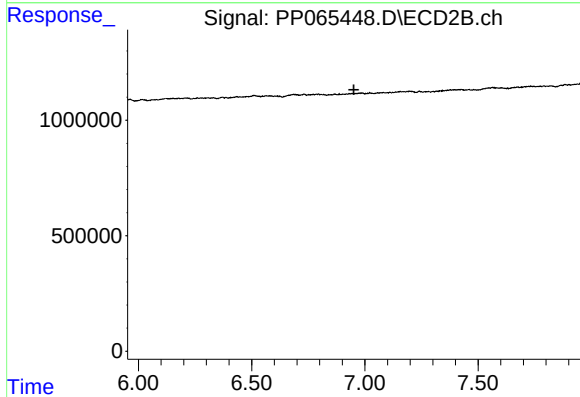


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

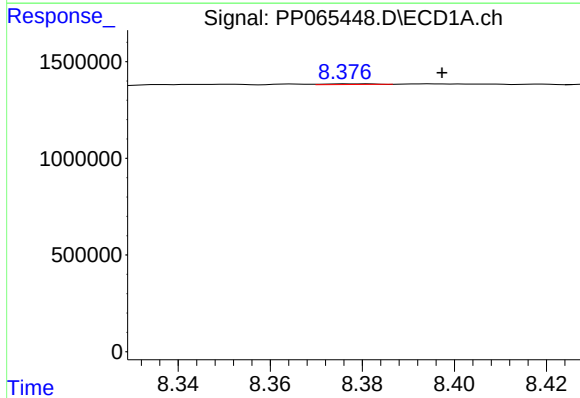

#37 AR-1262-2

R.T.: 8.377 min
Delta R.T.: -0.021 min
Response: 29118
Conc: 0.16 ng/ml

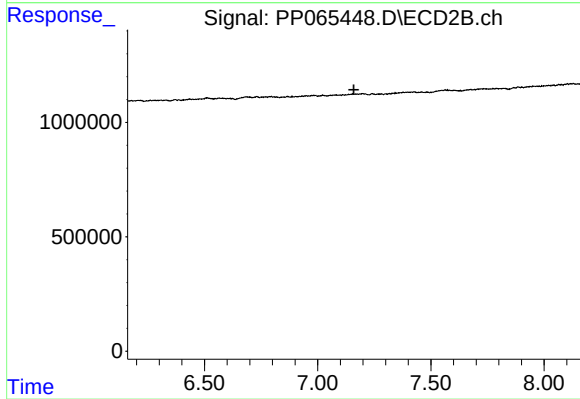

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.