

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060424\
 Data File : PP065462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 15:43
 Operator : YP\AJ
 Sample : PB161300BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB161300BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 00:58:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 04 04:29:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.471	3.750	35930683	29630457	21.587	19.789
2) SA Decachlor...	10.209	8.812	37416218	29142043	22.685	19.919
Target Compounds						
3) L1 AR-1016-1	5.625	0.000	179538	0	3.162	N.D. #
9) L2 AR-1221-2	4.777f	0.000	470944	0	26.996	N.D. #
16) L4 AR-1242-1	5.625	0.000	179538	0	3.869	N.D. #
21) L5 AR-1248-1	5.625	0.000	179538	0	5.098	N.D. #
33) L7 AR-1260-3	7.839	0.000	174868	0	2.186	N.D. #
35) L7 AR-1260-5	8.386	0.000	177291	0	1.091	N.D. #
36) L8 AR-1262-1	7.915	0.000	110599	0	2.286	N.D. #
37) L8 AR-1262-2	8.386	0.000	177291	0	0.945	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060424\
Data File : PP065462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 15:43
Operator : YP\AJ
Sample : PB161300BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB161300BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 00:58:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 04 04:29:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

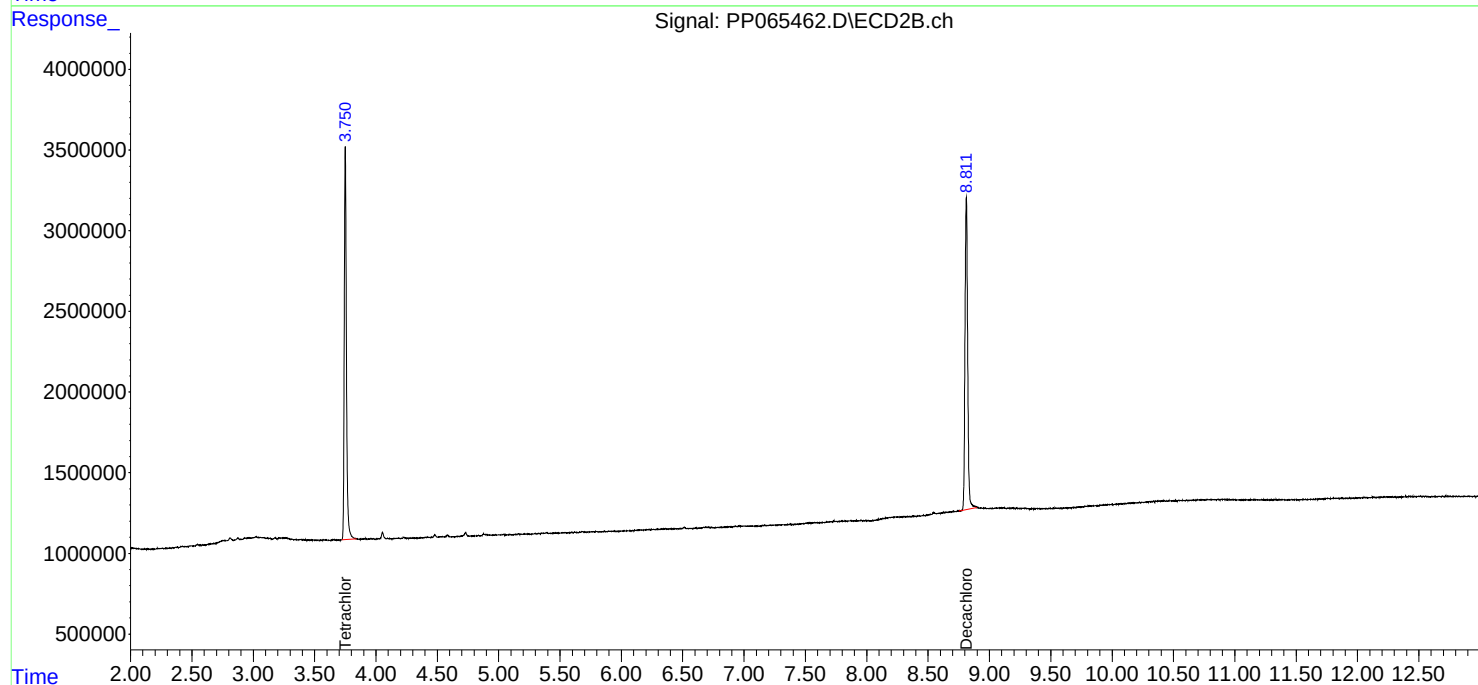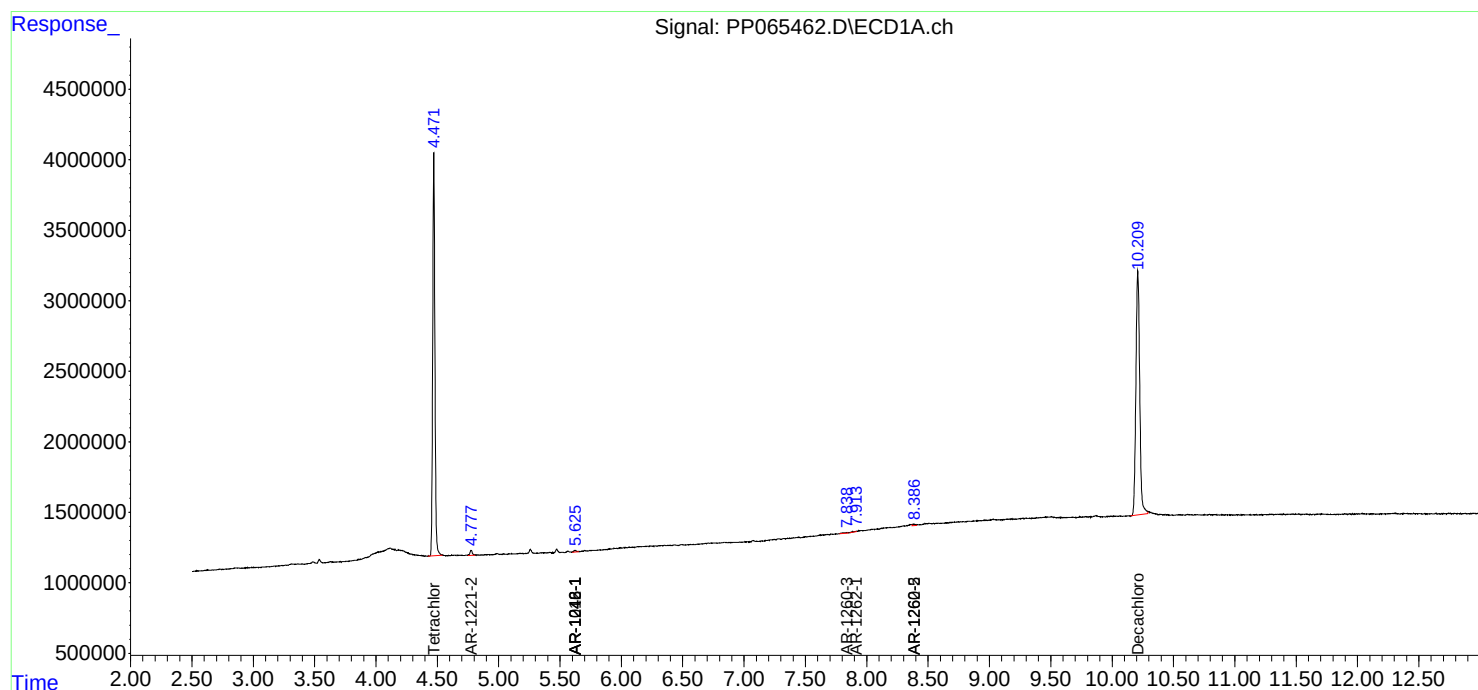


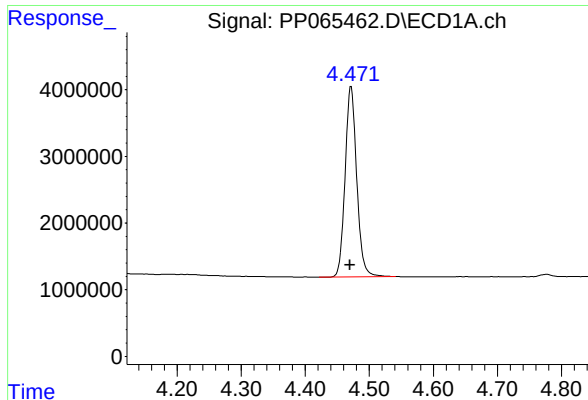

#1 Tetrachloro-m-xylene


R.T.: 4.471 min
Delta R.T.: 0.001 min
Response: 35930683
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161300BL

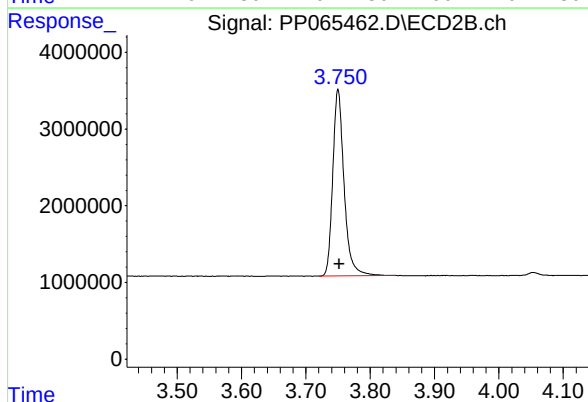


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.002 min
Response: 29630457
Conc: 19.79 ng/ml

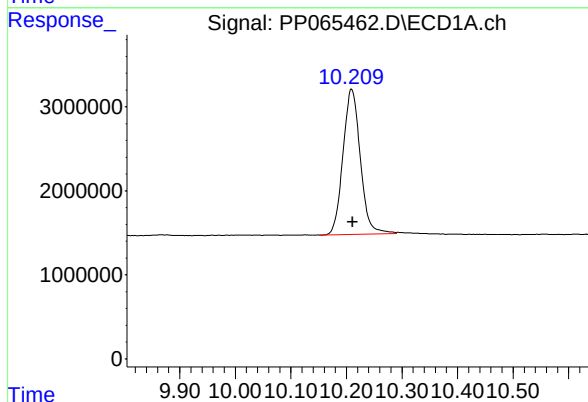


#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.002 min
Response: 37416218
Conc: 22.69 ng/ml

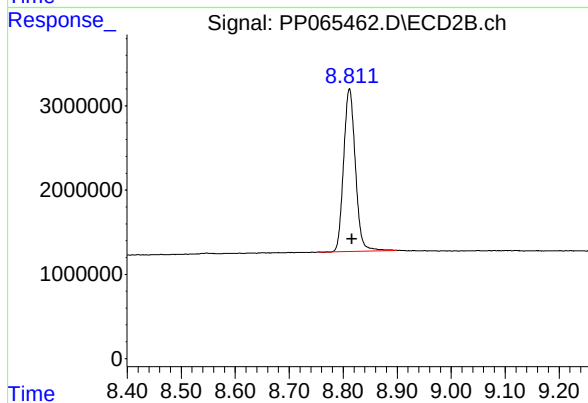

#2 Decachlorobiphenyl


R.T.: 8.812 min
Delta R.T.: -0.005 min
Response: 29142043
Conc: 19.92 ng/ml

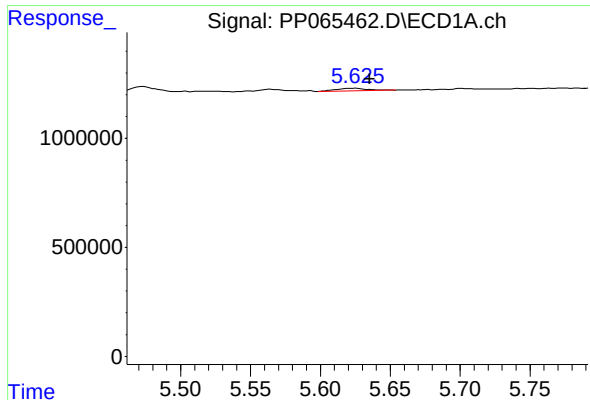

#3 AR-1016-1


R.T.: 5.625 min
Delta R.T.: -0.010 min
Response: 179538
Conc: 3.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161300BL

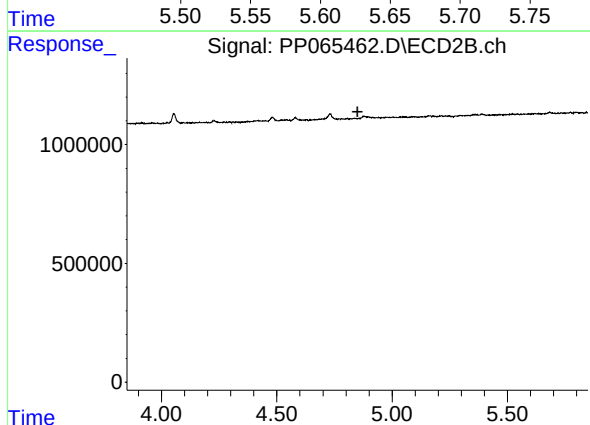


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.850 min
Response: 0
Conc: N.D.

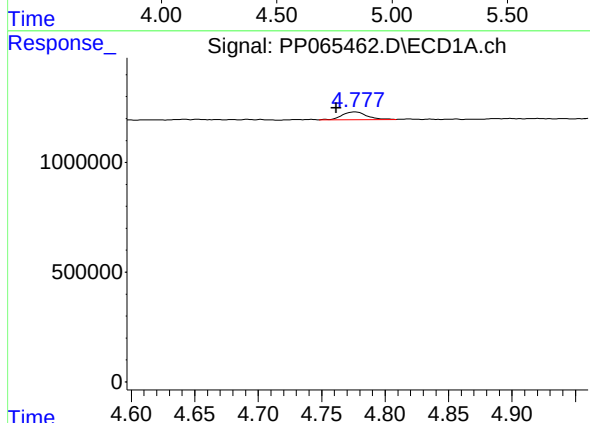


#9 AR-1221-2

R.T.: 4.777 min
Delta R.T.: 0.015 min
Response: 470944
Conc: 27.00 ng/ml

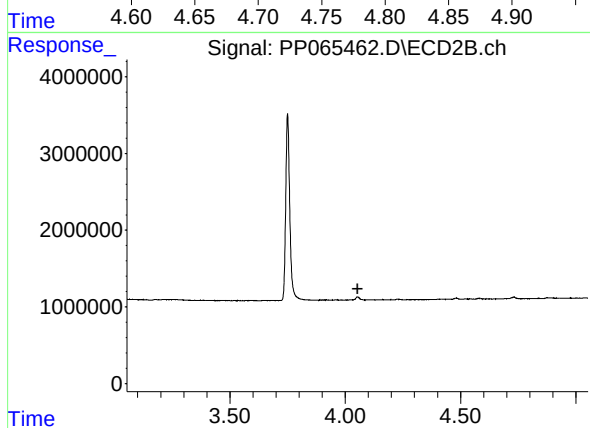

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.053 min
Response: 0
Conc: N.D.

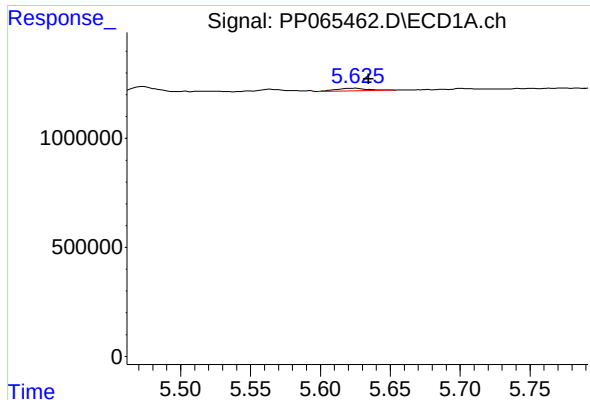

#16 AR-1242-1


R.T.: 5.625 min
Delta R.T.: -0.010 min
Response: 179538
Conc: 3.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161300BL

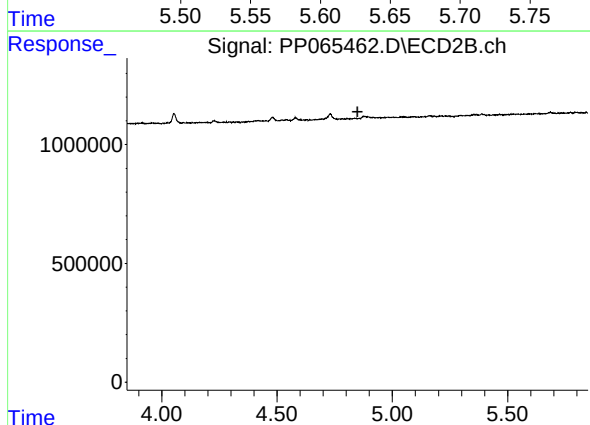


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.849 min
Response: 0
Conc: N.D.

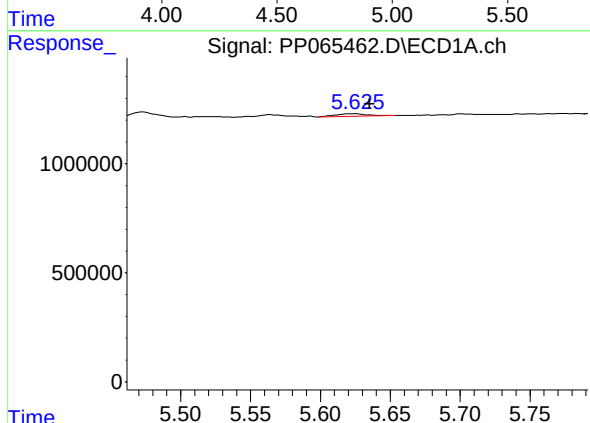


#21 AR-1248-1

R.T.: 5.625 min
Delta R.T.: -0.010 min
Response: 179538
Conc: 5.10 ng/ml

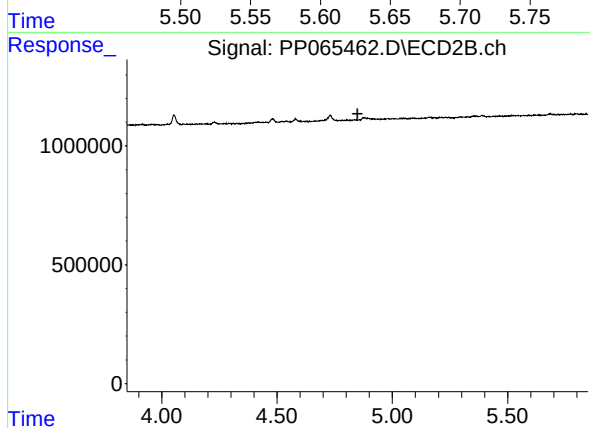

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.849 min
Response: 0
Conc: N.D.

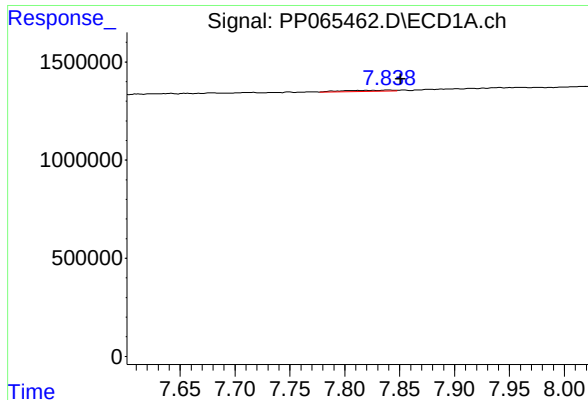

#33 AR-1260-3


R.T.: 7.839 min
Delta R.T.: -0.011 min
Response: 174868
Conc: 2.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161300BL

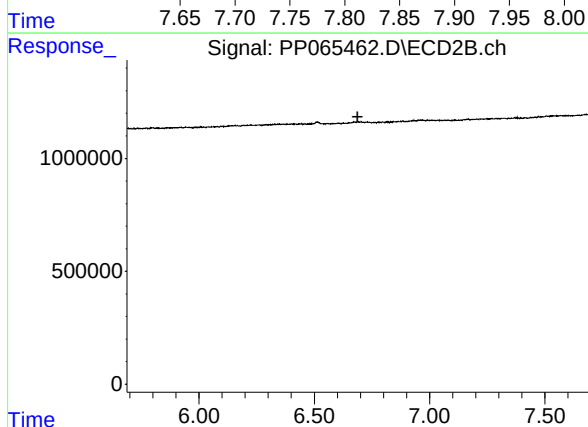


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.688 min
Response: 0
Conc: N.D.

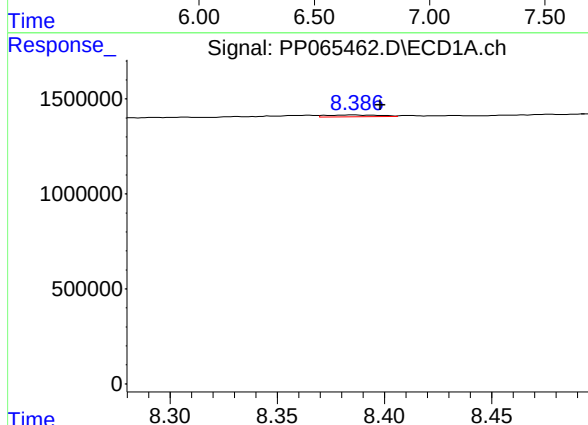


#35 AR-1260-5

R.T.: 8.386 min
Delta R.T.: -0.012 min
Response: 177291
Conc: 1.09 ng/ml

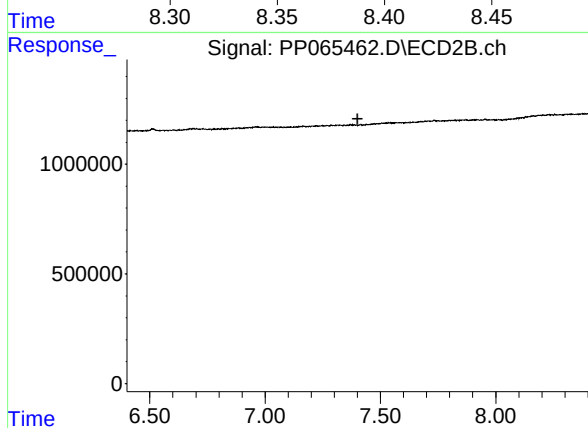

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.400 min
Response: 0
Conc: N.D.

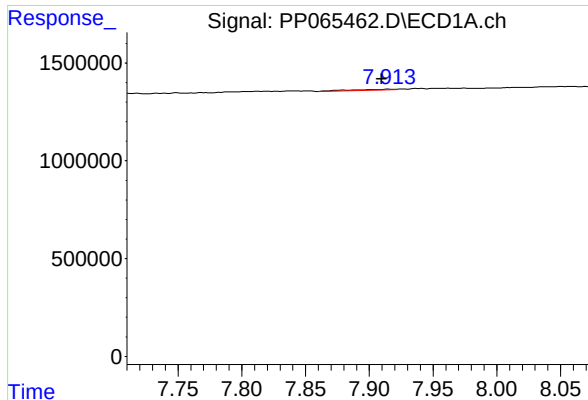

#36 AR-1262-1


R.T.: 7.915 min
Delta R.T.: 0.005 min
Response: 110599
Conc: 2.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB161300BL

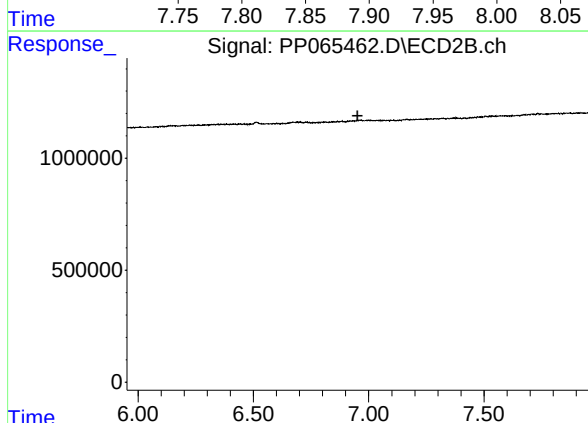


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

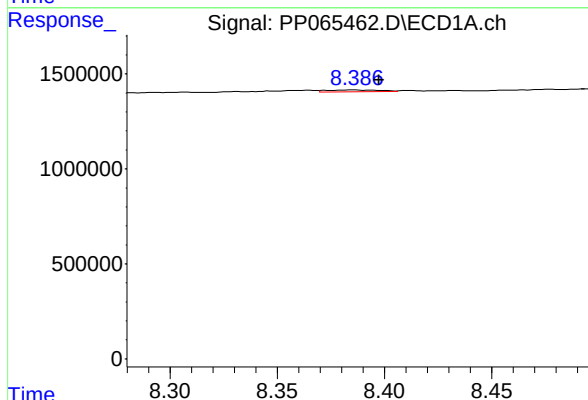

#37 AR-1262-2

R.T.: 8.386 min
Delta R.T.: -0.011 min
Response: 177291
Conc: 0.95 ng/ml

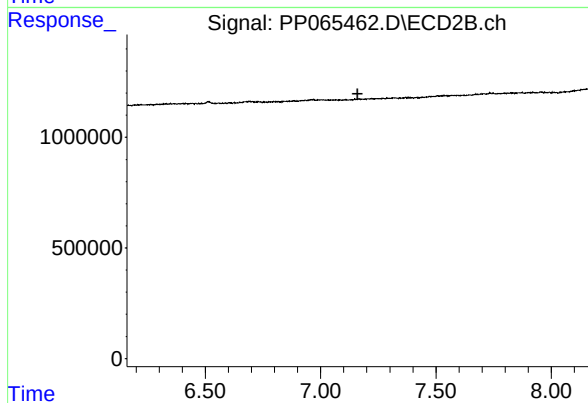

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.