

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060523\
 Data File : PP058215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2023 10:29
 Operator : YP\AJ
 Sample : 02998-01 (Sig #1); 02998-01RE (Sig #2)
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-2-053123

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 11:22:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.619	53565798	58224859	24.416	25.669
2) SA Decachlor...	10.205	8.678	32043250	33404829	28.276	21.280

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060523\
Data File : PP058215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2023 10:29
Operator : YP\AJ
Sample : 02998-01 (Sig #1); 02998-01RE (Sig #2)
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PAT-2-053123

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 11:22:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

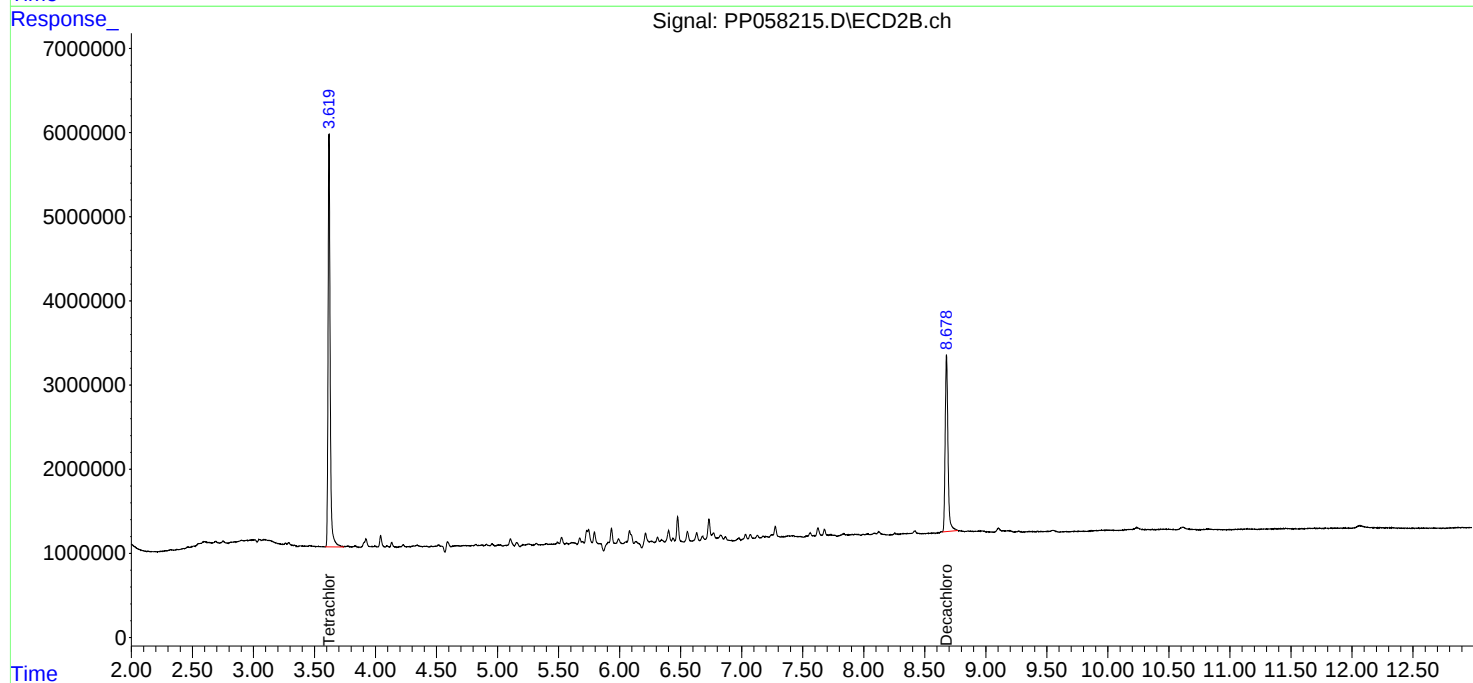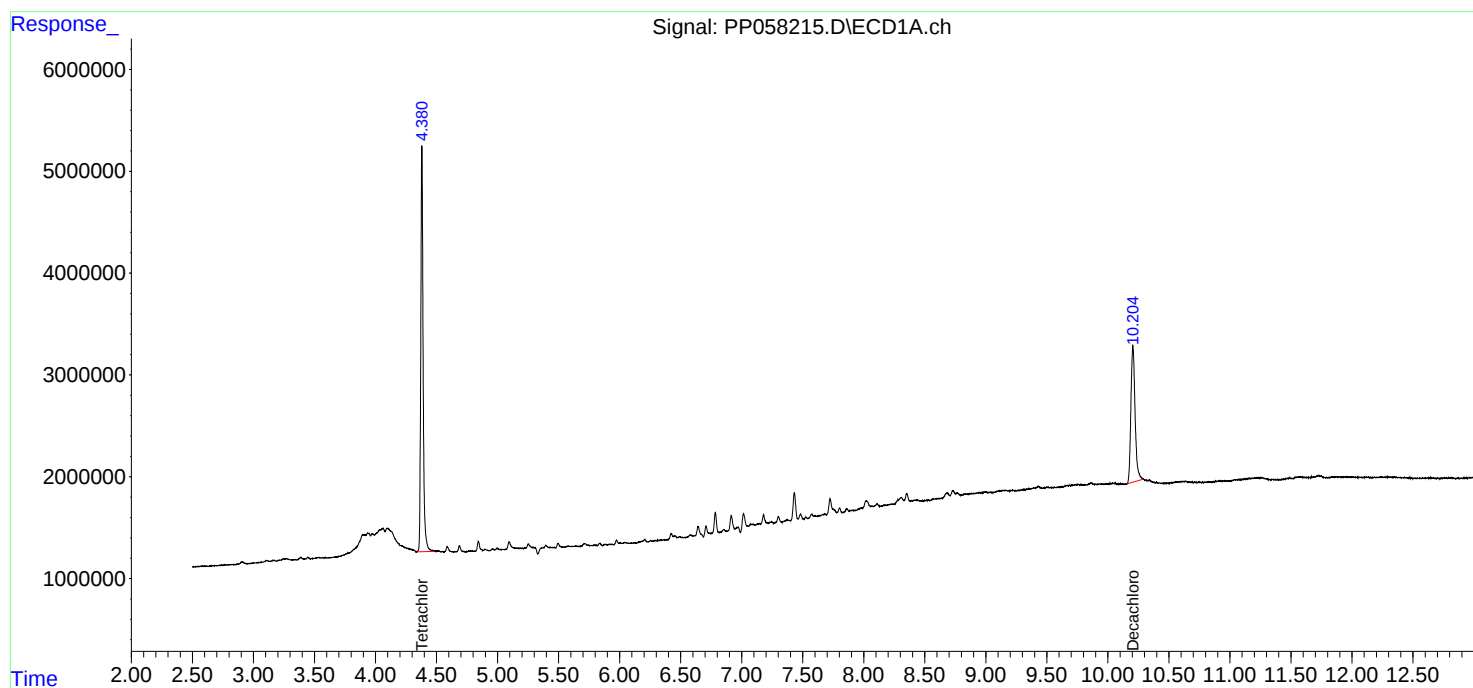


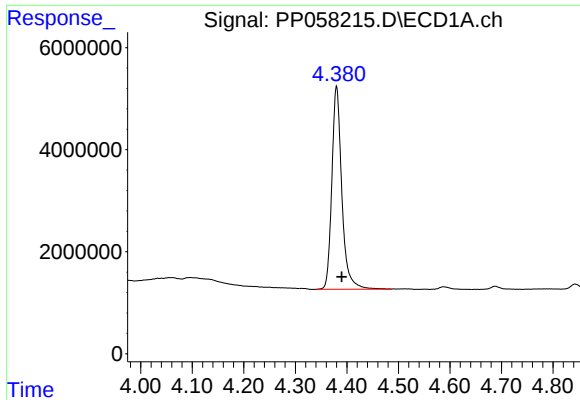

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: -0.010 min
Response: 53565798
Conc: 24.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-2-053123

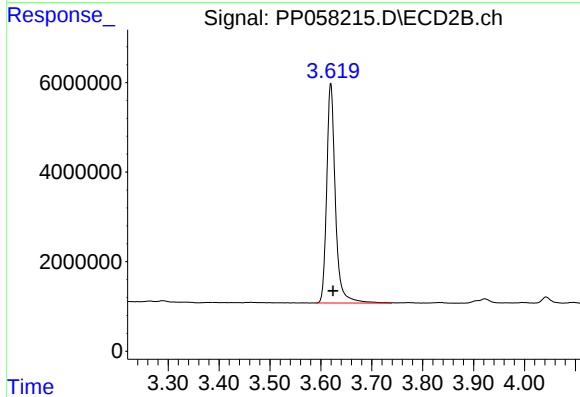


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.004 min
Response: 58224859
Conc: 25.67 ng/ml

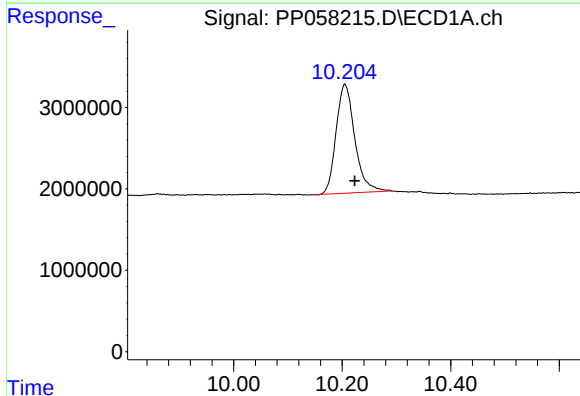

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.018 min
Response: 32043250
Conc: 28.28 ng/ml

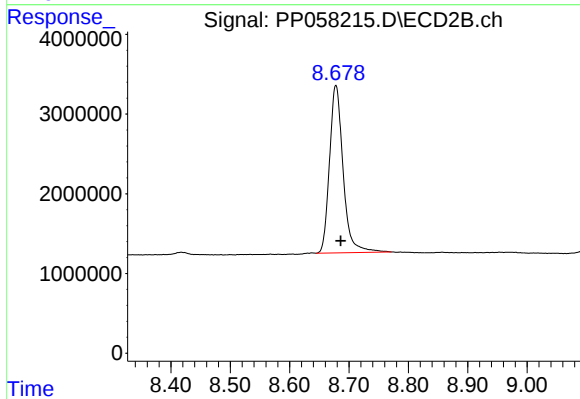

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.008 min
Response: 33404829
Conc: 21.28 ng/ml