



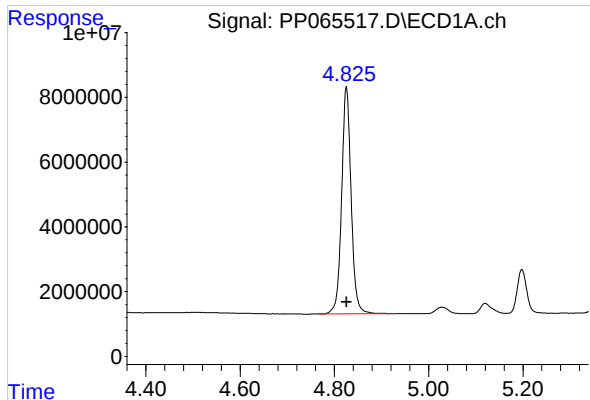

#1 Tetrachloro-m-xylene

R.T.: 4.826 min
Delta R.T.: 0.000 min
Response: 98475177
Conc: 51.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP060524

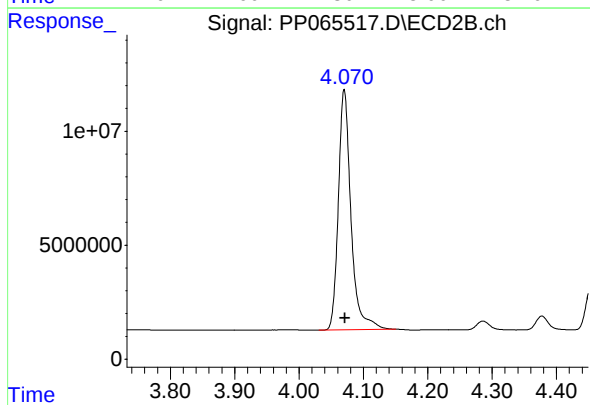

#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.001 min
Response: 144118909
Conc: 51.61 ng/ml