

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
 Data File : PP036251.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2021 13:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 15:16:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.969	3.963	840798	557850	18.891	19.988
2)	SA Decachlor...	11.000	9.270	820197	530039	19.192	23.104
Target Compounds							
9)	L2 AR-1221-2	5.321	0.000	12018	0	28.831	N.D. #
15)	L3 AR-1232-5	6.575	0.000	8078	0	25.133	N.D. #
20)	L4 AR-1242-5	7.255	0.000	14130	0	14.823	N.D. #
22)	L5 AR-1248-2	6.575	0.000	8078	0	6.757	N.D. #
24)	L5 AR-1248-4	7.231	0.000	34579	0	21.713	N.D. #
25)	L5 AR-1248-5	7.255	0.000	14130	0	9.051	N.D. #
26)	L6 AR-1254-1	7.200	0.000	63976	0	39.488	N.D. #
32)	L7 AR-1260-2	8.238	0.000	3209	0	1.313	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
Data File : PP036251.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2021 13:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 15:16:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

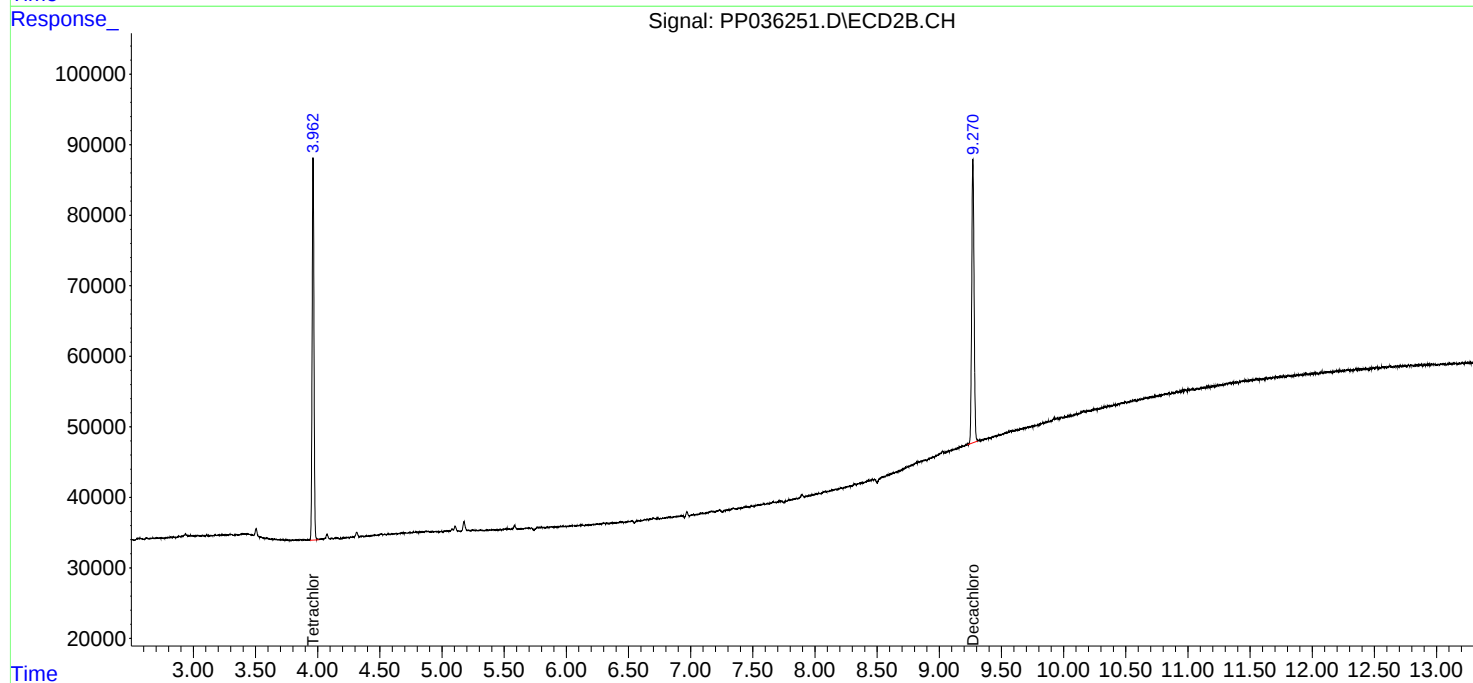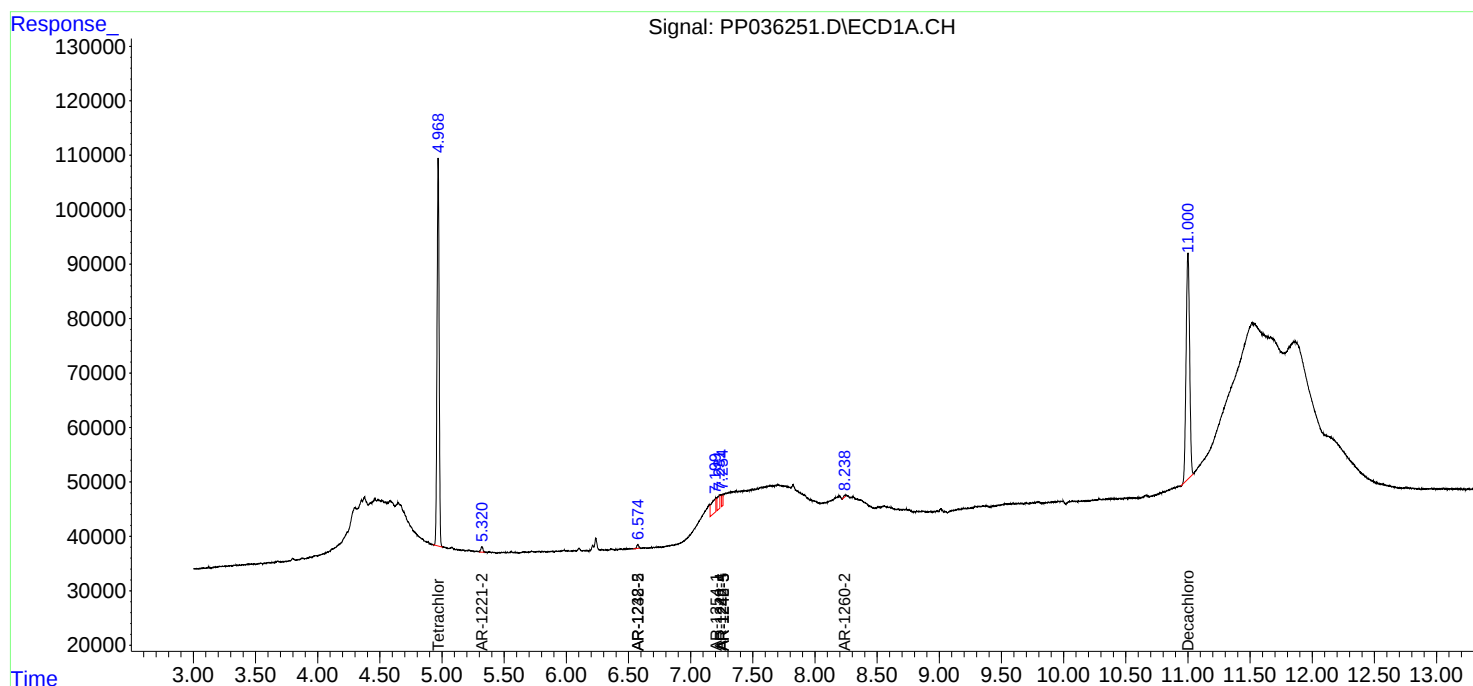


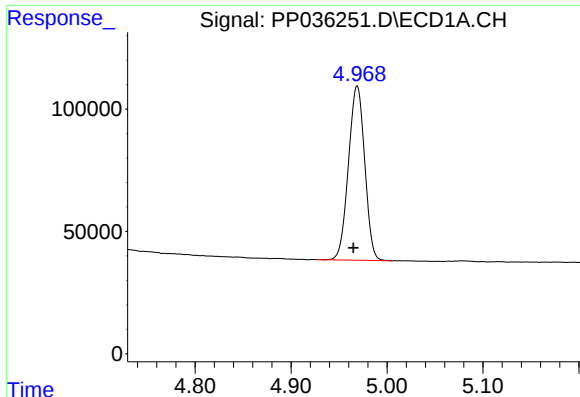

#1 Tetrachloro-m-xylene


R.T.: 4.969 min
Delta R.T.: 0.004 min
Response: 840798
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

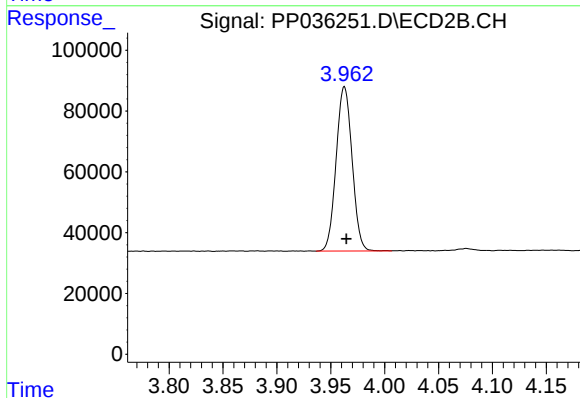


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.002 min
Response: 557850
Conc: 19.99 ng/ml

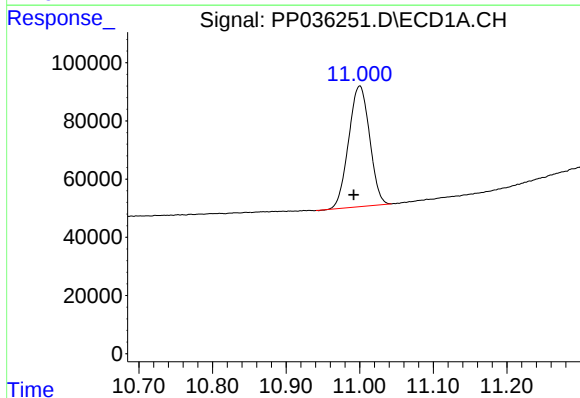


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.008 min
Response: 820197
Conc: 19.19 ng/ml

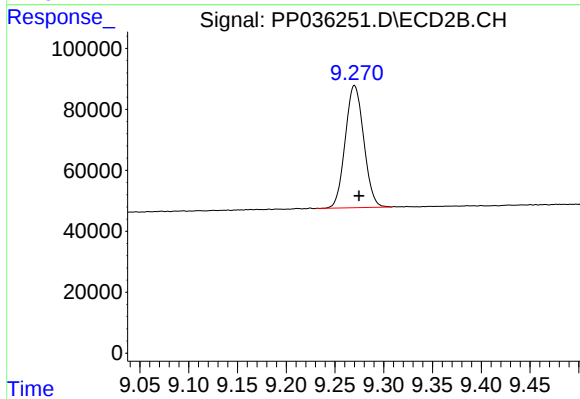

#2 Decachlorobiphenyl


R.T.: 9.270 min
Delta R.T.: -0.005 min
Response: 530039
Conc: 23.10 ng/ml

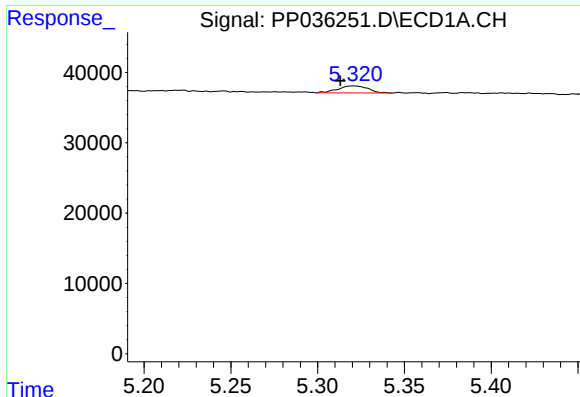

#9 AR-1221-2


R.T.: 5.321 min
Delta R.T.: 0.007 min
Response: 12018
Conc: 28.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

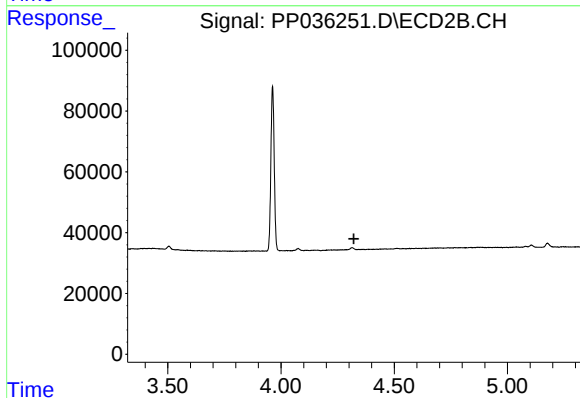


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.322 min
Response: 0
Conc: N.D.

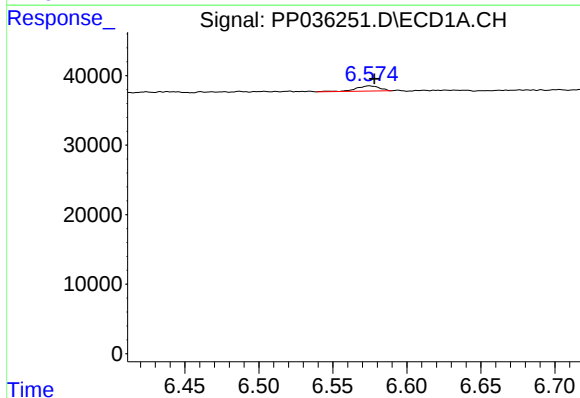


#15 AR-1232-5

R.T.: 6.575 min
Delta R.T.: -0.003 min
Response: 8078
Conc: 25.13 ng/ml

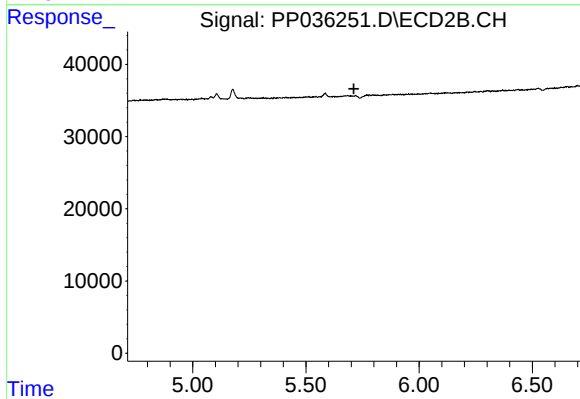

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

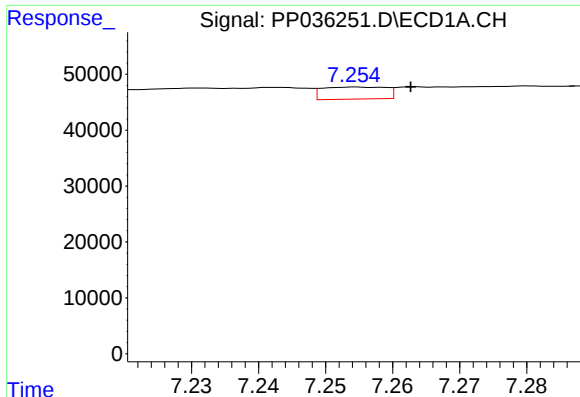

#20 AR-1242-5


R.T.: 7.255 min
Delta R.T.: -0.008 min
Response: 14130
Conc: 14.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

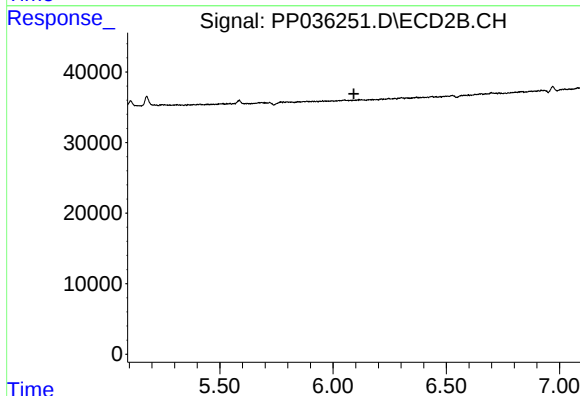


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.092 min
Response: 0
Conc: N.D.

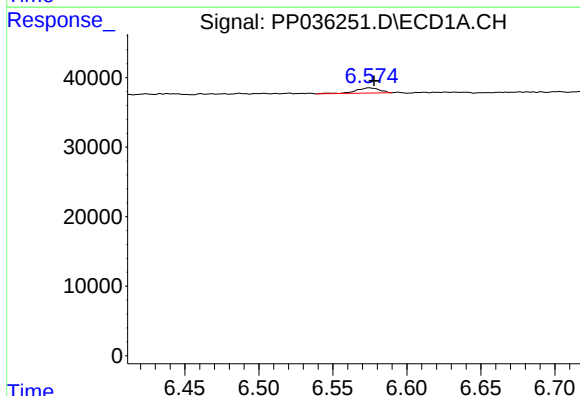


#22 AR-1248-2

R.T.: 6.575 min
Delta R.T.: -0.003 min
Response: 8078
Conc: 6.76 ng/ml

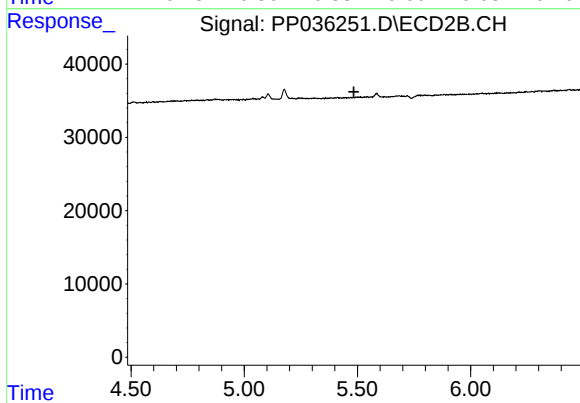

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.484 min
Response: 0
Conc: N.D.

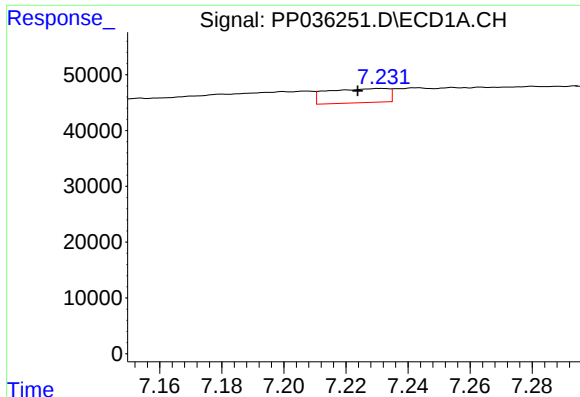

#24 AR-1248-4


R.T.: 7.231 min
Delta R.T.: 0.008 min
Response: 34579
Conc: 21.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

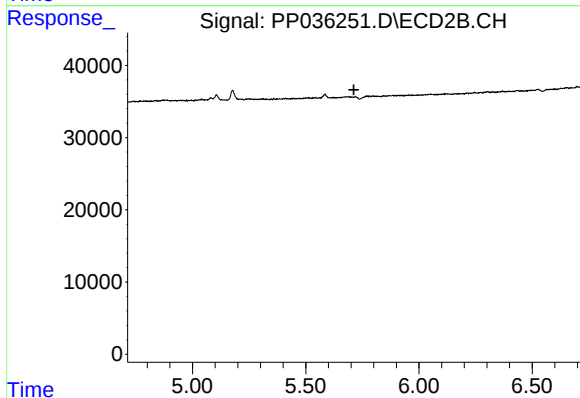


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

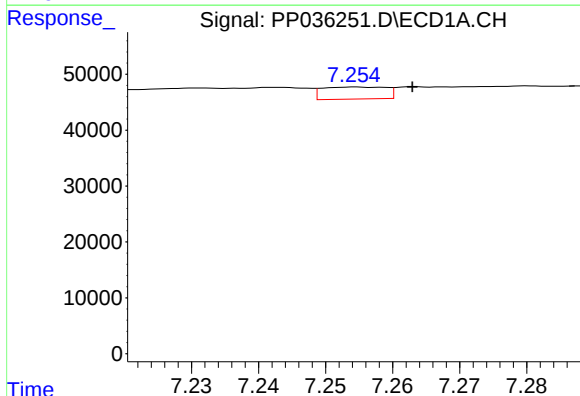


#25 AR-1248-5

R.T.: 7.255 min
Delta R.T.: -0.008 min
Response: 14130
Conc: 9.05 ng/ml

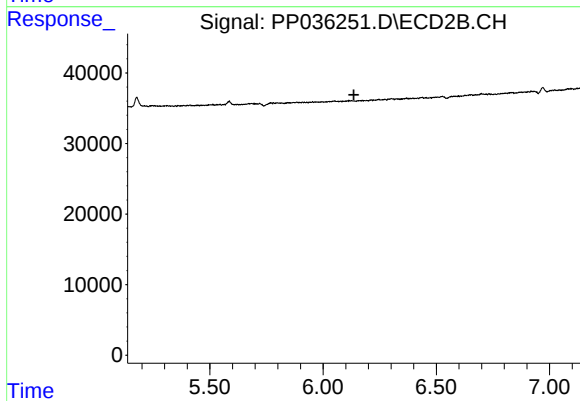

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

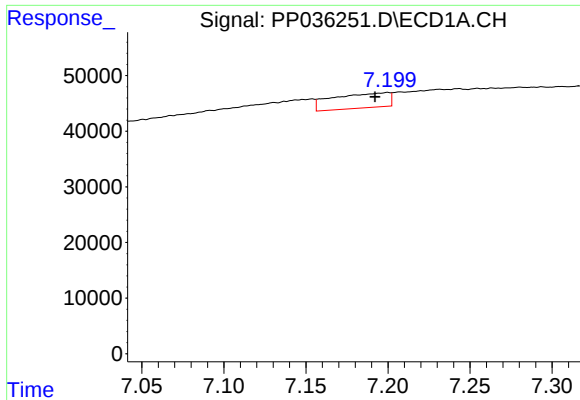

#26 AR-1254-1


R.T.: 7.200 min
Delta R.T.: 0.008 min
Response: 63976
Conc: 39.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

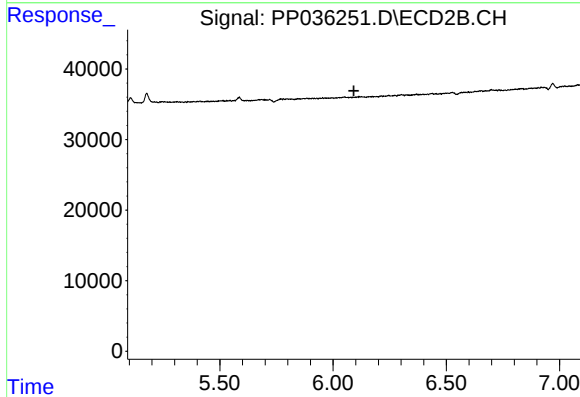


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.092 min
Response: 0
Conc: N.D.

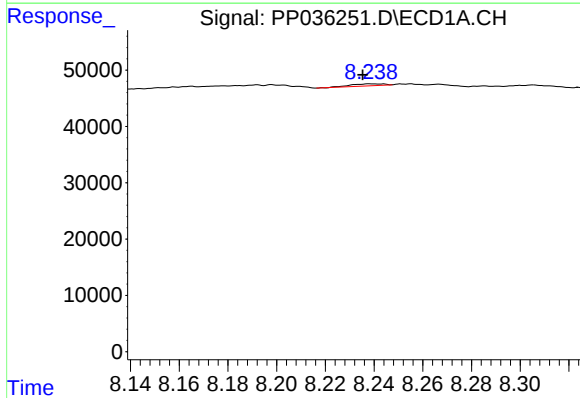

#32 AR-1260-2

R.T.: 8.238 min
Delta R.T.: 0.003 min
Response: 3209
Conc: 1.31 ng/ml

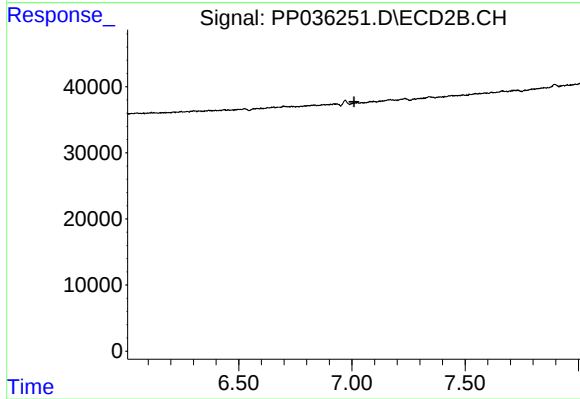

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.