

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
 Data File : PP036247.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2021 12:01
 Operator : DD\AJ
 Sample : M2609-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IDW-AQ-FT1-060321

Manual Integrations
 APPROVED

Ankita
 6/8/2021 3:22:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 15:15:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.964	3.960	984192	681416	22.112	24.415m
2) SA Decachlor...	10.991	9.267	845461	519282	19.783	22.635

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
Data File : PP036247.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2021 12:01
Operator : DD\AJ
Sample : M2609-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IDW-AQ-FT1-060321


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 15:15:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

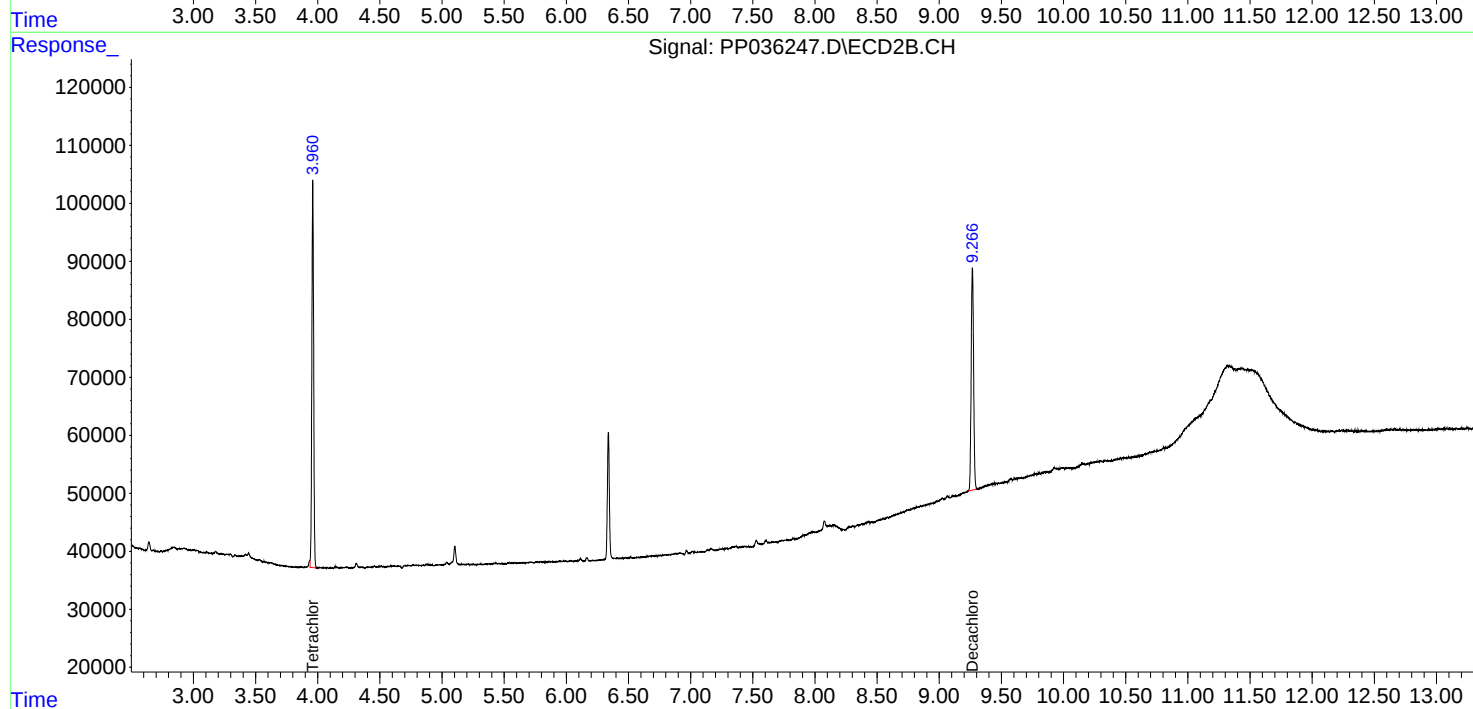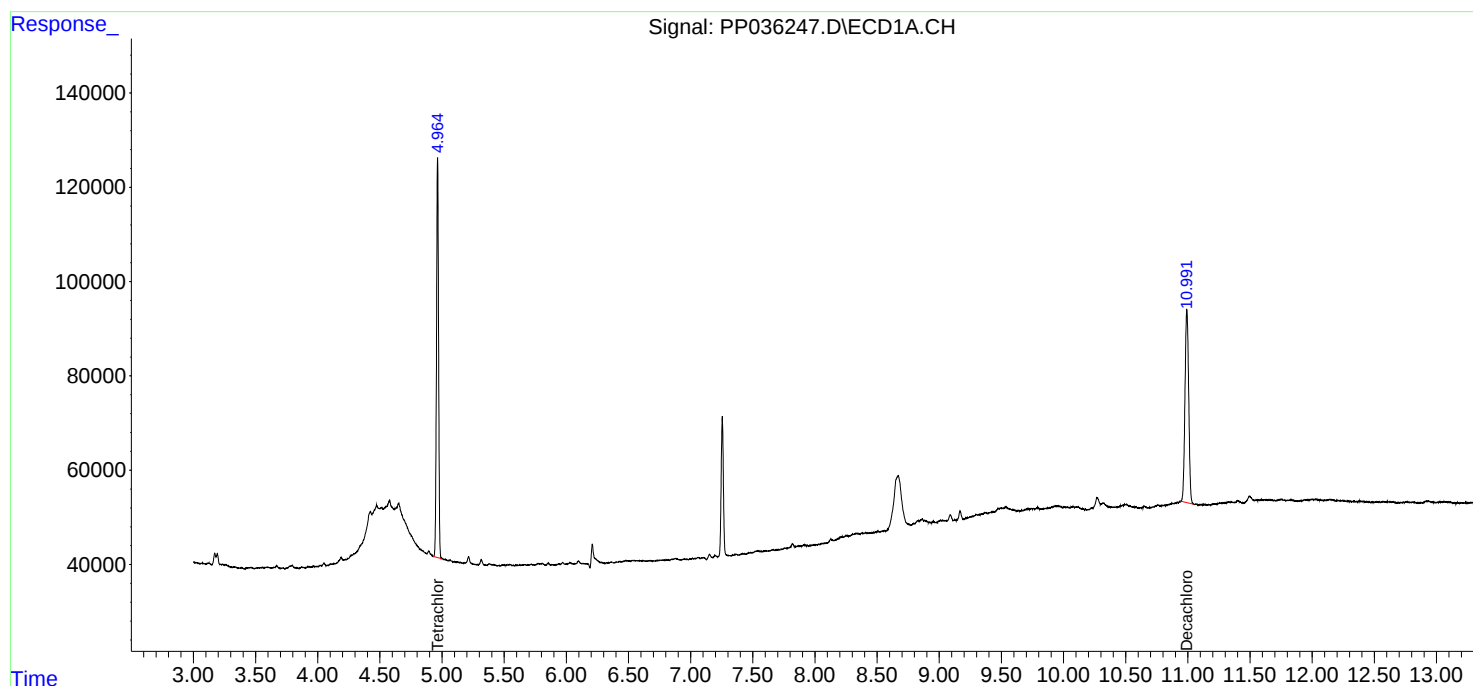

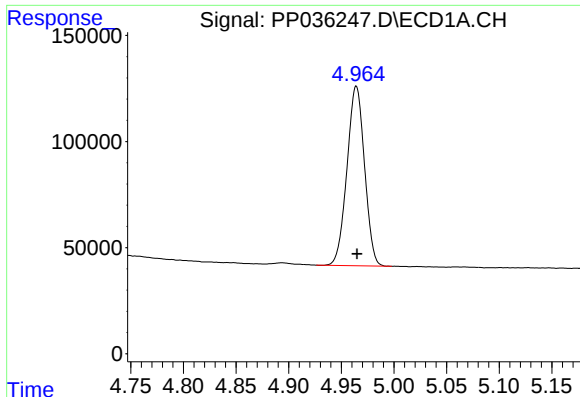


#1 Tetrachloro-m-xylene

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 984192
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
IDW-AQ-FT1-060321


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:07 PM

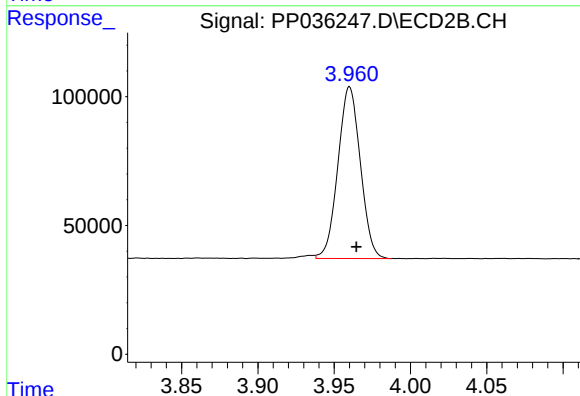


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.005 min
Response: 681416
Conc: 24.42 ng/ml m

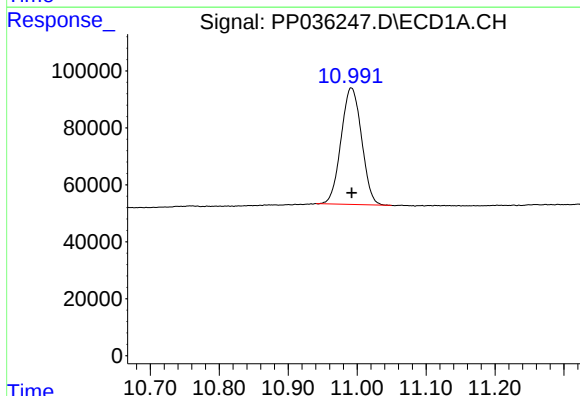

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: 0.000 min
Response: 845461
Conc: 19.78 ng/ml

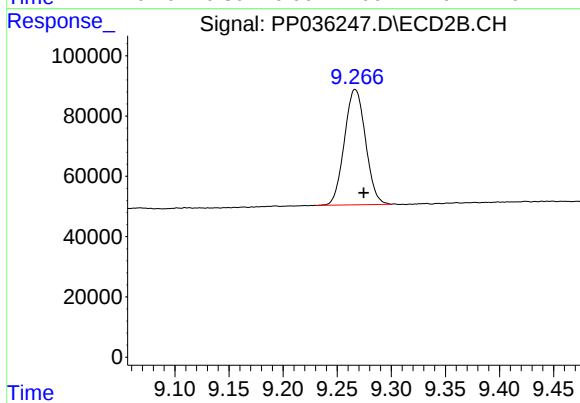

#2 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.008 min
Response: 519282
Conc: 22.63 ng/ml