

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
 Data File : PP036252.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2021 13:27
 Operator : DD\AJ
 Sample : M2603-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FAM4-WC1

Manual Integrations
 APPROVED

Ankita
 6/8/2021 3:22:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 15:16:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.961	840266	560539	18.879	20.084
2) SA Decachlor...	10.994	9.268	693350	415506	16.224	18.111
Target Compounds						
31) L7 AR-1260-1	7.971	6.807	133958	88535	66.129	70.959m
32) L7 AR-1260-2	8.235	7.004	232798	102419	95.293	67.964 #
33) L7 AR-1260-3	8.601	7.157	106534	95431	57.367	67.902
34) L7 AR-1260-4	8.830	7.643	169303	59820	75.817	51.167 #
35) L7 AR-1260-5	9.160	7.891	200323	137431	46.917	49.647

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060721\
Data File : PP036252.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2021 13:27
Operator : DD\AJ
Sample : M2603-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
FAM4-WC1


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 15:16:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

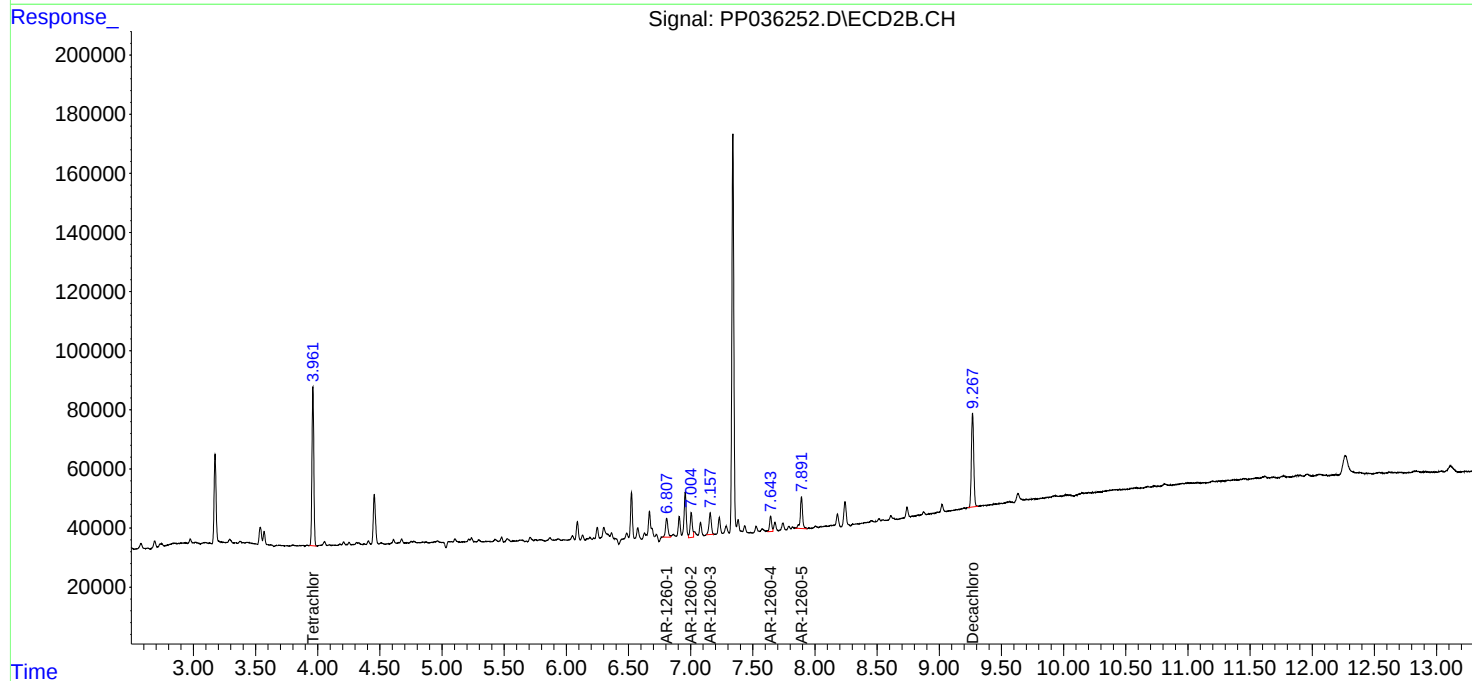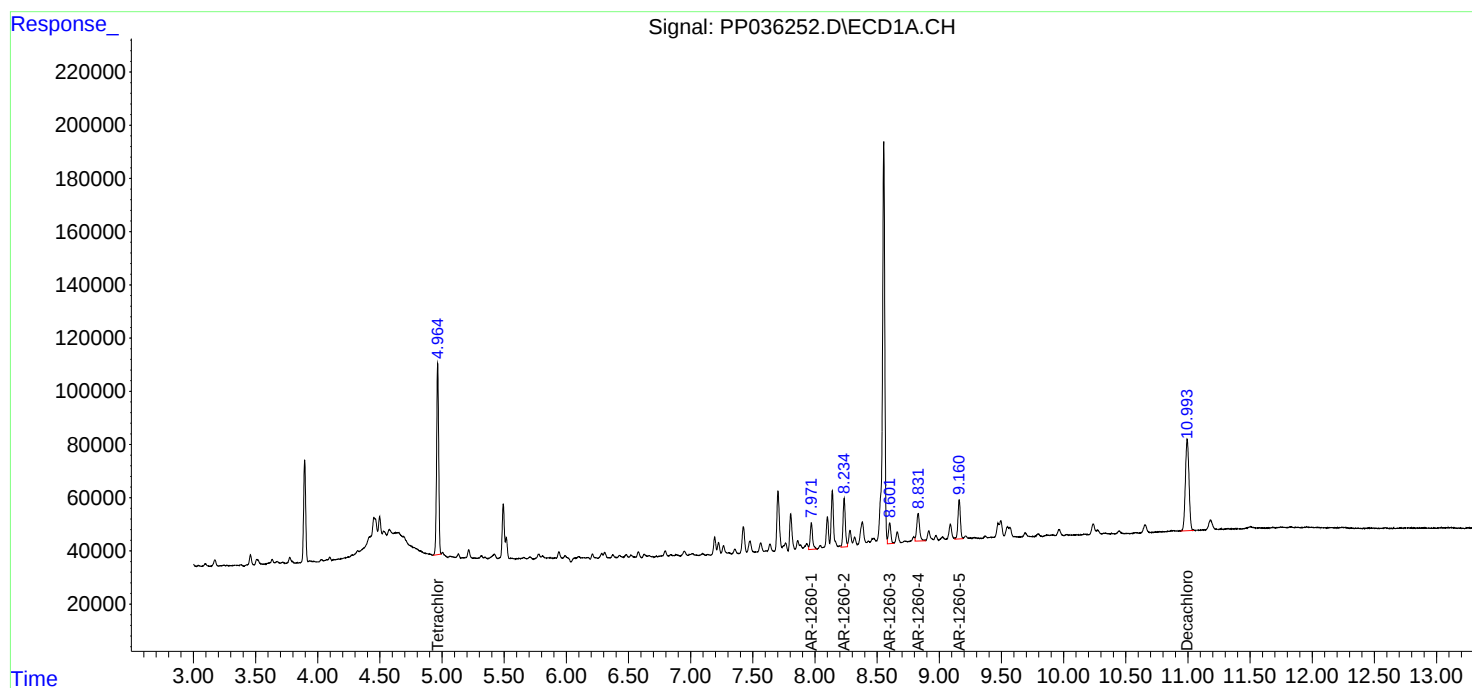

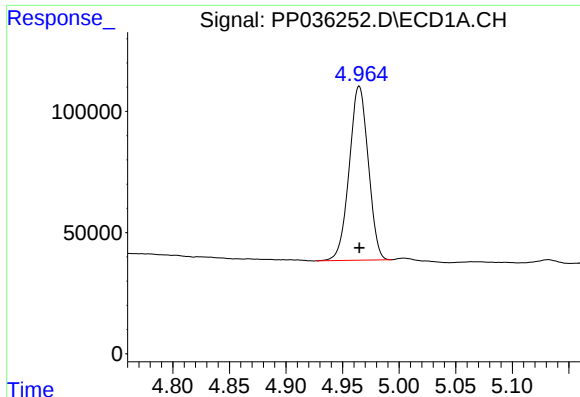


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 840266
Conc: 18.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
FAM4-WC1


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:12 PM

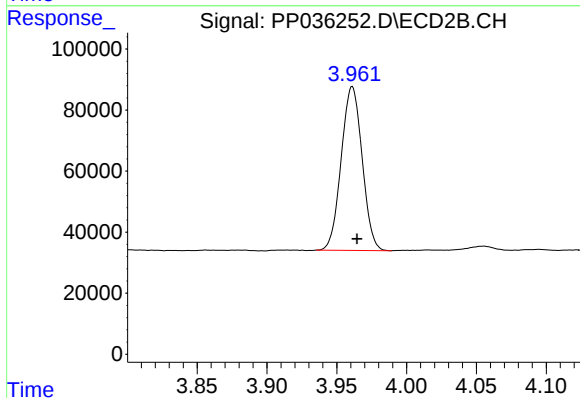


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.003 min
Response: 560539
Conc: 20.08 ng/ml

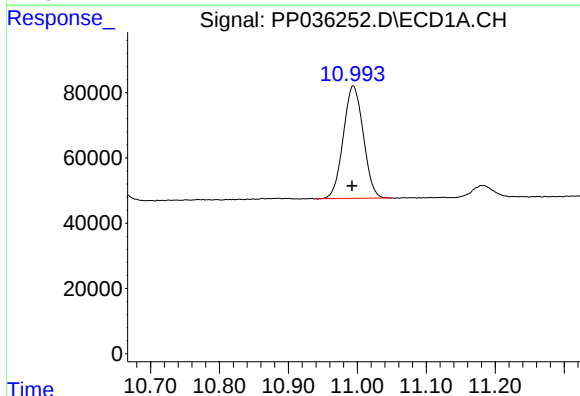


#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: 0.002 min
Response: 693350
Conc: 16.22 ng/ml

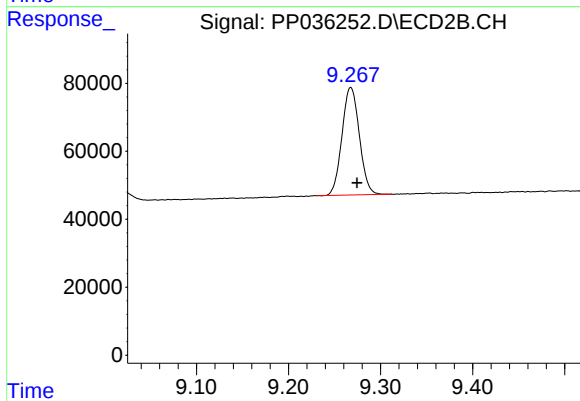

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: -0.007 min
Response: 415506
Conc: 18.11 ng/ml

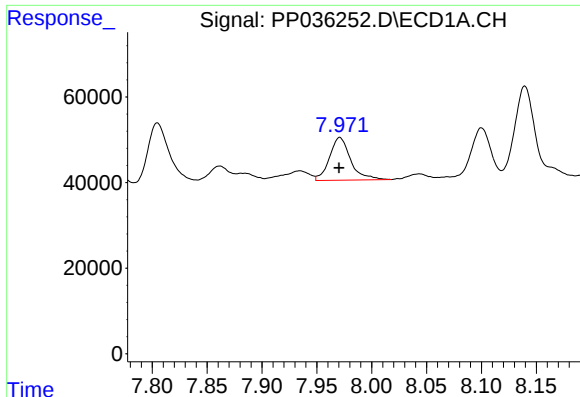


#31 AR-1260-1

R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 133958
Conc: 66.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
FAM4-WC1


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:12 PM

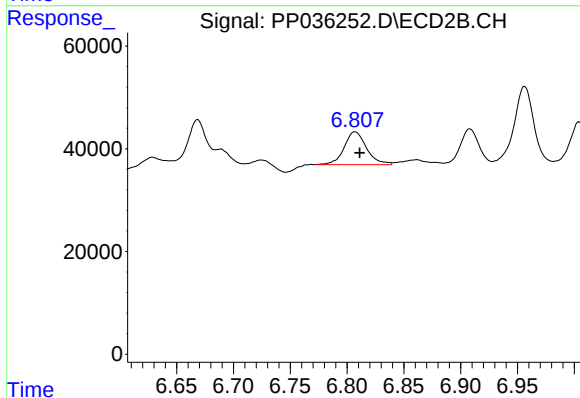


#31 AR-1260-1

R.T.: 6.807 min
Delta R.T.: -0.004 min
Response: 88535
Conc: 70.96 ng/ml m

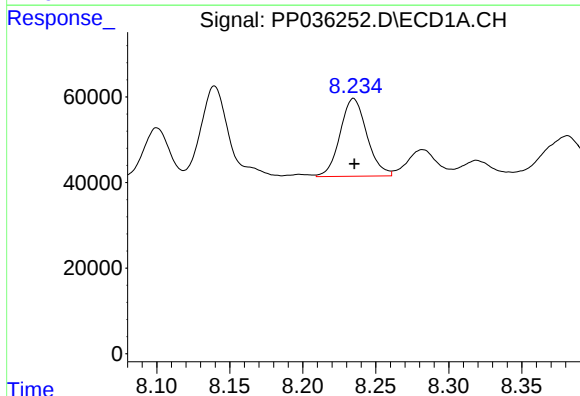


#32 AR-1260-2

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 232798
Conc: 95.29 ng/ml

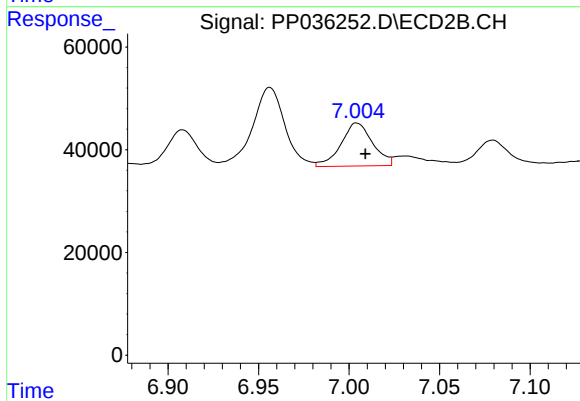

#32 AR-1260-2

R.T.: 7.004 min
Delta R.T.: -0.005 min
Response: 102419
Conc: 67.96 ng/ml

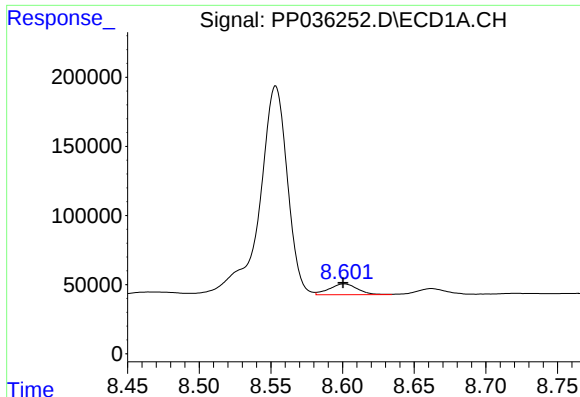


#33 AR-1260-3

R.T.: 8.601 min
Delta R.T.: 0.000 min
Response: 106534
Conc: 57.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
FAM4-WC1


Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:12 PM

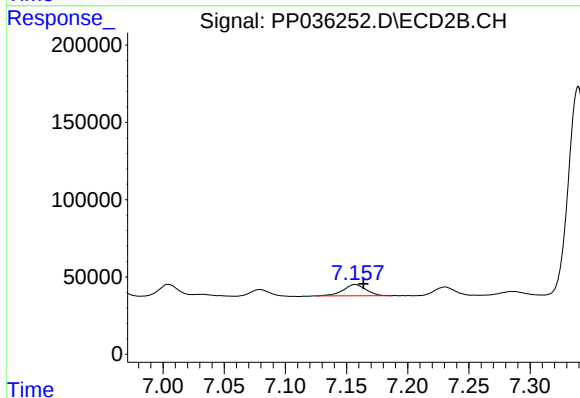


#33 AR-1260-3

R.T.: 7.157 min
Delta R.T.: -0.007 min
Response: 95431
Conc: 67.90 ng/ml

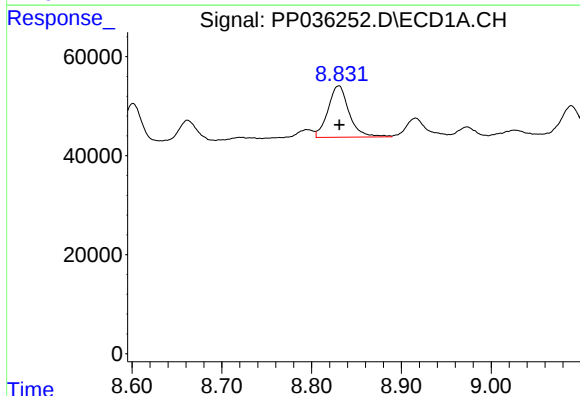


#34 AR-1260-4

R.T.: 8.830 min
Delta R.T.: 0.000 min
Response: 169303
Conc: 75.82 ng/ml

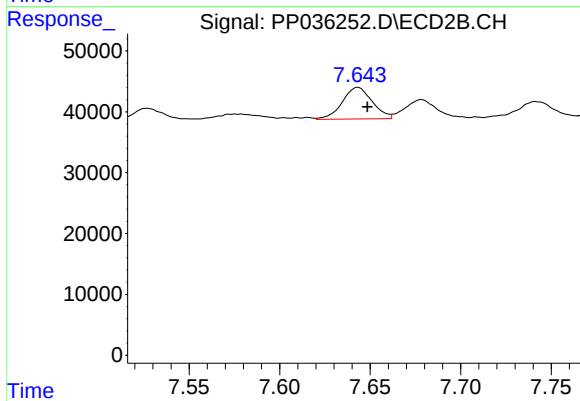

#34 AR-1260-4

R.T.: 7.643 min
Delta R.T.: -0.005 min
Response: 59820
Conc: 51.17 ng/ml

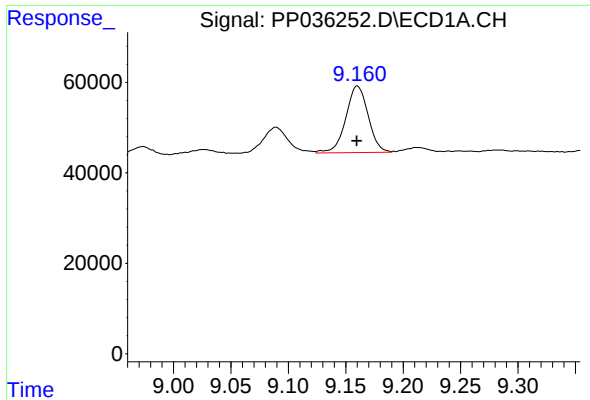


#35 AR-1260-5

R.T.: 9.160 min
Delta R.T.: 0.000 min
Response: 200323
Conc: 46.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FAM4-WC1

Manual Integrations
APPROVED

Ankita
6/8/2021 3:22:12 PM

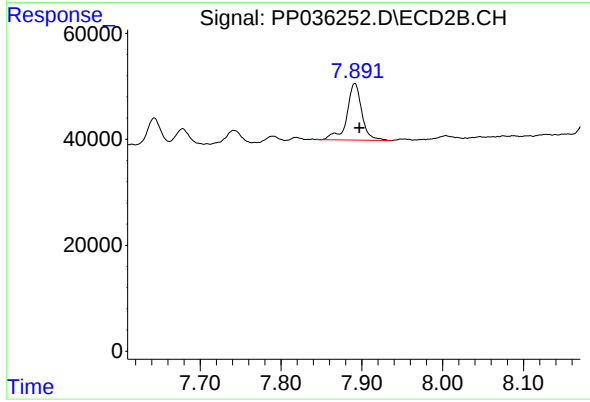

#35 AR-1260-5

R.T.: 7.891 min
Delta R.T.: -0.005 min
Response: 137431
Conc: 49.65 ng/ml