

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060821\
 Data File : PP036290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jun 2021 13:44
 Operator : DD\AJ
 Sample : M2626-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 18-B12(222-226)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 04:08:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.959	984507	653011	22.119	23.398
2)	SA Decachlor...	10.994	9.266	937572	576614	21.938	25.134

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060821\
Data File : PP036290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jun 2021 13:44
Operator : DD\AJ
Sample : M2626-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
18-B12(222-226)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 04:08:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

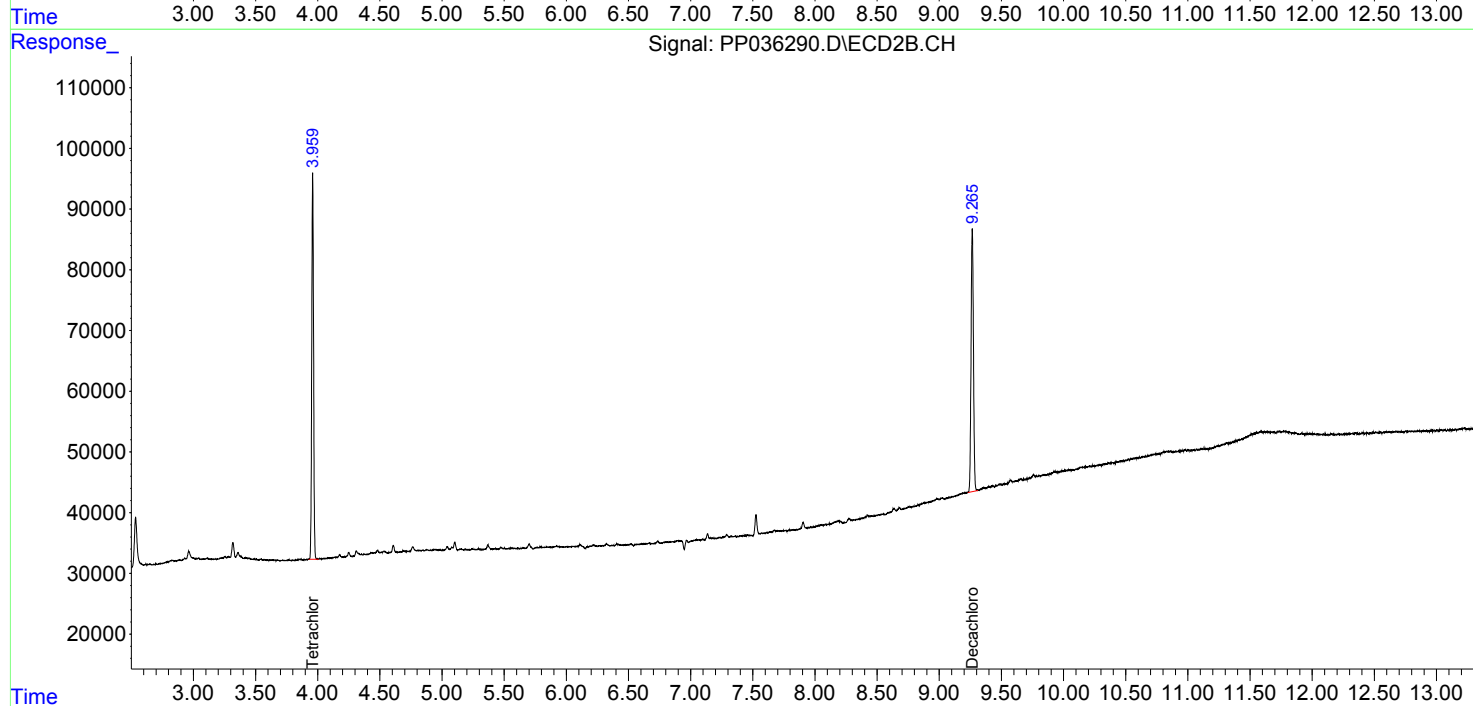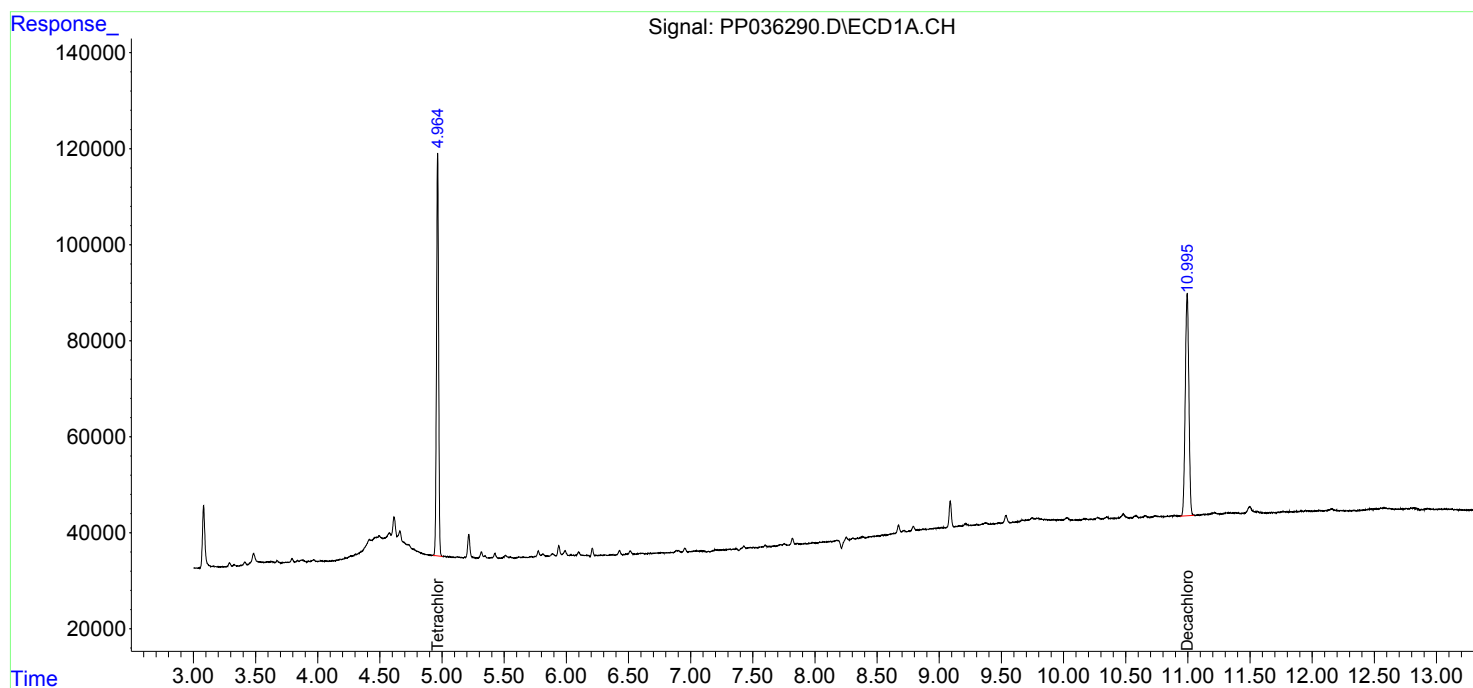


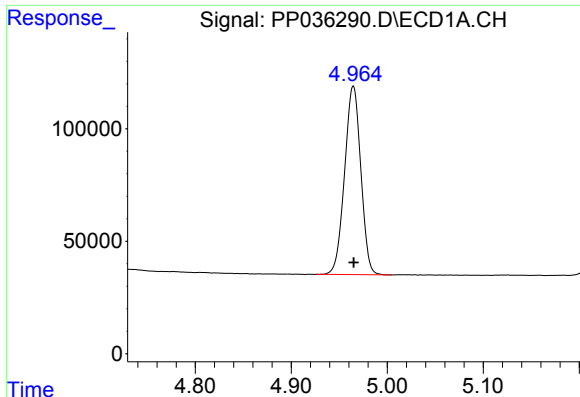

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 984507
Conc: 22.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
18-B12(222-226)

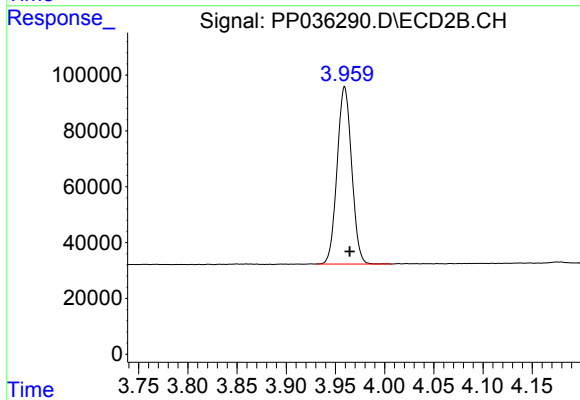


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.005 min
Response: 653011
Conc: 23.40 ng/ml

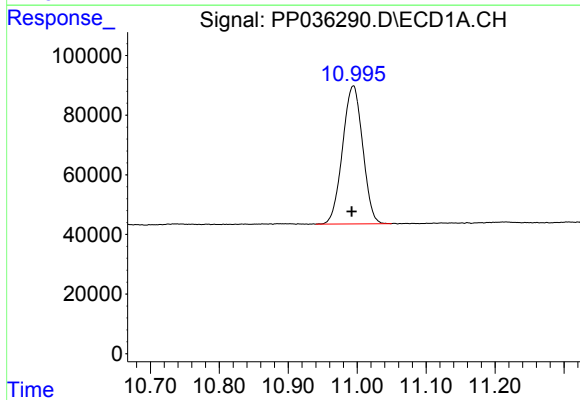

#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: 0.002 min
Response: 937572
Conc: 21.94 ng/ml

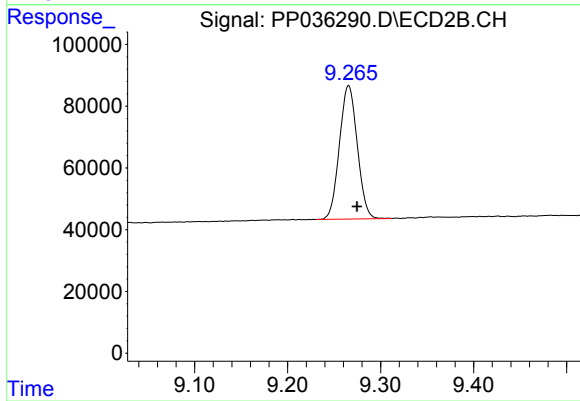

#2 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.009 min
Response: 576614
Conc: 25.13 ng/ml