

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
 Data File : PP058315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 14:30
 Operator : YP\AJ
 Sample : 03044-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-04-5.0-7.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:19:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 06 04:59:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.617	55196547	56415436	24.117	26.146
2) SA Decachlor...	10.206	8.678	32001055	36471044	28.648	22.120
Target Compounds						
26) L6 AR-1254-1	6.423	5.525	9183710	11077258	125.683	102.164
27) L6 AR-1254-2	6.644	5.674	13799647	10384954	134.376	106.980
28) L6 AR-1254-3	7.014	6.081	16882448	22561178	171.245	145.713
29) L6 AR-1254-4	7.303	6.311	12903575	9350081	194.465m	99.642 #
30) L6 AR-1254-5	7.726	6.732	15480615	25511237	211.550	175.505

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
Data File : PP058315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 14:30
Operator : YP\AJ
Sample : 03044-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:19:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 06 04:59:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

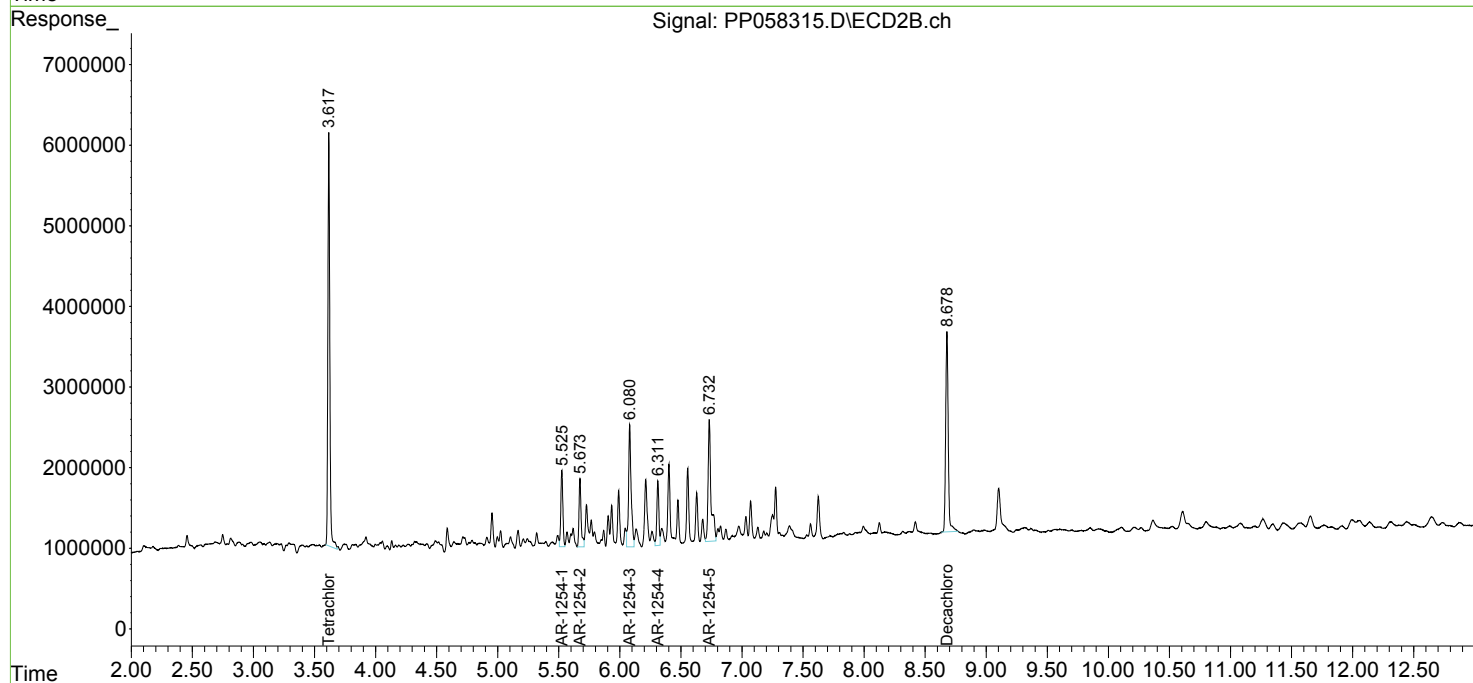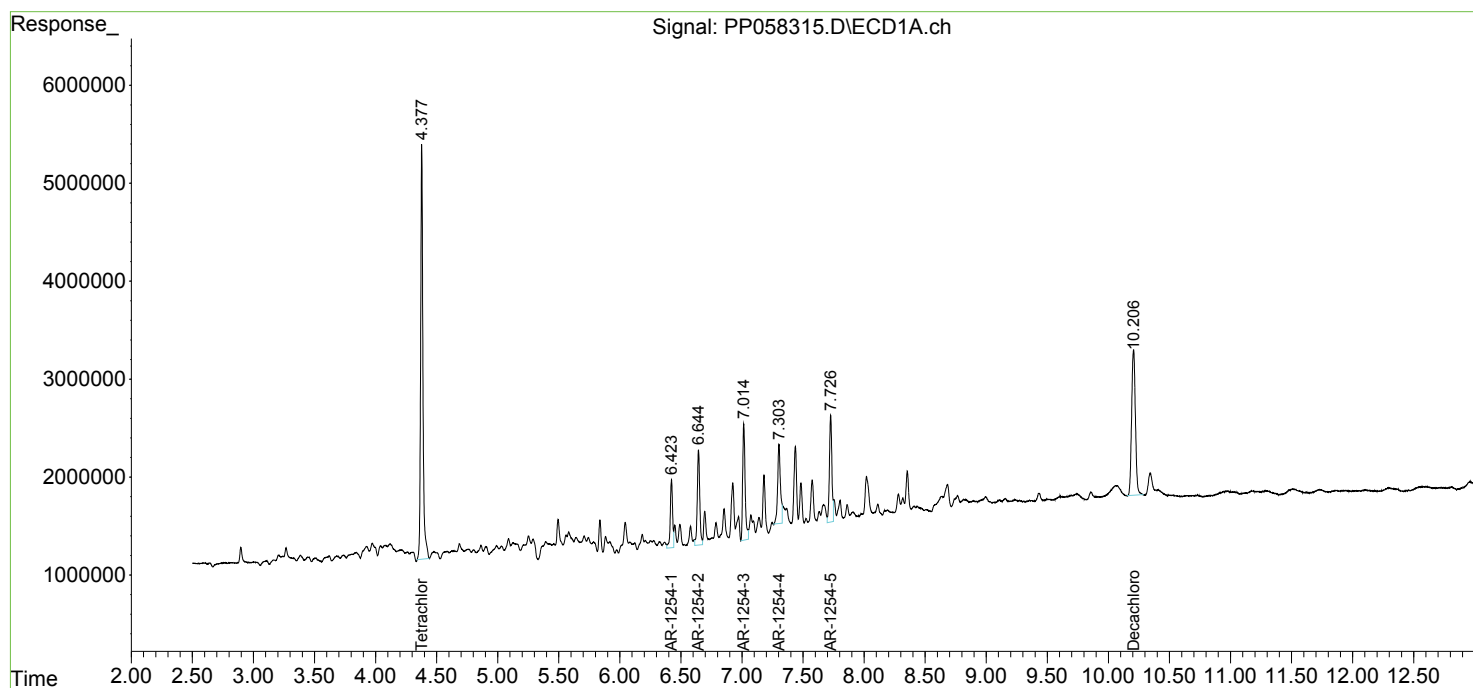

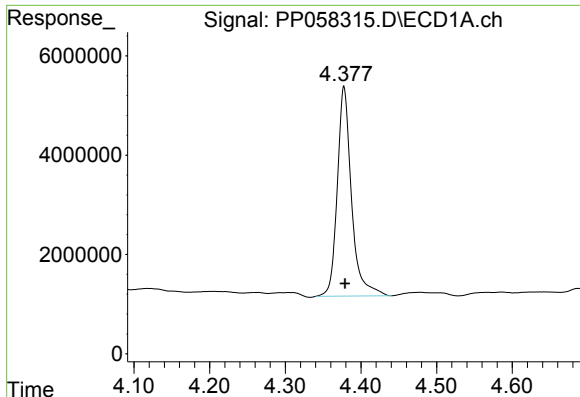


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: -0.001 min
Response: 55196547
Conc: 24.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

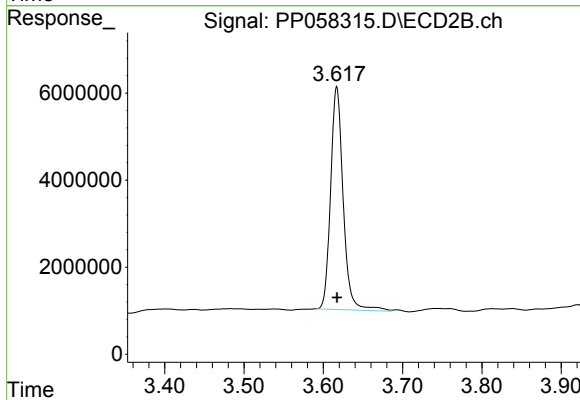


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 56415436
Conc: 26.15 ng/ml

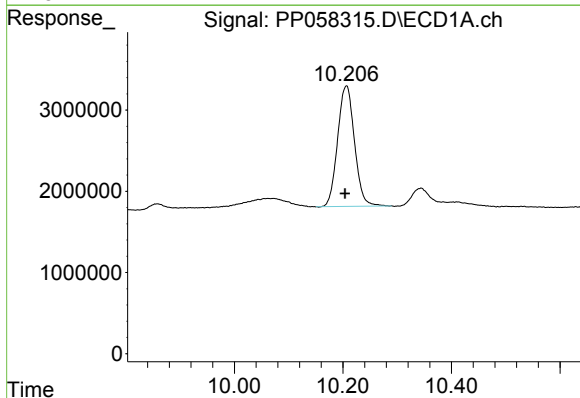


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: 0.002 min
Response: 32001055
Conc: 28.65 ng/ml

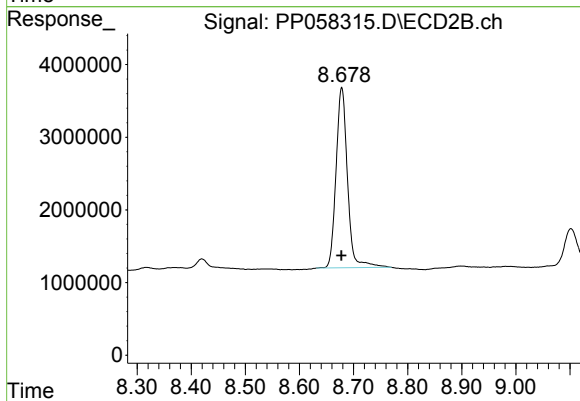

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: 0.000 min
Response: 36471044
Conc: 22.12 ng/ml

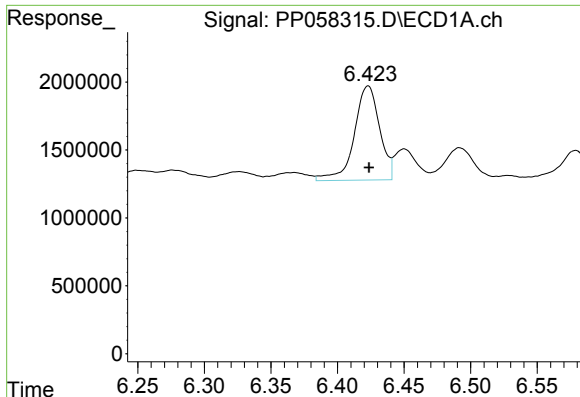


#26 AR-1254-1

R.T.: 6.423 min
Delta R.T.: 0.000 min
Response: 9183710
Conc: 125.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

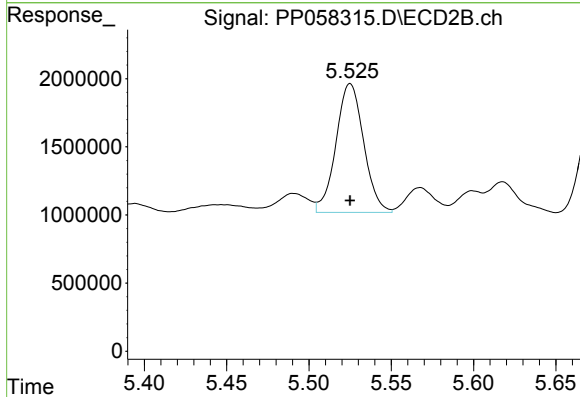


#26 AR-1254-1

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 11077258
Conc: 102.16 ng/ml

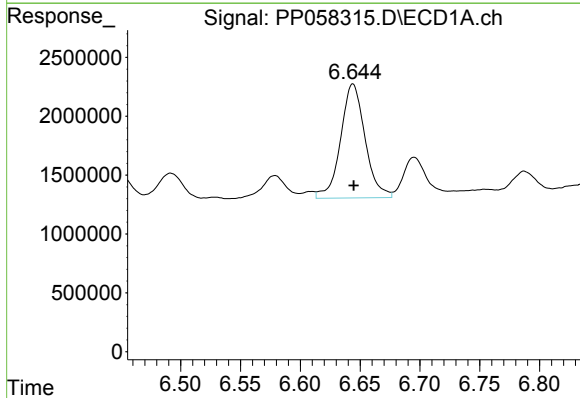


#27 AR-1254-2

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 13799647
Conc: 134.38 ng/ml

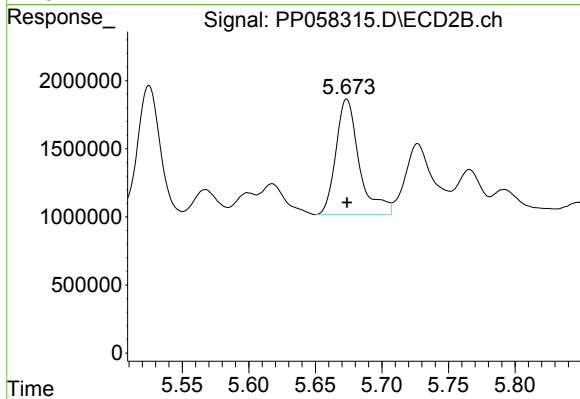

#27 AR-1254-2

R.T.: 5.674 min
Delta R.T.: 0.000 min
Response: 10384954
Conc: 106.98 ng/ml

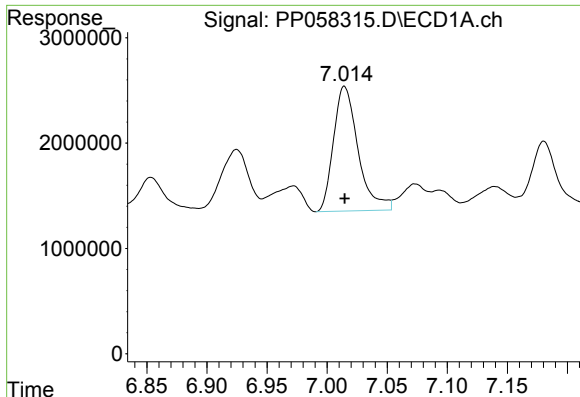


#28 AR-1254-3

R.T.: 7.014 min
Delta R.T.: 0.000 min
Response: 16882448
Conc: 171.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

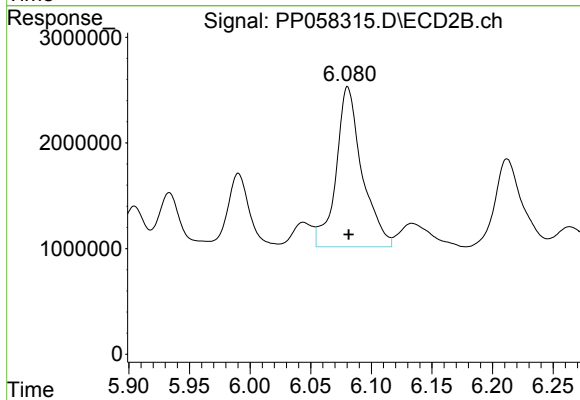


#28 AR-1254-3

R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 22561178
Conc: 145.71 ng/ml

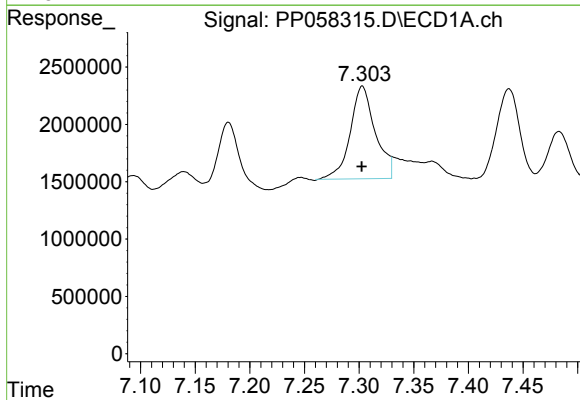


#29 AR-1254-4

R.T.: 7.303 min
Delta R.T.: 0.000 min
Response: 12903575
Conc: 194.46 ng/ml m

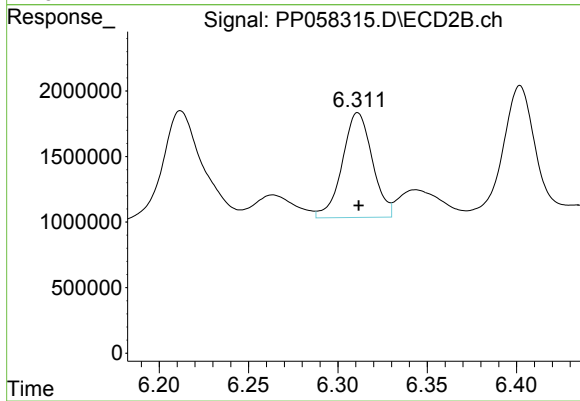

#29 AR-1254-4

R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 9350081
Conc: 99.64 ng/ml

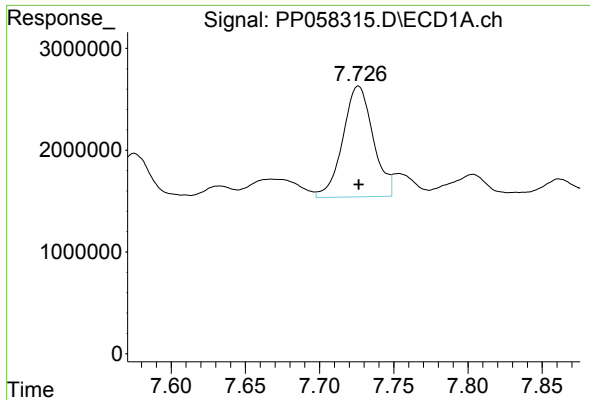


#30 AR-1254-5

R.T.: 7.726 min
Delta R.T.: 0.000 min
Response: 15480615
Conc: 211.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-04-5.0-7.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

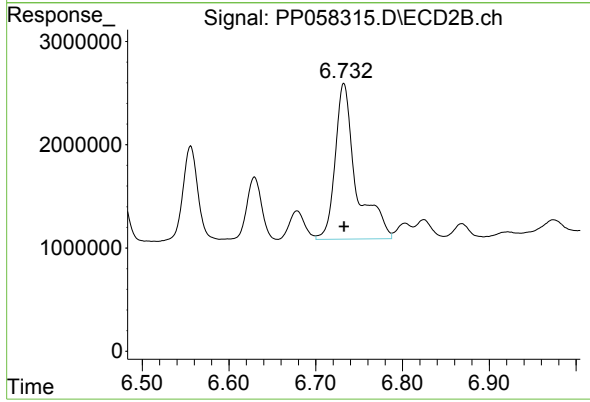

#30 AR-1254-5

R.T.: 6.732 min
Delta R.T.: 0.000 min
Response: 25511237
Conc: 175.51 ng/ml