

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
 Data File : PP058325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 17:43
 Operator : YP\AJ
 Sample : 03039-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MW-34

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 06 04:59:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.617	51498863	49474095	22.502	22.929
2) SA Decachlor...	10.204	8.677	24970289	27250271	22.354	16.528m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
Data File : PP058325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 17:43
Operator : YP\AJ
Sample : 03039-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MW-34


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 06 04:59:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

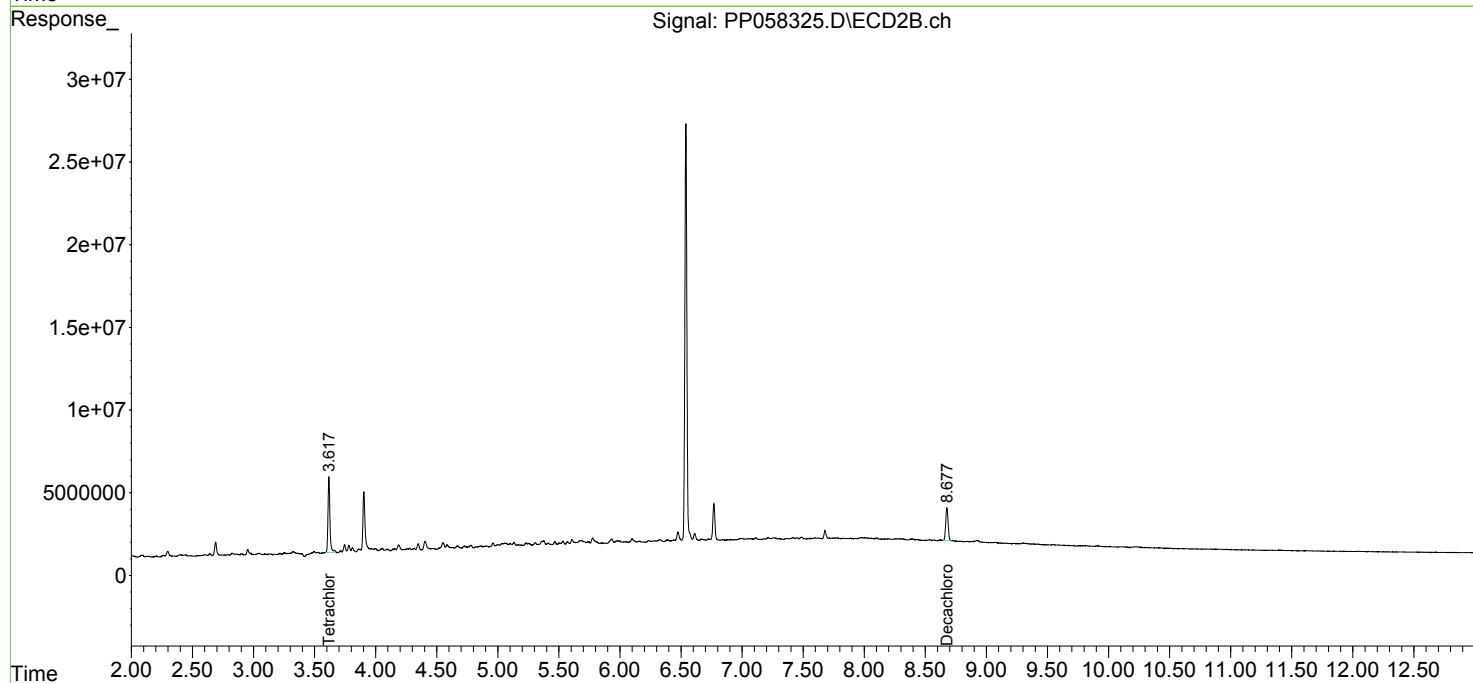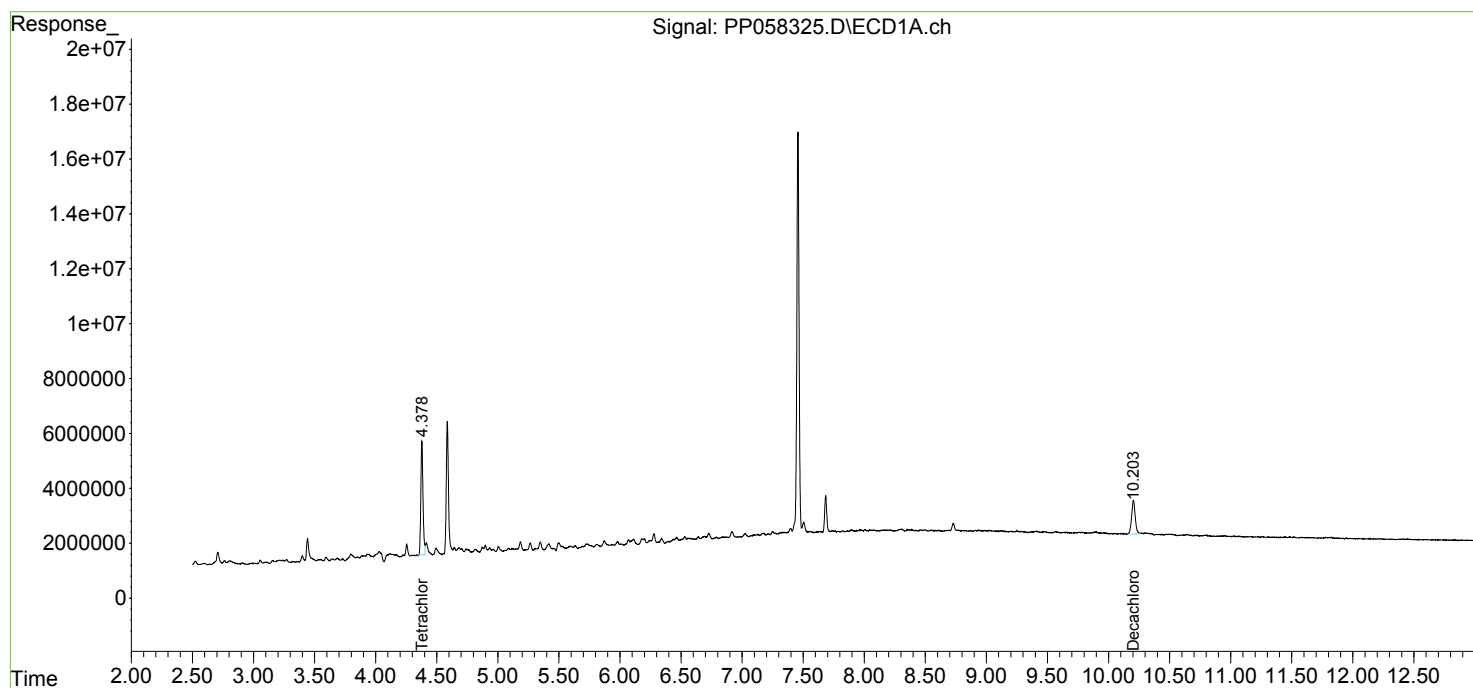

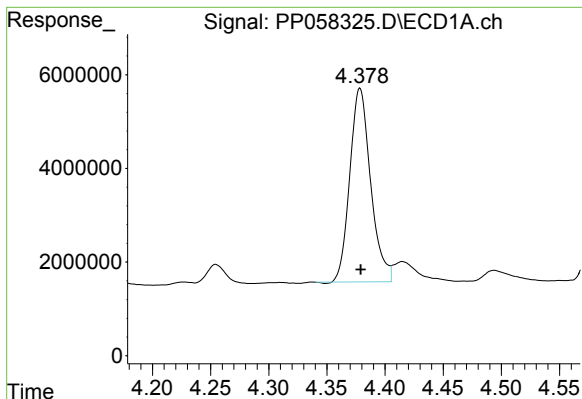


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 51498863
Conc: 22.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
MW-34


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

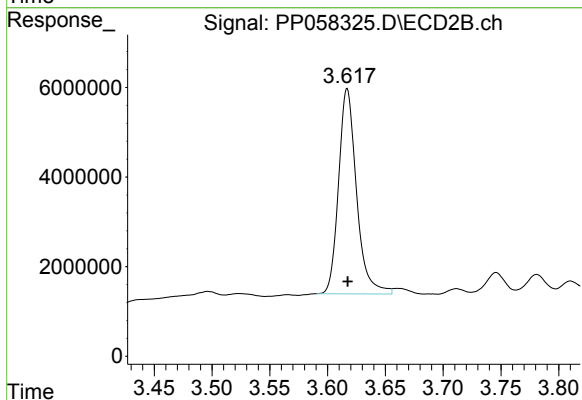


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 49474095
Conc: 22.93 ng/ml

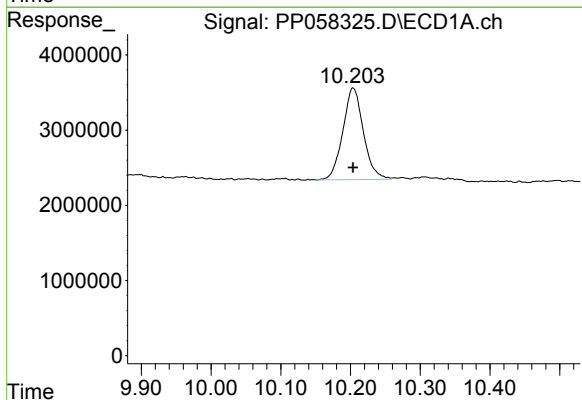

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: 0.000 min
Response: 24970289
Conc: 22.35 ng/ml

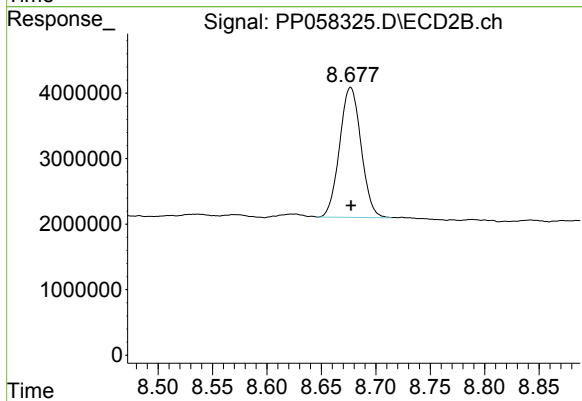

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: 0.000 min
Response: 27250271
Conc: 16.53 ng/ml m