

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
 Data File : PP058340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 22:11
 Operator : YP\AJ
 Sample : 03065-05 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC288060LOZ-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:48:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 06 04:59:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.617	5177720	4865169	2.262	2.255
2) SA Decachlor...	10.207	8.679	4140047	3586390	3.706	2.175m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060823\
Data File : PP058340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 22:11
Operator : YP\AJ
Sample : 03065-05 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC288060LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:48:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 06 04:59:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

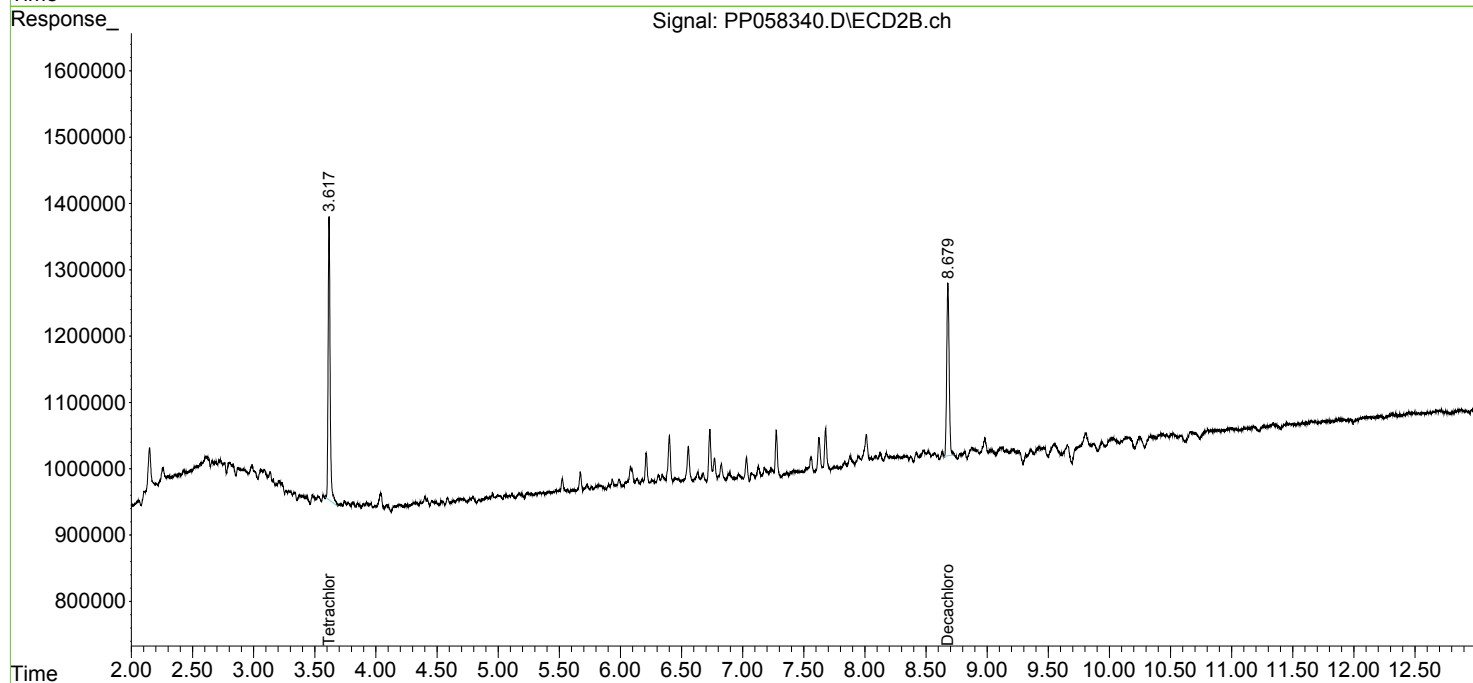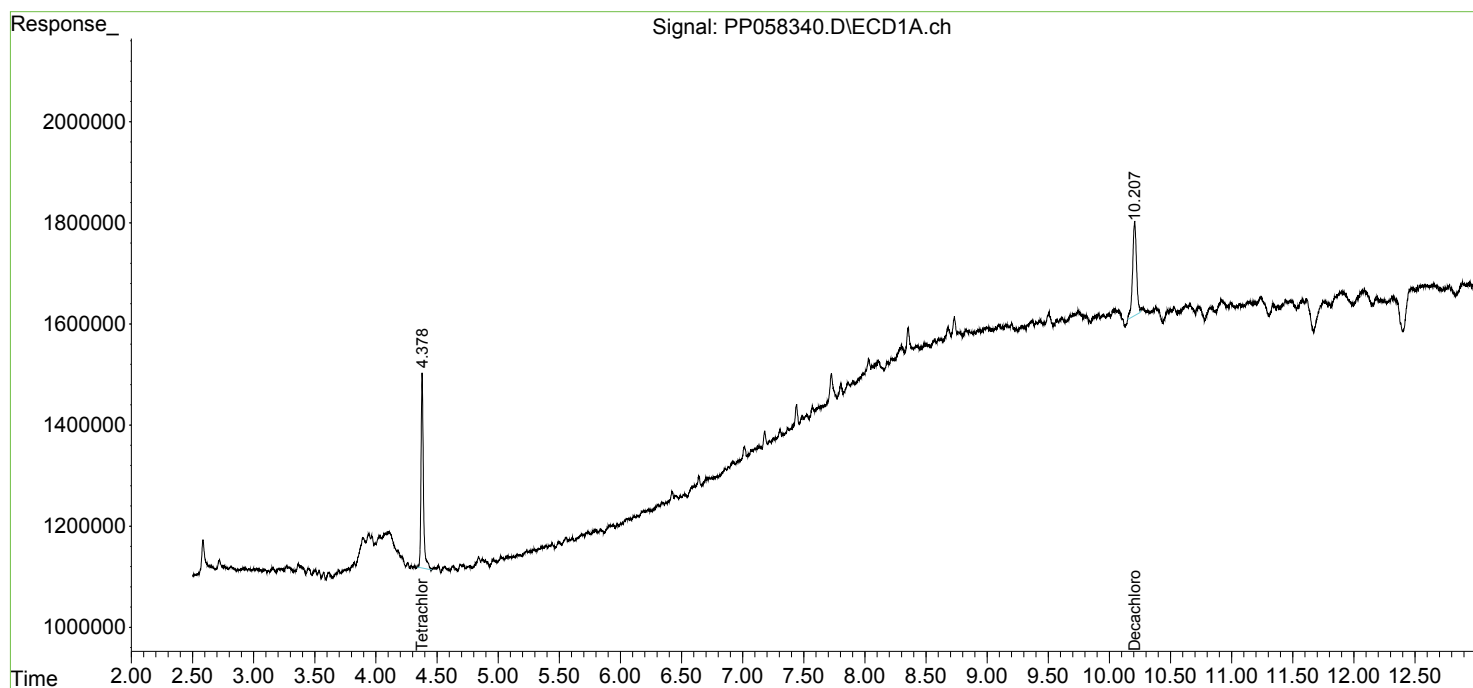

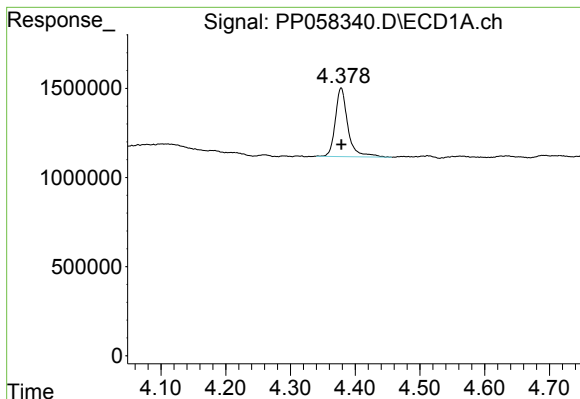


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 5177720
Conc: 2.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC288060LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

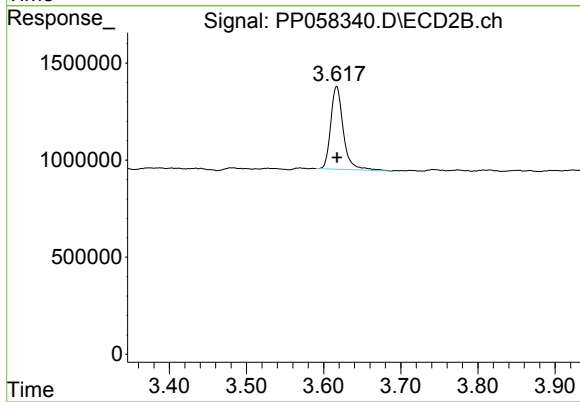


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 4865169
Conc: 2.25 ng/ml

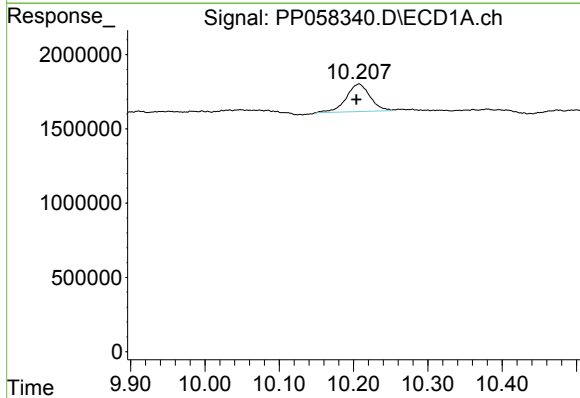

#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: 0.003 min
Response: 4140047
Conc: 3.71 ng/ml

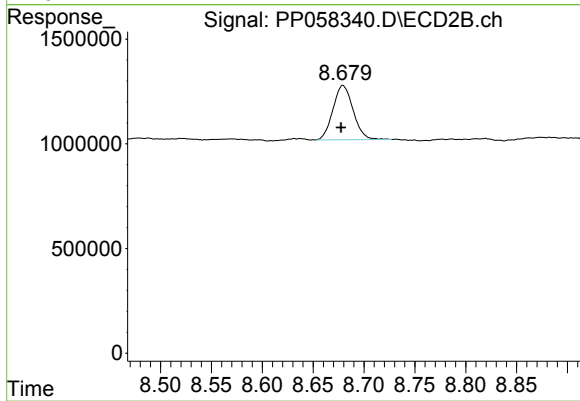

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: 0.001 min
Response: 3586390
Conc: 2.18 ng/ml m