

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060921\
 Data File : PP036299.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jun 2021 9:00
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 06:45:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	7.262	6.116f	6113	44207	6.413 68.312 #
24)	L5	AR-1248-4	7.209	0.000	134723	0	84.594 N.D. #
25)	L5	AR-1248-5	7.262	6.116f	6113	44207	3.916 50.270 #
26)	L6	AR-1254-1	7.209f	6.116f	134723	44207	83.156 33.829 #
28)	L6	AR-1254-3	7.831f	6.649f	36706	1164	13.914 0.612 #
29)	L6	AR-1254-4	8.091	0.000	7883	0	3.906 N.D. #
38)	L8	AR-1262-3	0.000	8.180	0	86116	N.D. 72.473 #
41)	L9	AR-1268-1	0.000	8.180	0	86116	N.D. 25.355 #
43)	L9	AR-1268-3	9.812f	0.000	4610	0	1.105 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060921\
Data File : PP036299.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jun 2021 9:00
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 06:45:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

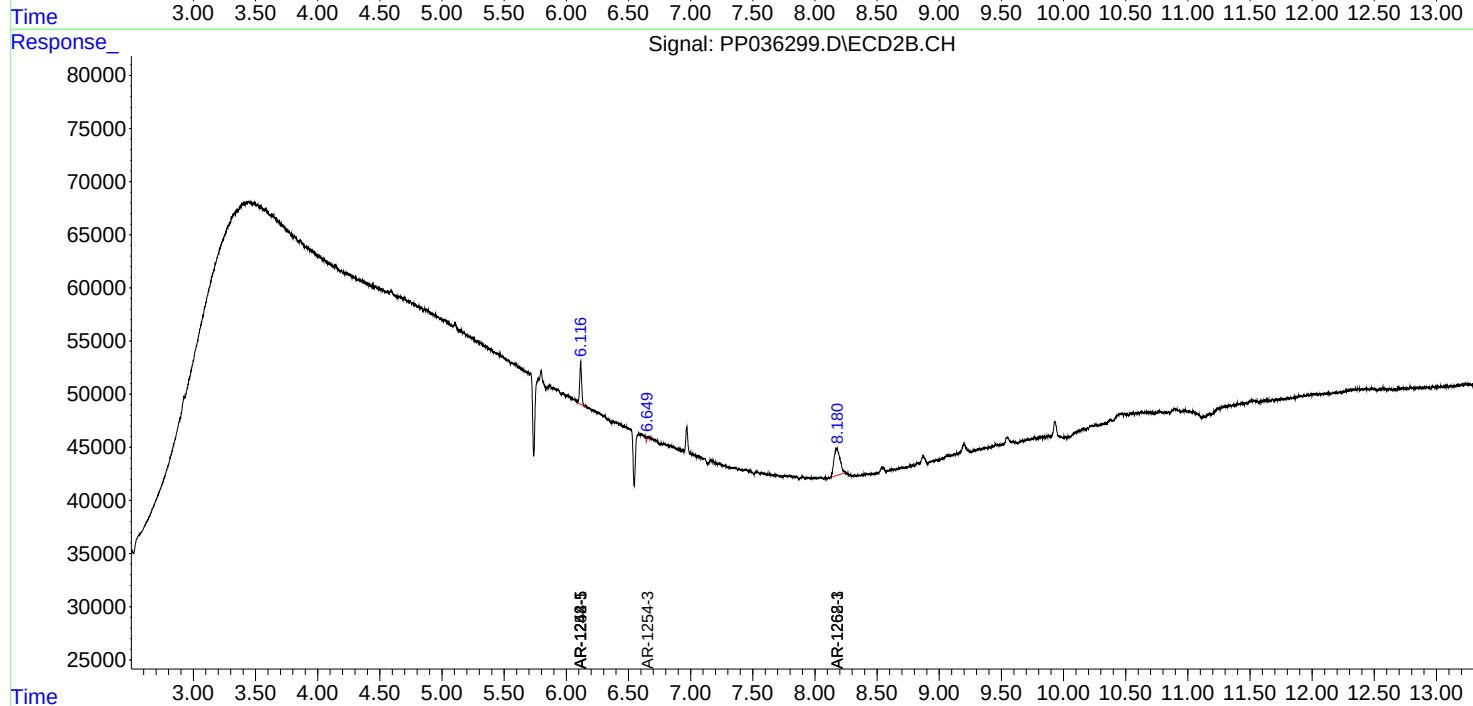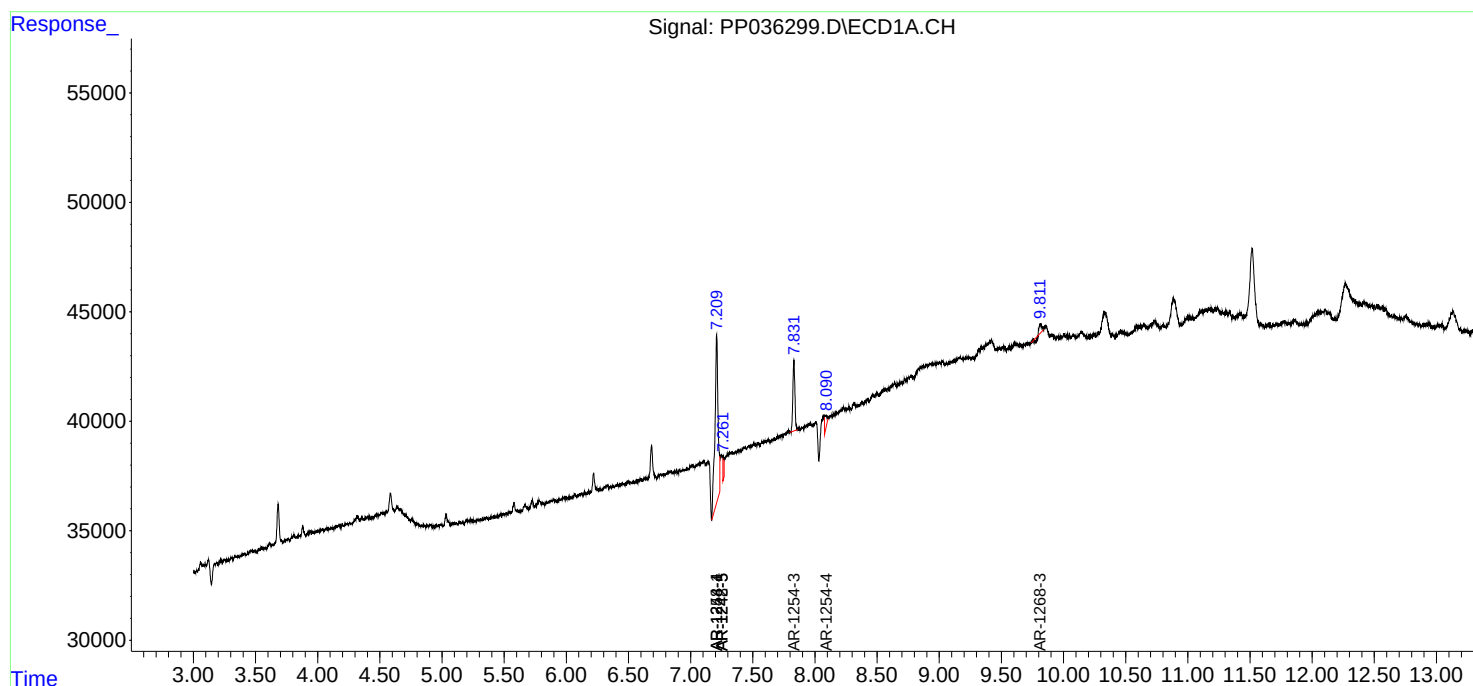


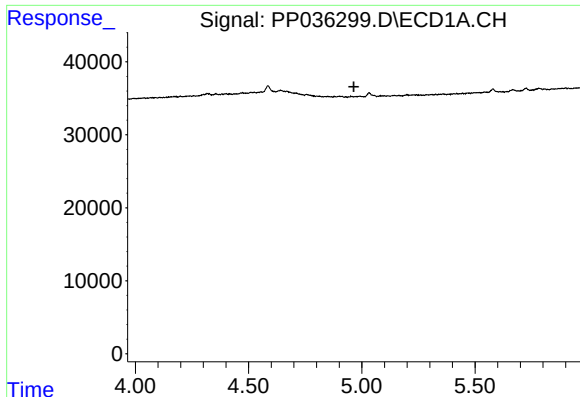

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

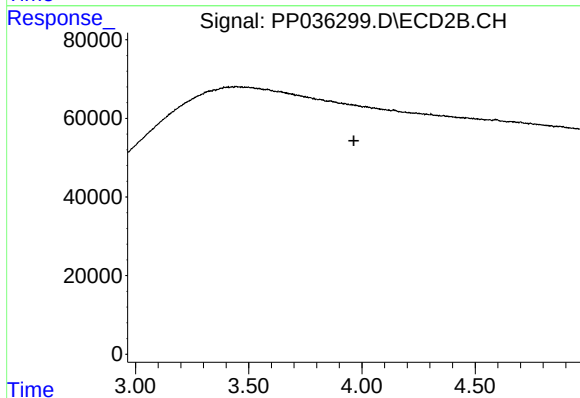


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.964 min
Response: 0
Conc: N.D.

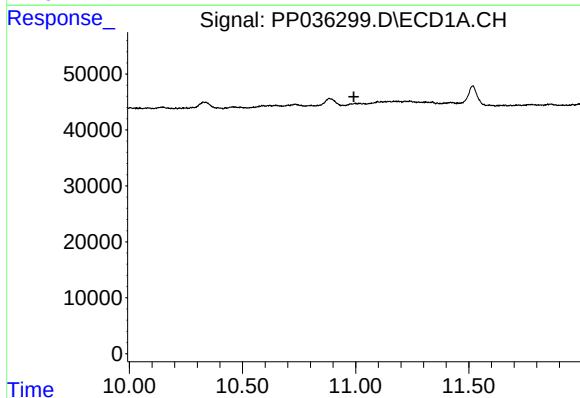


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.

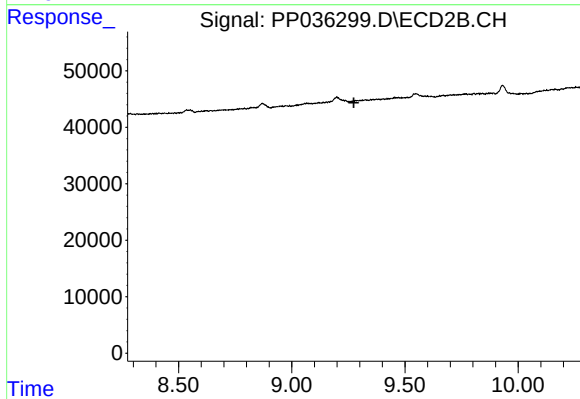

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

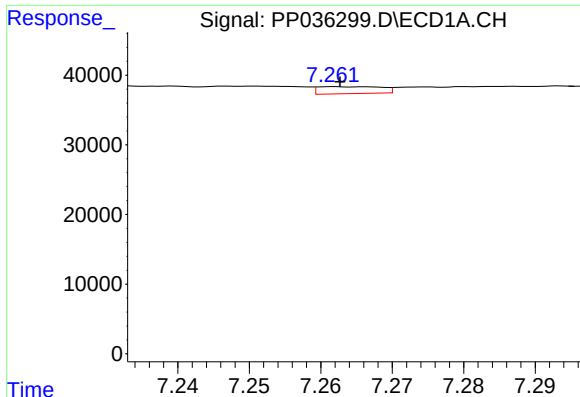

#20 AR-1242-5


R.T.: 7.262 min
Delta R.T.: 0.000 min
Response: 6113
Conc: 6.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

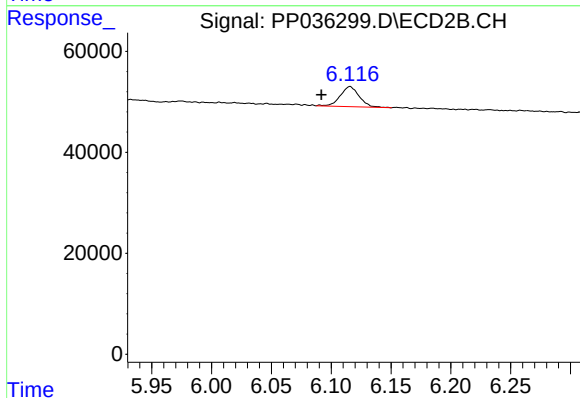


#20 AR-1242-5

R.T.: 6.116 min
Delta R.T.: 0.024 min
Response: 44207
Conc: 68.31 ng/ml

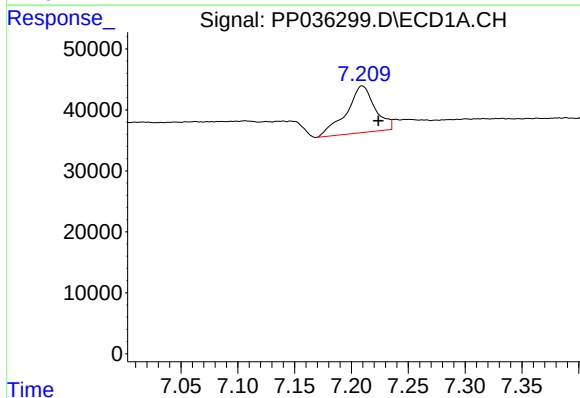


#24 AR-1248-4

R.T.: 7.209 min
Delta R.T.: -0.015 min
Response: 134723
Conc: 84.59 ng/ml

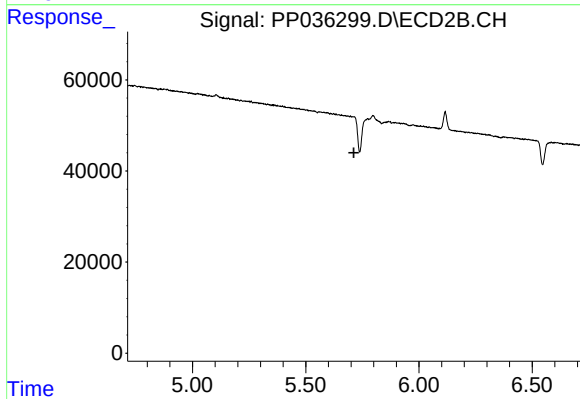

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.712 min
Response: 0
Conc: N.D.

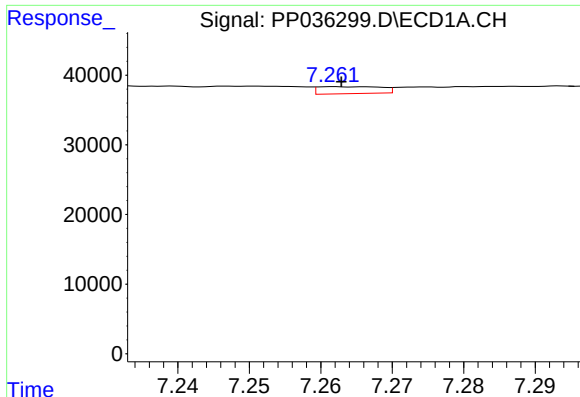

#25 AR-1248-5


R.T.: 7.262 min
Delta R.T.: 0.000 min
Response: 6113
Conc: 3.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

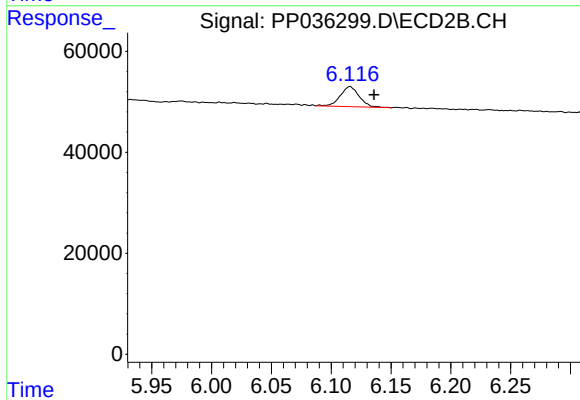


#25 AR-1248-5

R.T.: 6.116 min
Delta R.T.: -0.020 min
Response: 44207
Conc: 50.27 ng/ml

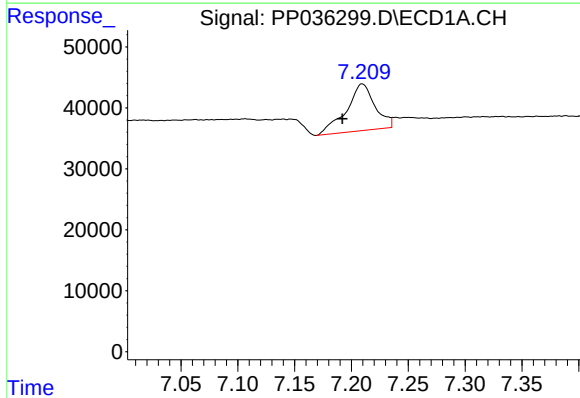


#26 AR-1254-1

R.T.: 7.209 min
Delta R.T.: 0.017 min
Response: 134723
Conc: 83.16 ng/ml

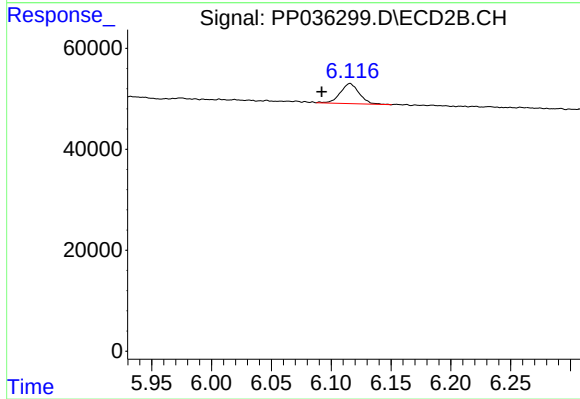

#26 AR-1254-1


R.T.: 6.116 min
Delta R.T.: 0.024 min
Response: 44207
Conc: 33.83 ng/ml

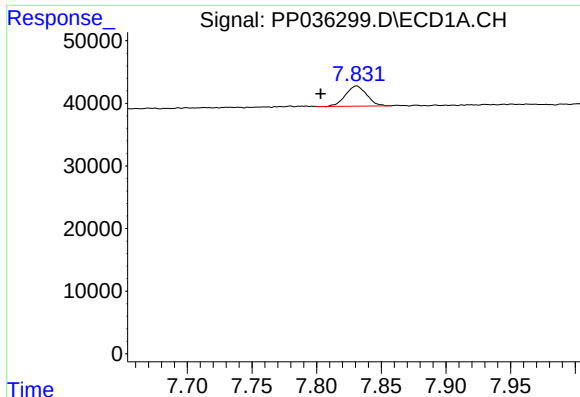

#28 AR-1254-3


R.T.: 7.831 min
Delta R.T.: 0.028 min
Response: 36706
Conc: 13.91 ng/ml

Instrument :
ECD_P
ClientSampleId :

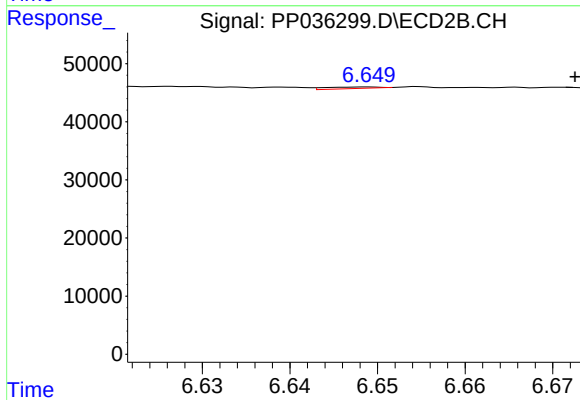


#28 AR-1254-3

R.T.: 6.649 min
Delta R.T.: -0.024 min
Response: 1164
Conc: 0.61 ng/ml

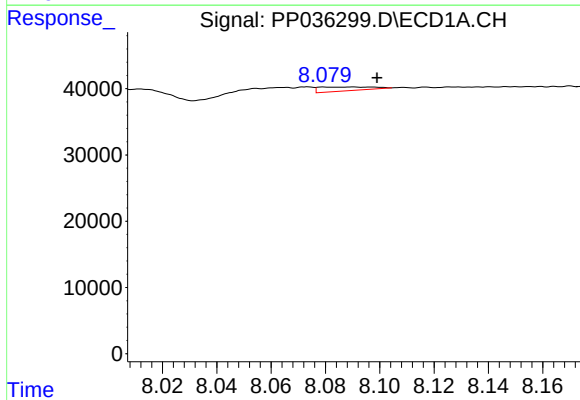


#29 AR-1254-4

R.T.: 8.091 min
Delta R.T.: -0.008 min
Response: 7883
Conc: 3.91 ng/ml

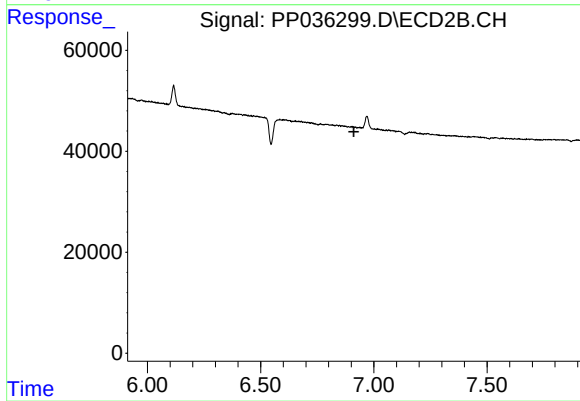

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 6.912 min
Response: 0
Conc: N.D.

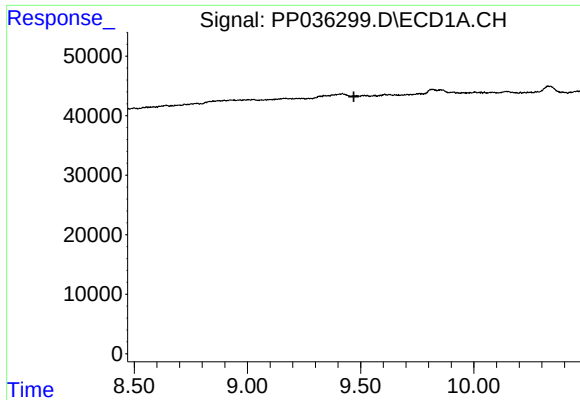

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

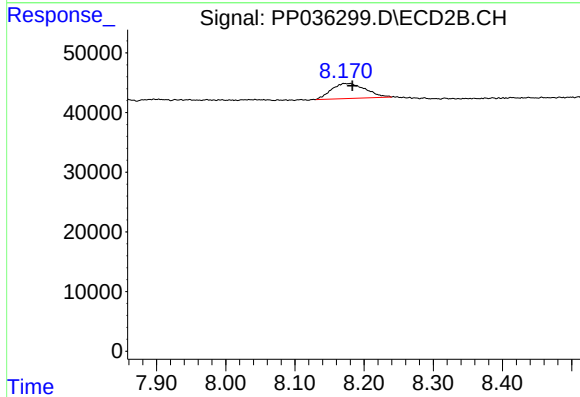


#38 AR-1262-3

R.T.: 8.180 min
Delta R.T.: -0.003 min
Response: 86116
Conc: 72.47 ng/ml

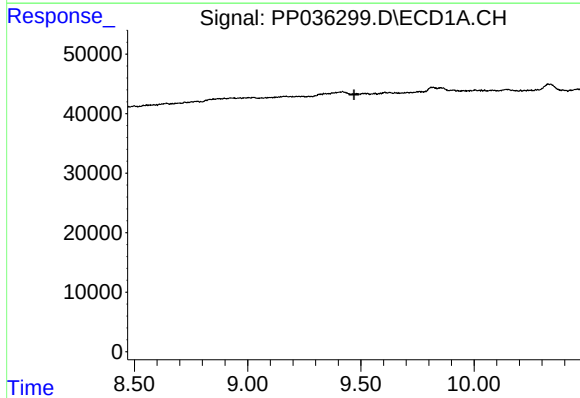


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

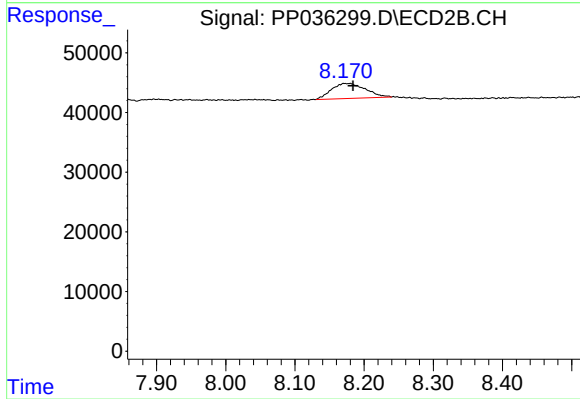

#41 AR-1268-1


R.T.: 8.180 min
Delta R.T.: -0.004 min
Response: 86116
Conc: 25.35 ng/ml

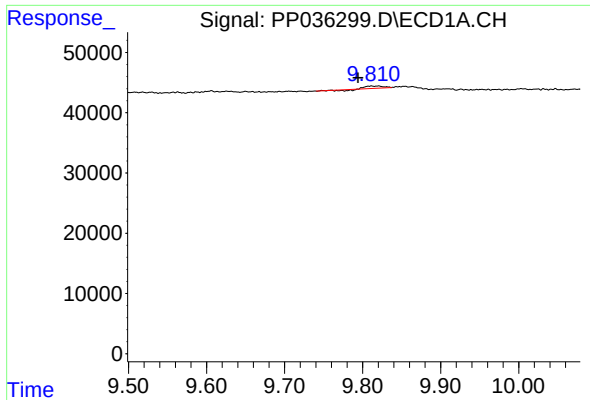

#43 AR-1268-3

R.T.: 9.812 min
Delta R.T.: 0.017 min
Response: 4610
Conc: 1.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

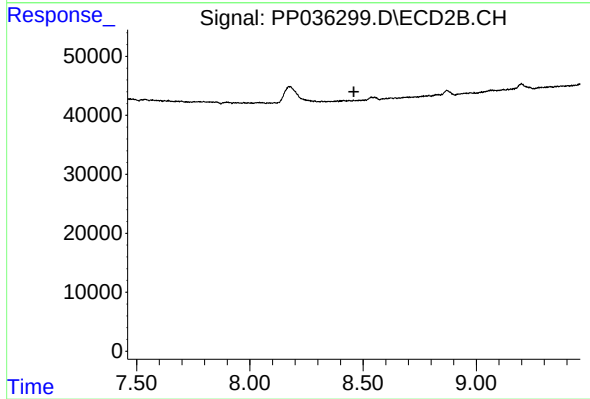

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.459 min
Response: 0
Conc: N.D.