

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060921\
 Data File : PP036309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jun 2021 14:20
 Operator : DD\AJ
 Sample : M2650-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DELAWANNA-RT10-STOCKPILE-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 06:49:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.960	1101313	743173	24.744	26.628
2) SA Decachlor...	10.994	9.266	1086789	676593	25.430	29.492

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060921\
Data File : PP036309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jun 2021 14:20
Operator : DD\AJ
Sample : M2650-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DELAWANNA-RT10-STOCKPILE-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 06:49:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

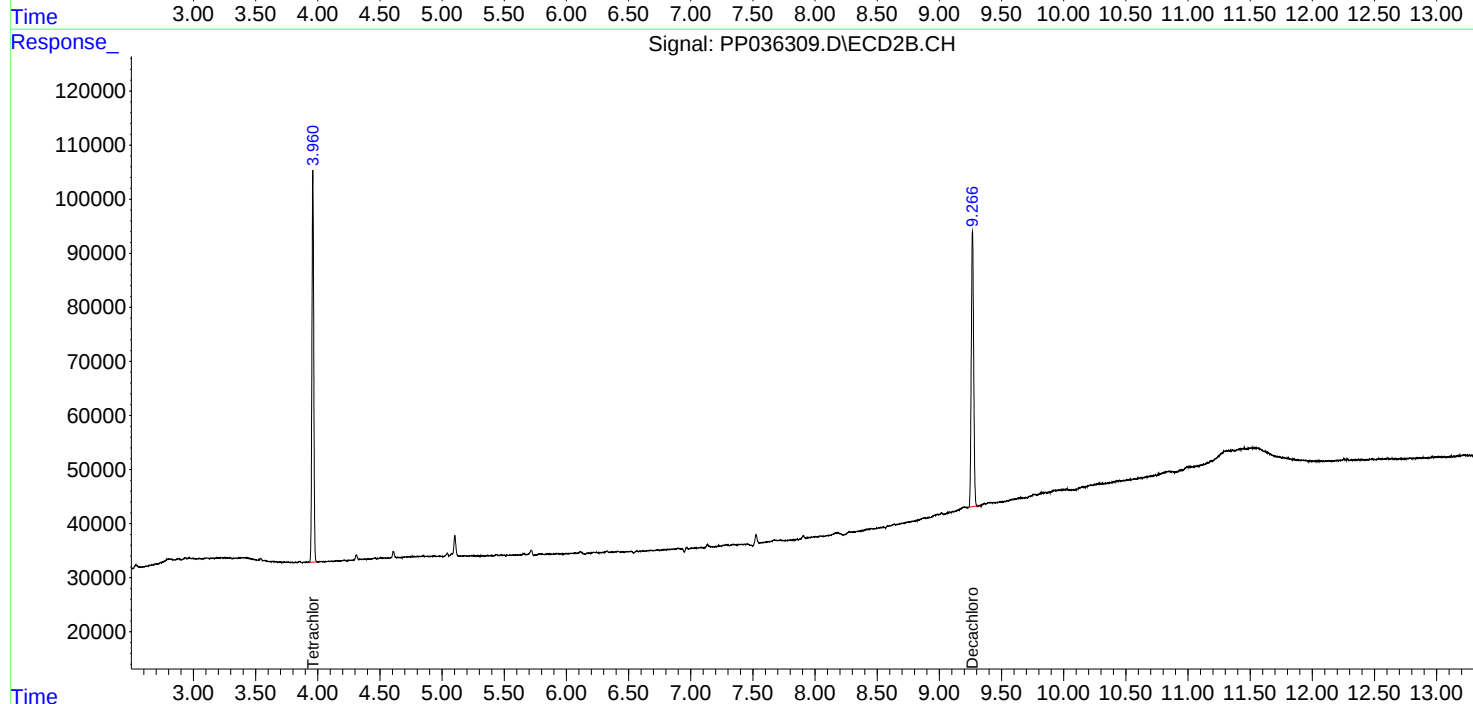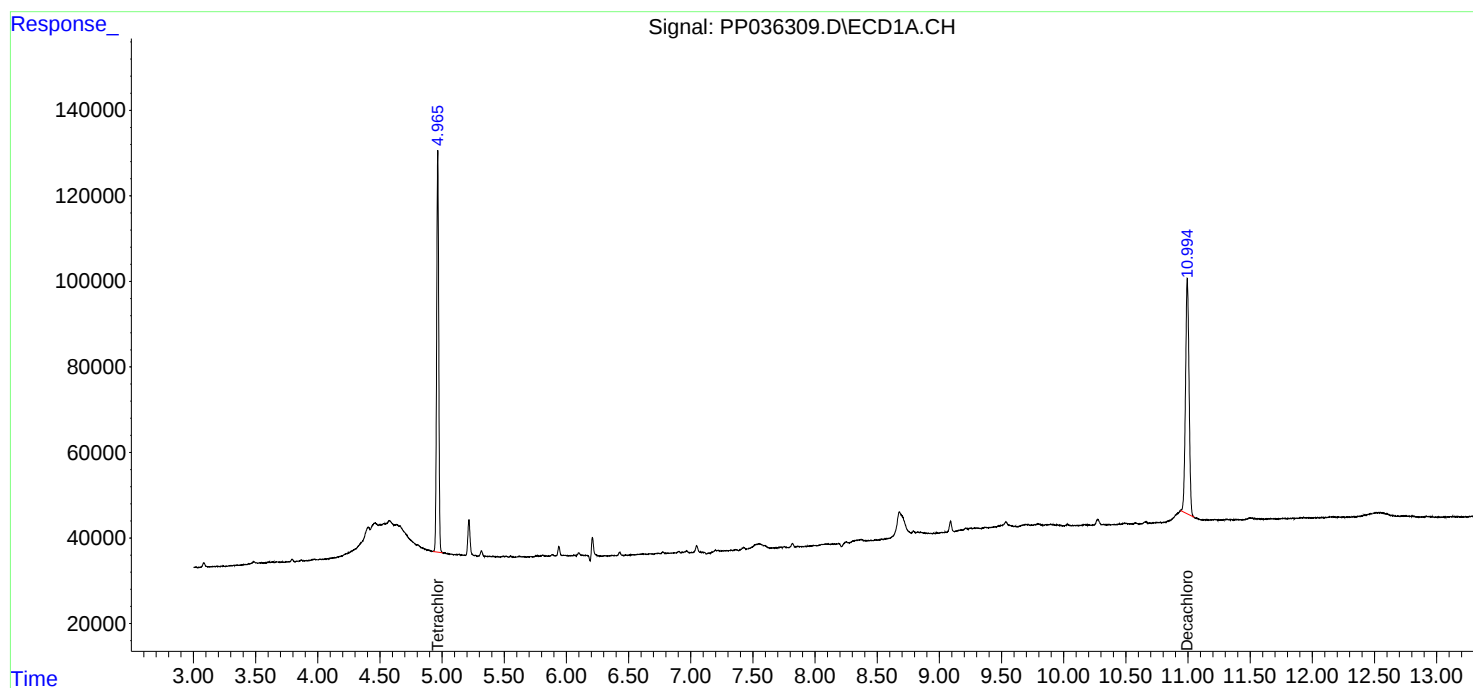


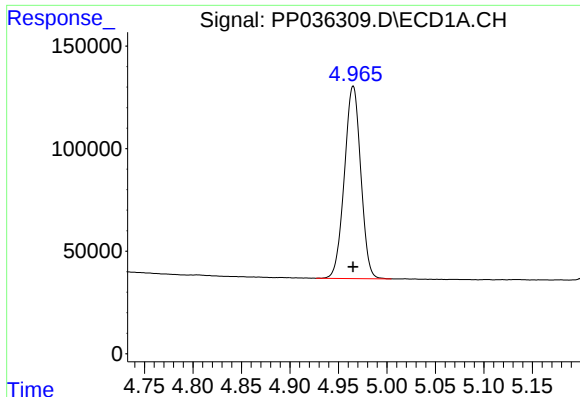

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 1101313
Conc: 24.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
DELAWANNA-RT10-STOCKPILE-3

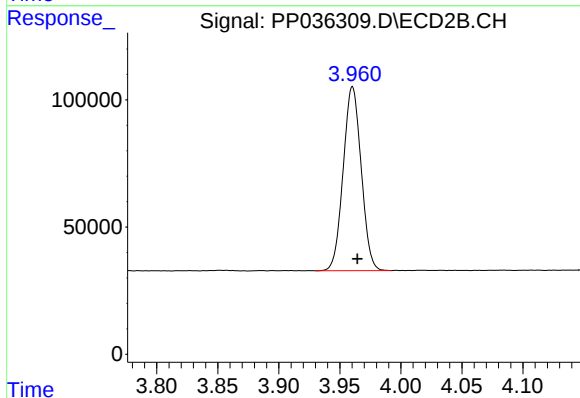


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.004 min
Response: 743173
Conc: 26.63 ng/ml

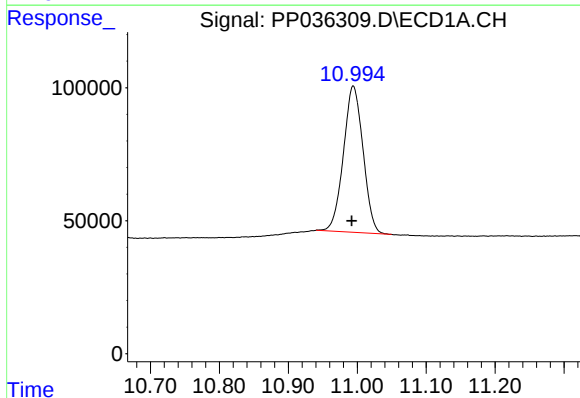

#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: 0.002 min
Response: 1086789
Conc: 25.43 ng/ml

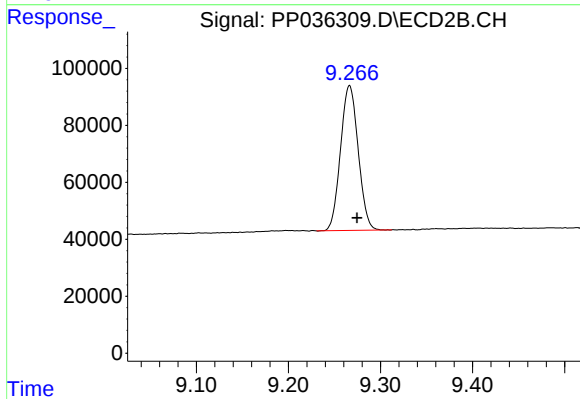

#2 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.008 min
Response: 676593
Conc: 29.49 ng/ml