

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060923\
 Data File : PP058384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2023 11:26
 Operator : YP\AJ
 Sample : 03051-02 (Sig #1); 03051-02RE (Sig #2)
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR-251580

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :Ankita Jodhani 06/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 11:52:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 06 04:59:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.618	54449685	56738297	23.791	26.296
2) SA Decachlor...	10.205	8.676	28245576	34928100	25.286	21.184m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060923\
Data File : PP058384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2023 11:26
Operator : YP\AJ
Sample : 03051-02 (Sig #1); 03051-02RE (Sig #2)
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR-251580


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Ankita Jodhani 06/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 11:52:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 06 04:59:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

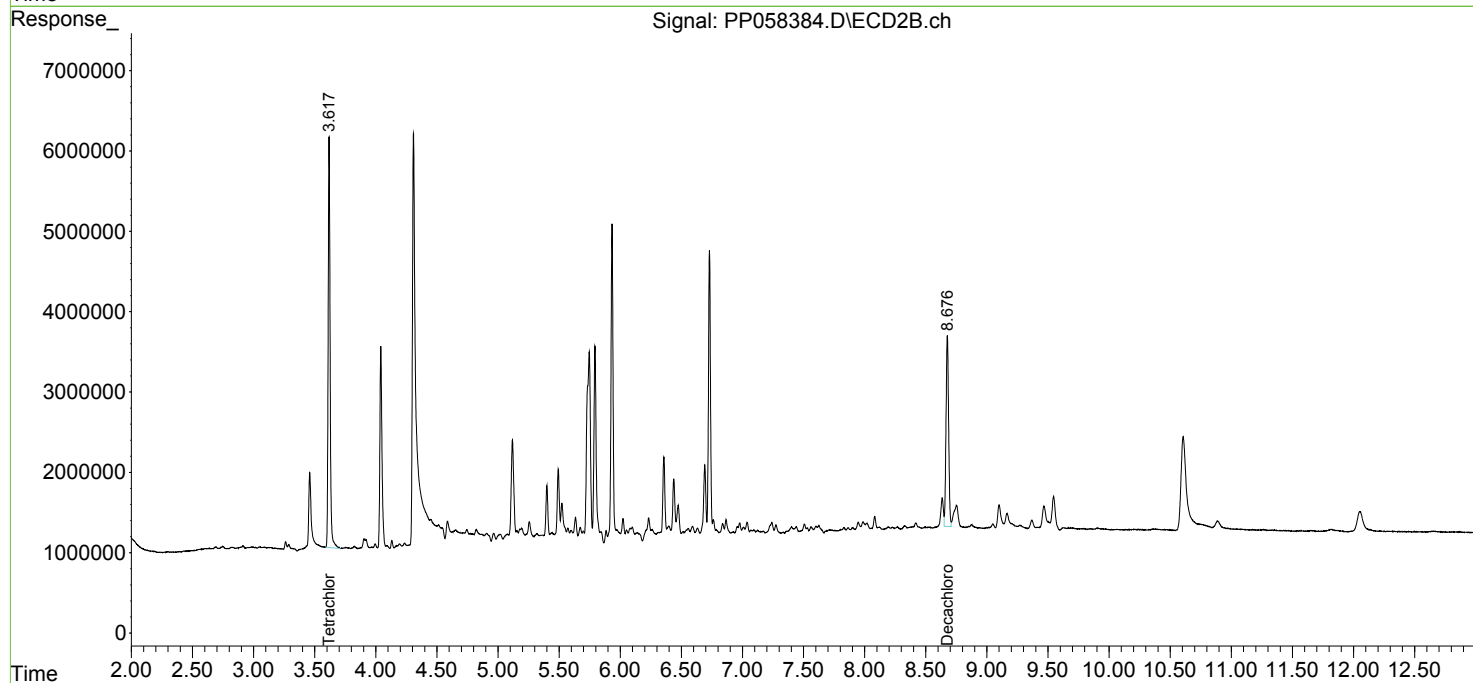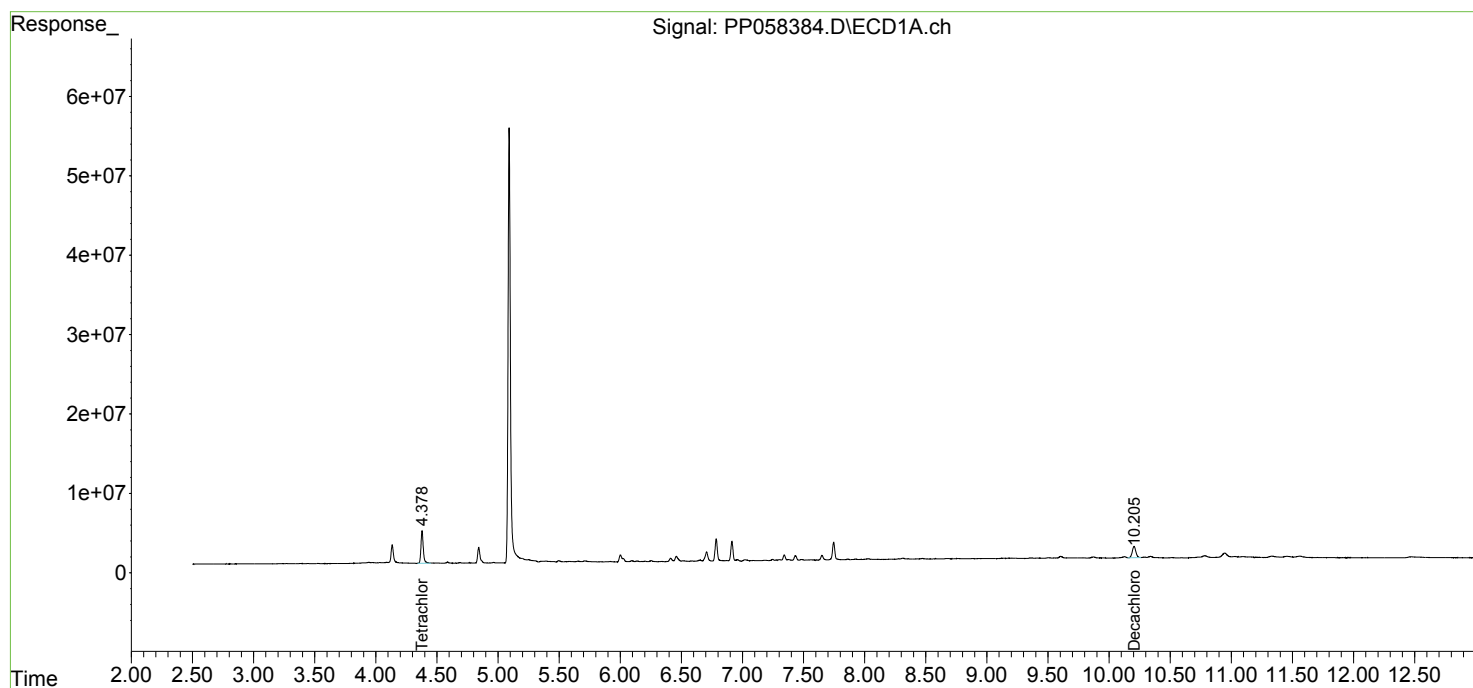

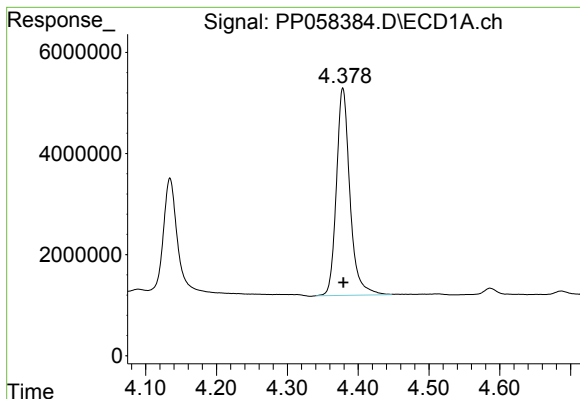

#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 54449685
Conc: 23.79 ng/ml

Instrument :

ECD_P


ClientSampleId :

RBR-251580

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Ankita Jodhani 06/09/2023

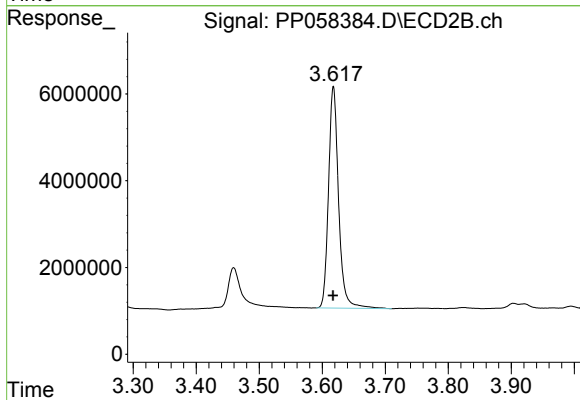


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: 0.000 min
Response: 56738297
Conc: 26.30 ng/ml

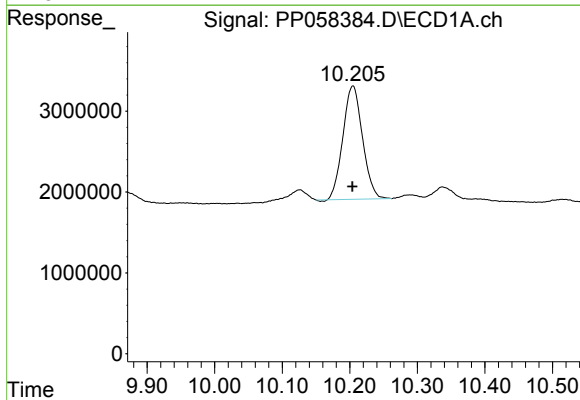

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.000 min
Response: 28245576
Conc: 25.29 ng/ml

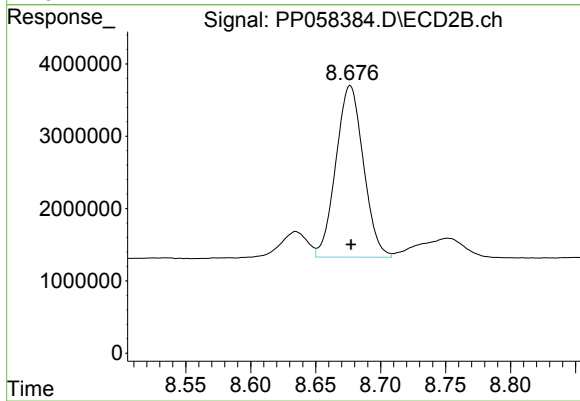

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.001 min
Response: 34928100
Conc: 21.18 ng/ml m