

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060923\
 Data File : PP058386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2023 11:59
 Operator : YP\AJ
 Sample : 03047-09RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MW-41RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :Ankita Jodhani 06/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 21:28:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 06 04:59:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.378	3.617	29812505	26731157	13.026m	12.389m
2) SA Decachlor...	10.205	8.675	11838936	11003779	10.599	6.674m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060923\
Data File : PP058386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2023 11:59
Operator : YP\AJ
Sample : 03047-09RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MW-41RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Ankita Jodhani 06/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 21:28:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060623.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 06 04:59:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

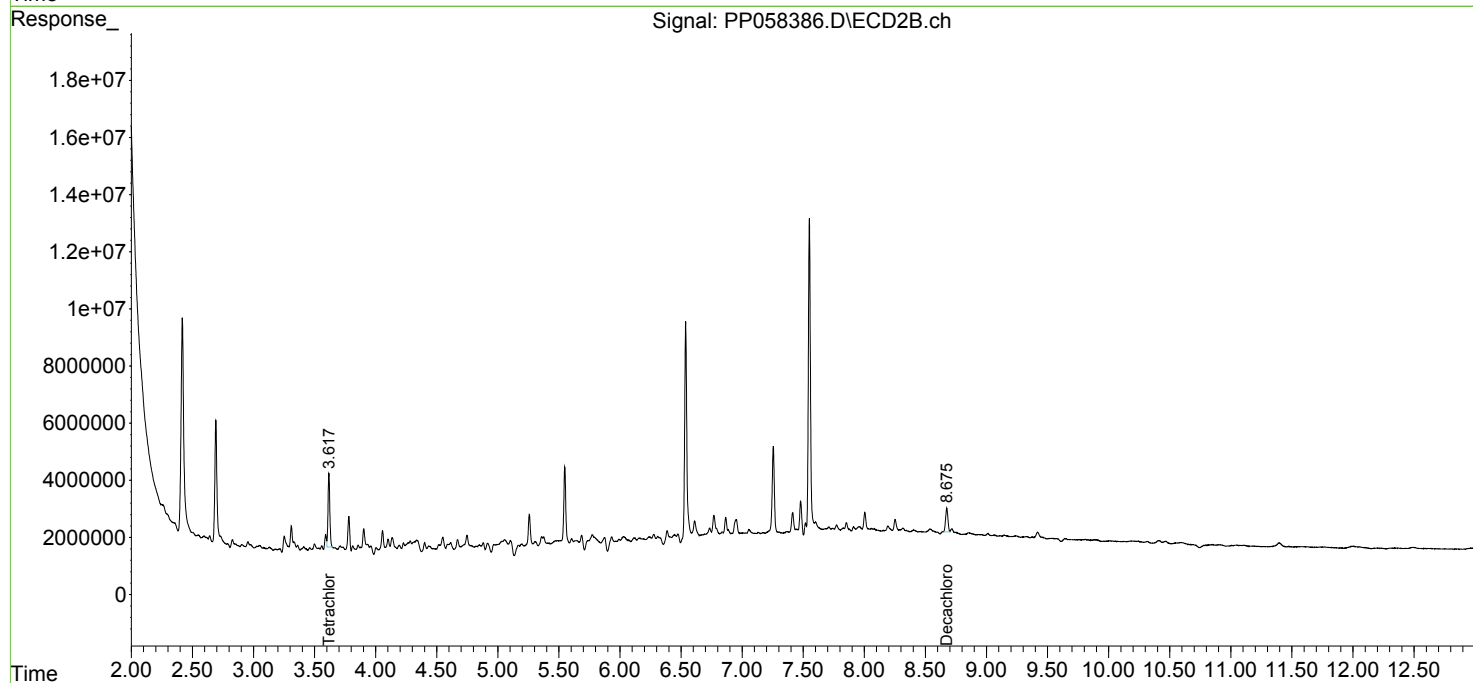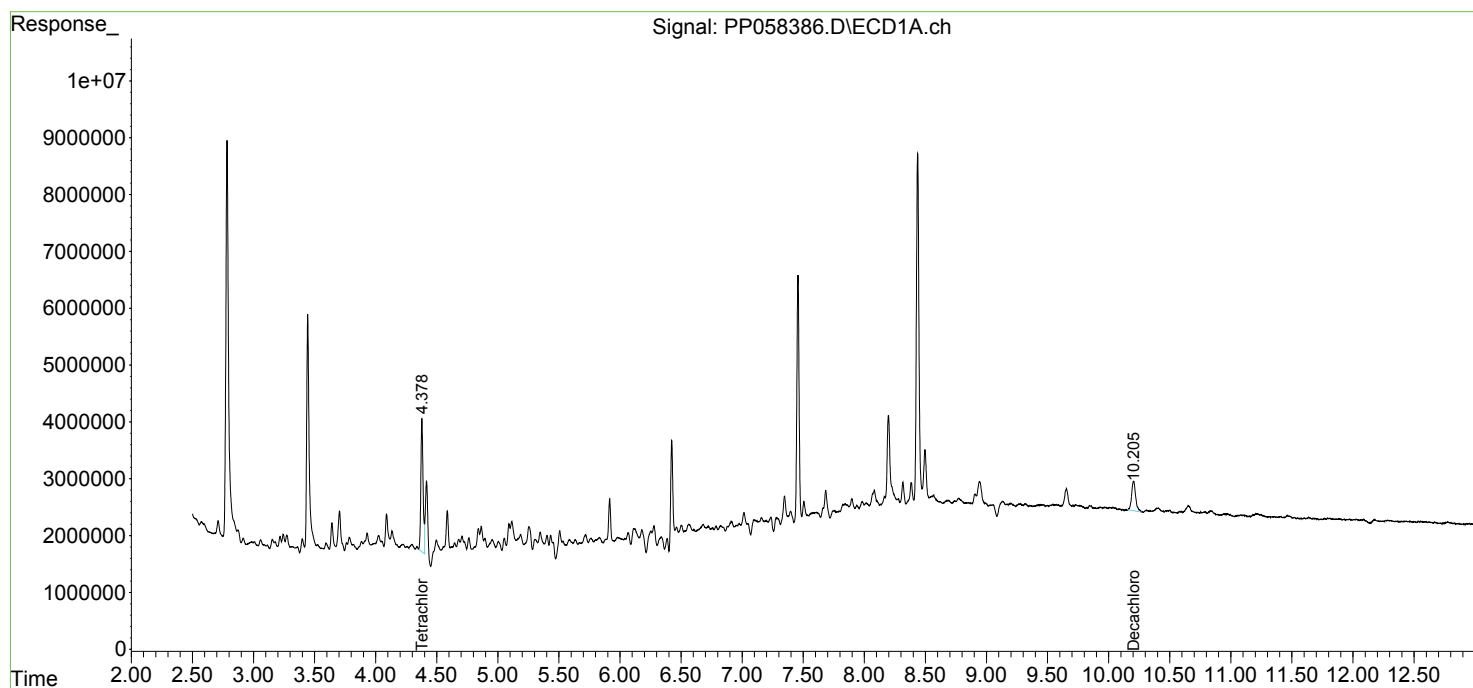

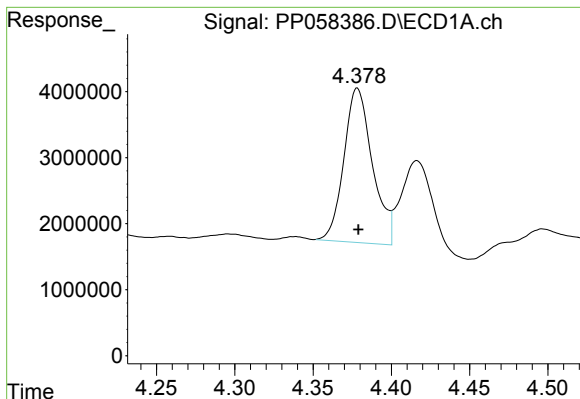


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: -0.001 min
Response: 29812505
Conc: 13.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MW-41RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Ankita Jodhani 06/09/2023

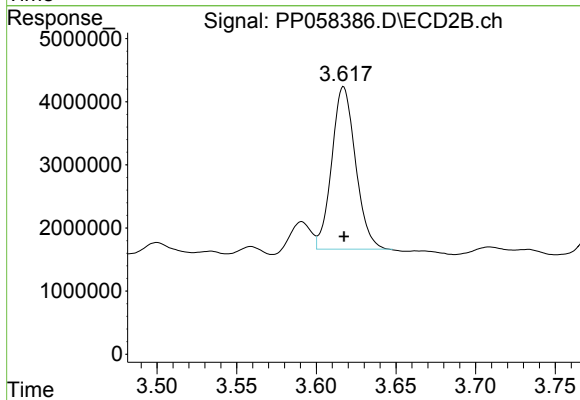


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 26731157
Conc: 12.39 ng/ml m

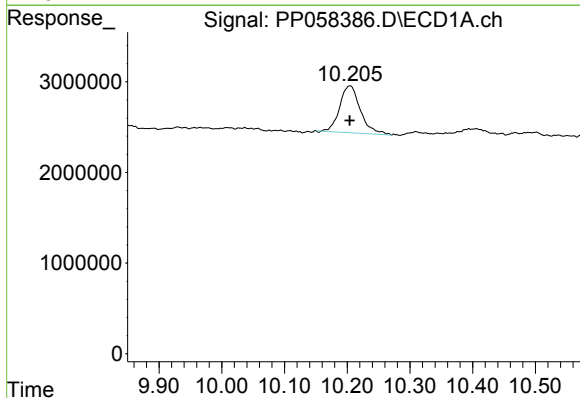

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.000 min
Response: 11838936
Conc: 10.60 ng/ml

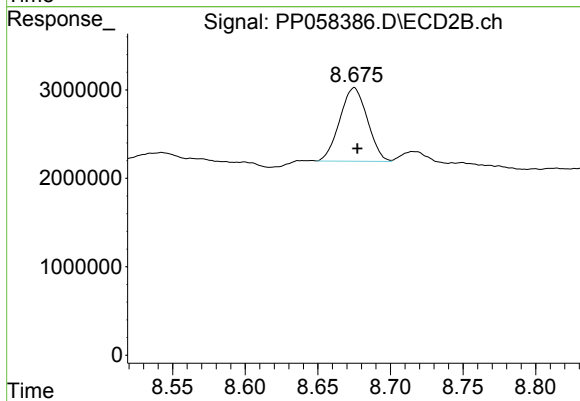

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.002 min
Response: 11003779
Conc: 6.67 ng/ml m