

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061022\
 Data File : PP048636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 13:59
 Operator : YP\AJ
 Sample : N3246-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 17156

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2022
 Supervised By :Ankita Jodhani 06/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:52:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.045	3.215	36908978	30933849	15.403m	16.252m
2) SA Decachlor...	10.385	8.615	40666787	26520122	21.336	21.657

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061022\
Data File : PP048636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 13:59
Operator : YP\AJ
Sample : N3246-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
17156


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2022
Supervised By :Ankita Jodhani 06/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:52:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

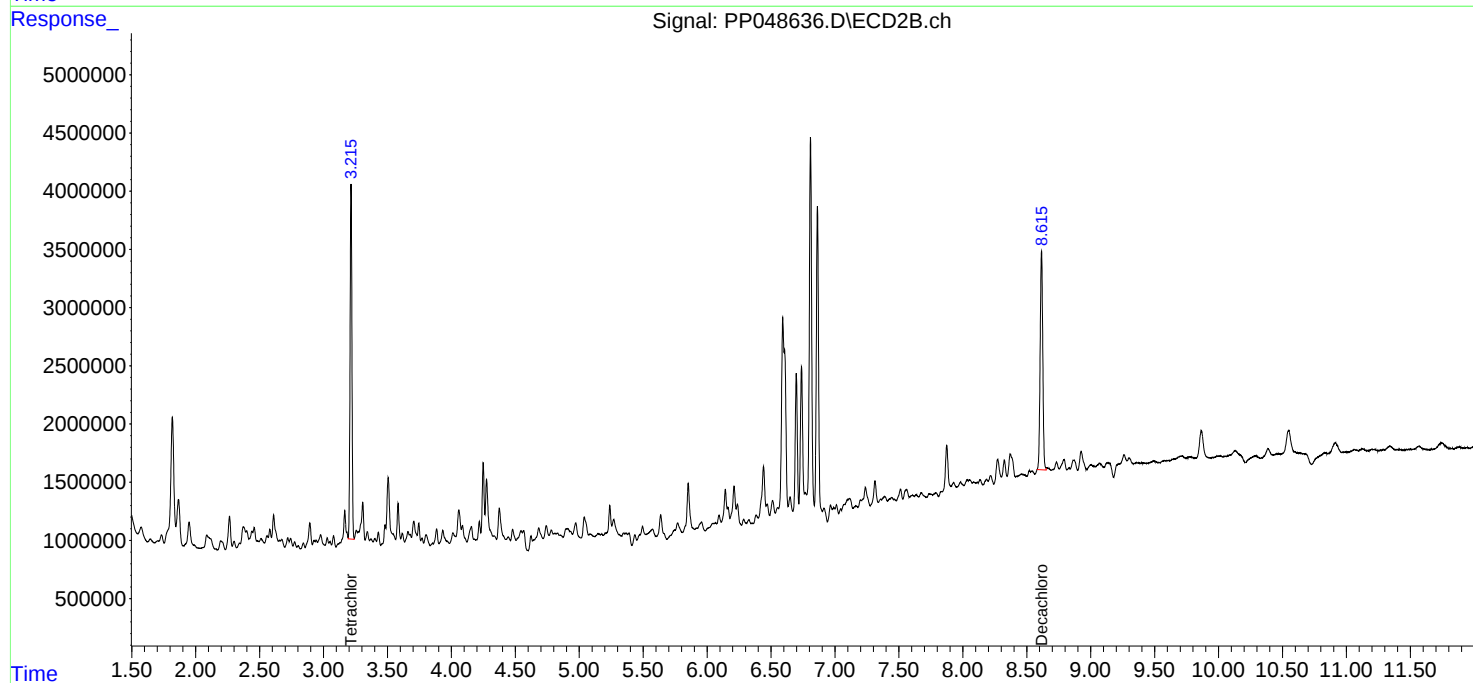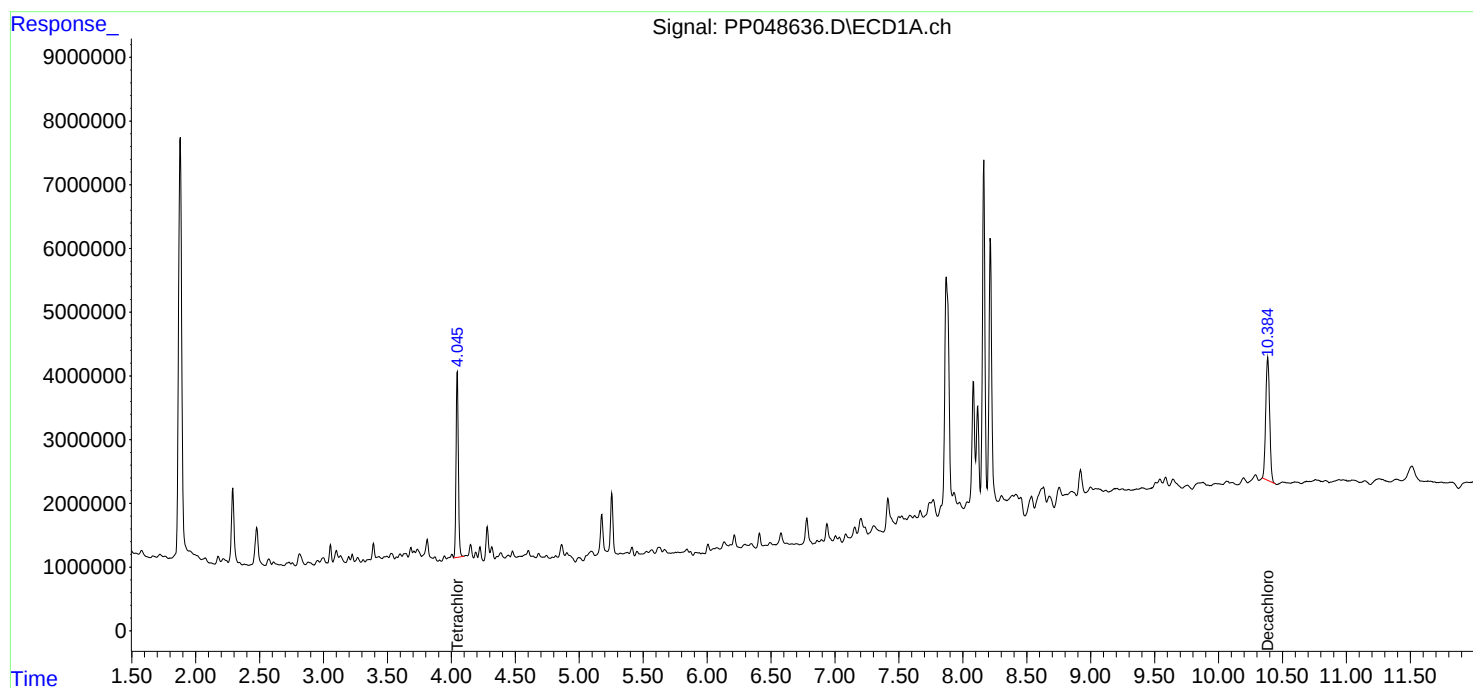

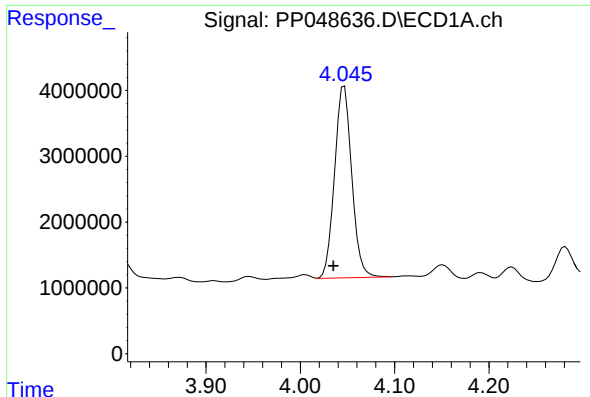


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.010 min
Response: 36908978
Conc: 15.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
17156


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2022
Supervised By :Ankita Jodhani 06/10/2022

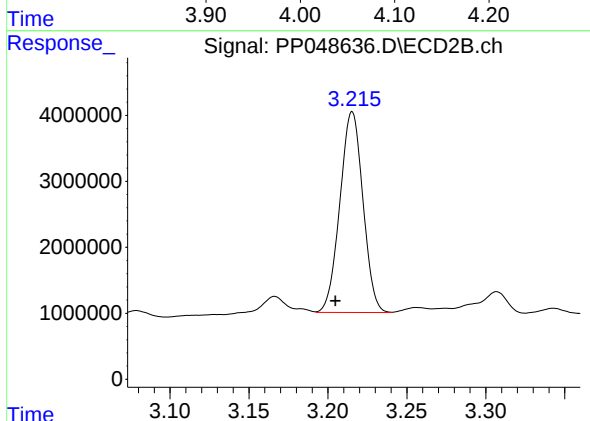


#1 Tetrachloro-m-xylene

R.T.: 3.215 min
Delta R.T.: 0.010 min
Response: 30933849
Conc: 16.25 ng/ml m

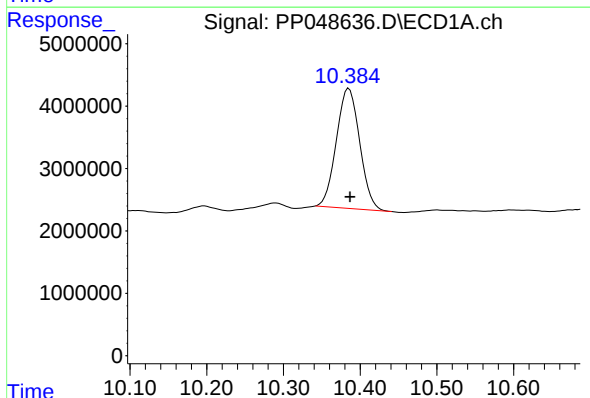

#2 Decachlorobiphenyl

R.T.: 10.385 min
Delta R.T.: -0.002 min
Response: 40666787
Conc: 21.34 ng/ml

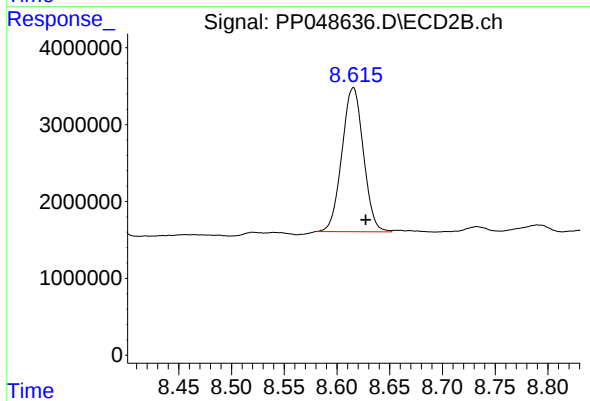

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: -0.012 min
Response: 26520122
Conc: 21.66 ng/ml