

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061022\
 Data File : PP048659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 20:13
 Operator : YP\AJ
 Sample : N3245-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SOM-2022-35A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2022
 Supervised By :Ankita Jodhani 06/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 03:15:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.037	3.202	4551065	4467500	1.899	2.347
2) SA Decachlor...	10.388	8.616	4082910	2503349	2.142	2.044m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061022\
Data File : PP048659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 20:13
Operator : YP\AJ
Sample : N3245-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SOM-2022-35A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2022
Supervised By :Ankita Jodhani 06/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 03:15:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

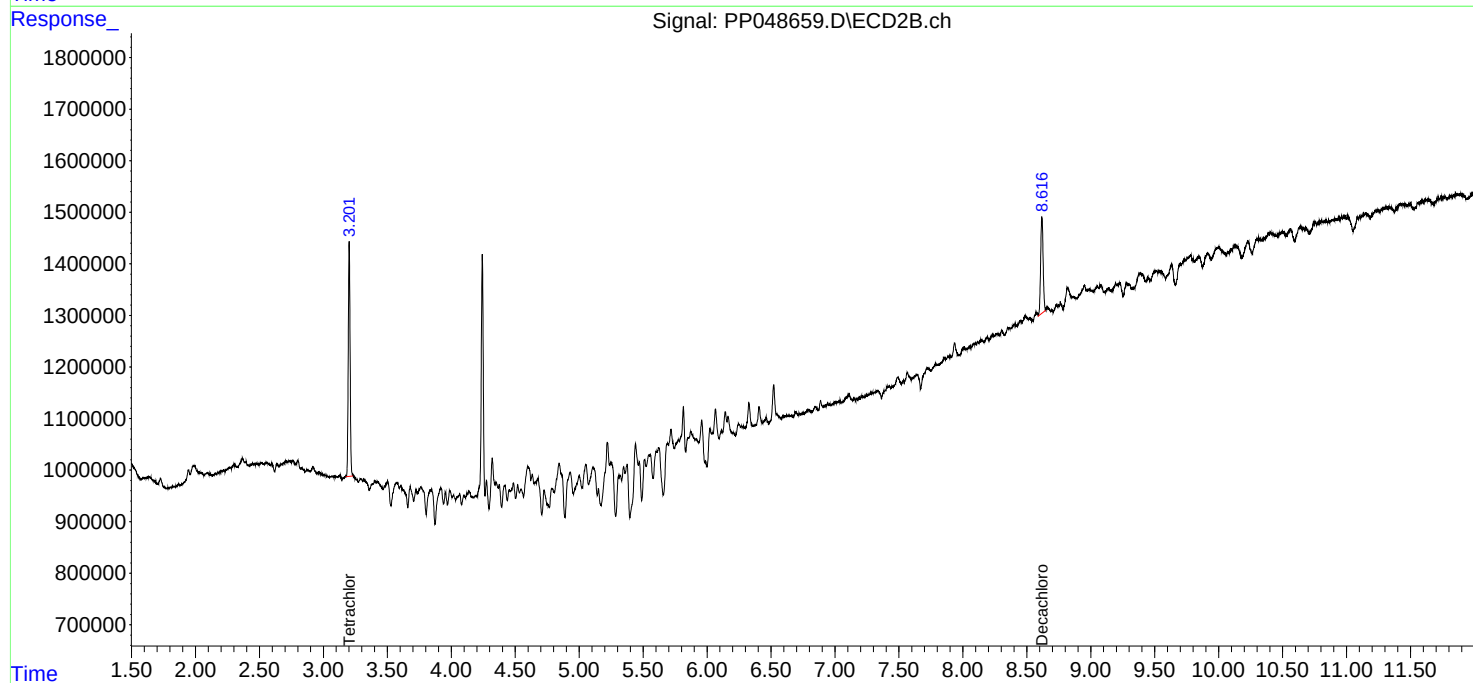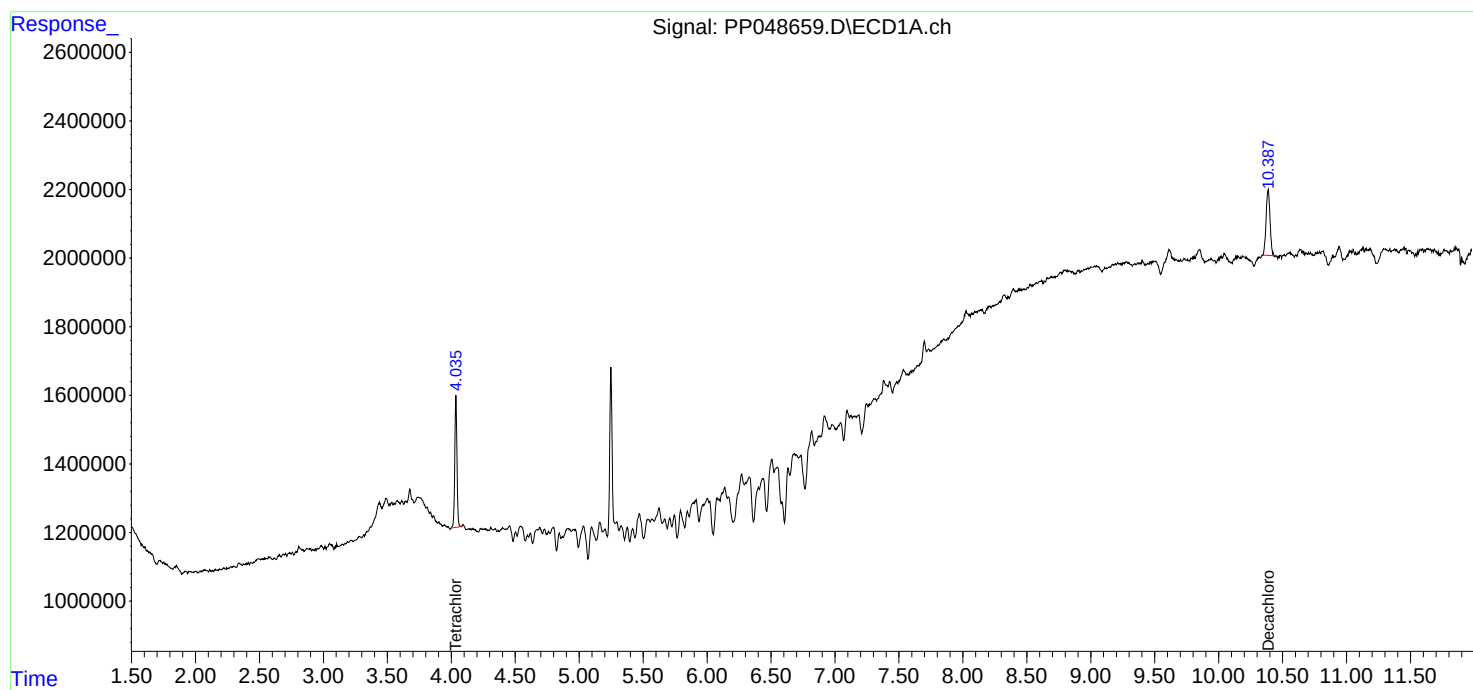

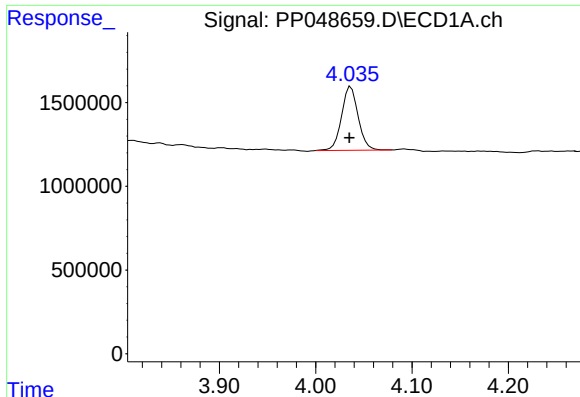


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.002 min
Response: 4551065
Conc: 1.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
SOM-2022-35A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2022
Supervised By :Ankita Jodhani 06/10/2022

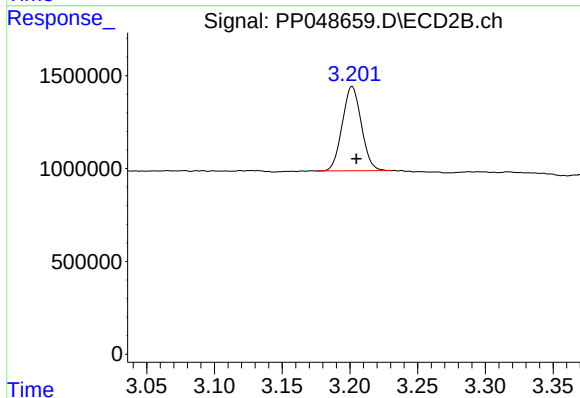


#1 Tetrachloro-m-xylene

R.T.: 3.202 min
Delta R.T.: -0.003 min
Response: 4467500
Conc: 2.35 ng/ml

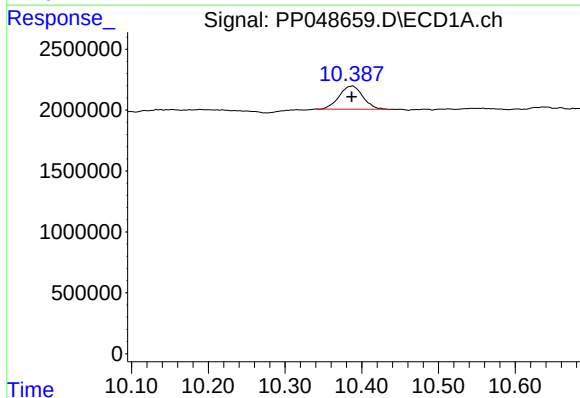

#2 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.001 min
Response: 4082910
Conc: 2.14 ng/ml

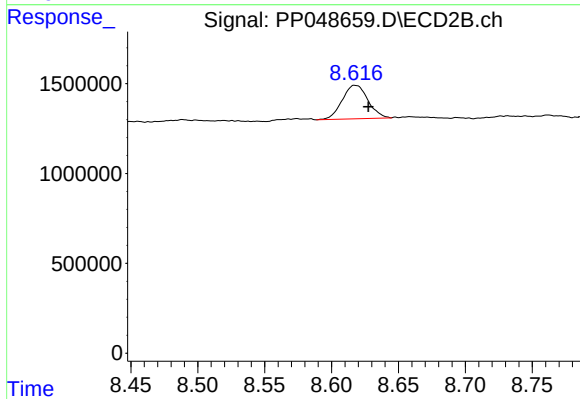

#2 Decachlorobiphenyl

R.T.: 8.616 min
Delta R.T.: -0.011 min
Response: 2503349
Conc: 2.04 ng/ml m