

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061024\
Data File : PP065546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 17:46
Operator : YP\AJ
Sample : P2808-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IRV-2024-1-A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:26:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.825	4.070	2733150	4016180	1.441	1.438
2) SA Decachlor...	10.842	9.261	4103021	2859050	2.086m	1.941

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061024\
Data File : PP065546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 17:46
Operator : YP\AJ
Sample : P2808-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IRV-2024-1-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:26:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

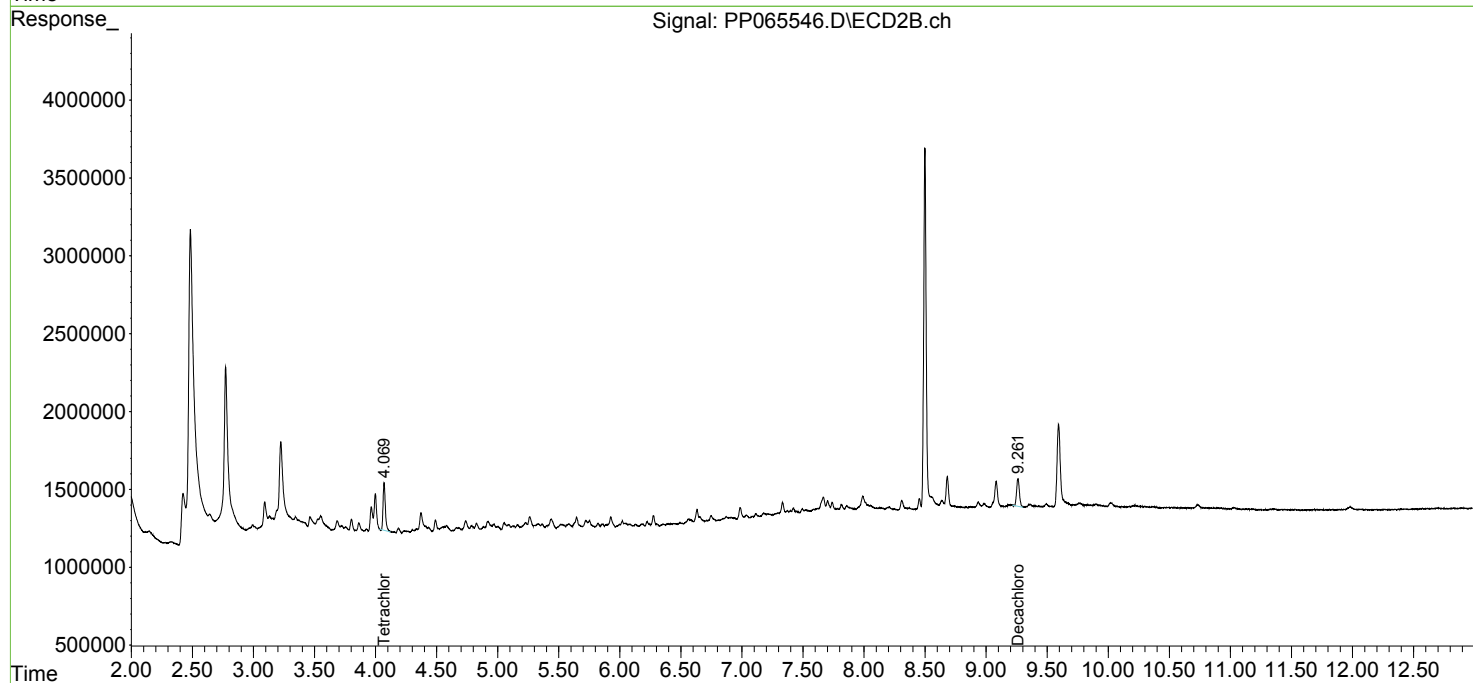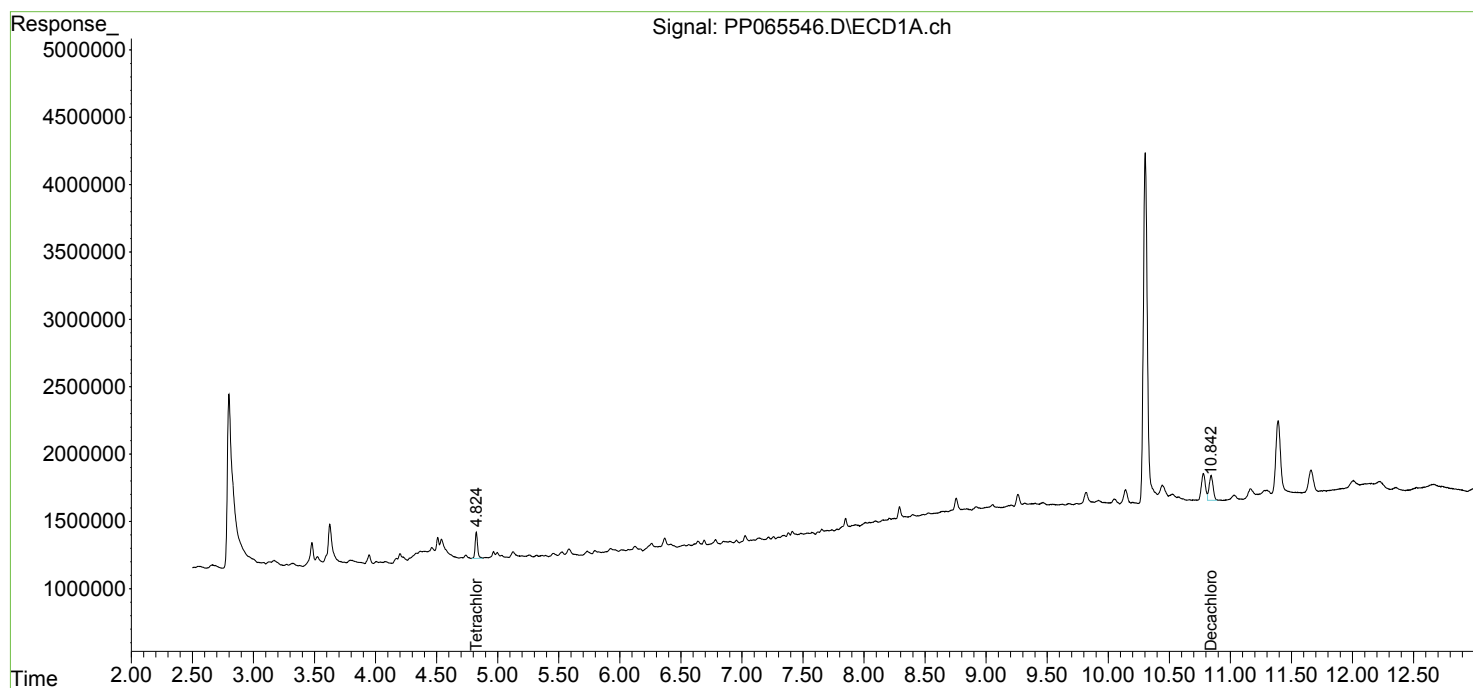

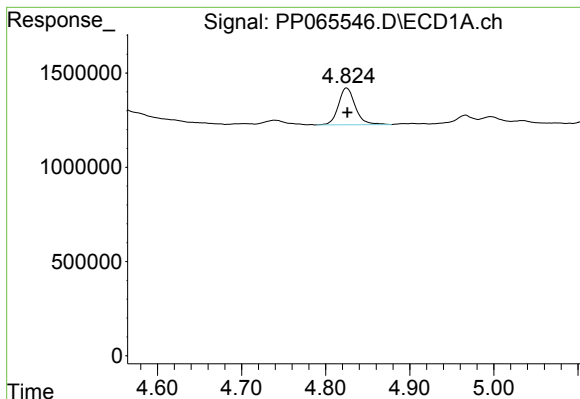


#1 Tetrachloro-m-xylene

R.T.: 4.825 min
Delta R.T.: -0.001 min
Response: 2733150
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2024-1-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

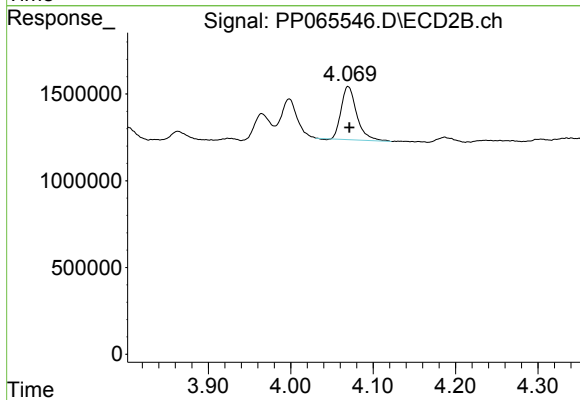


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.002 min
Response: 4016180
Conc: 1.44 ng/ml

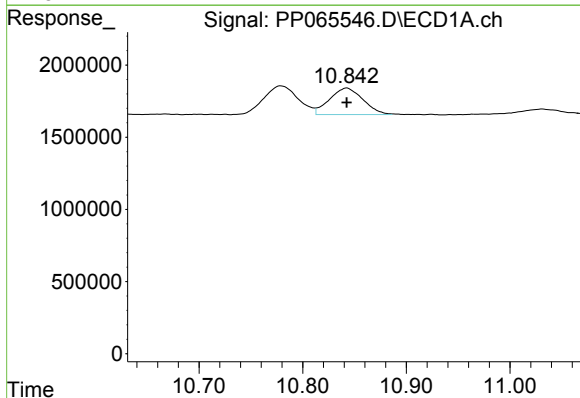

#2 Decachlorobiphenyl

R.T.: 10.842 min
Delta R.T.: 0.000 min
Response: 4103021
Conc: 2.09 ng/ml m

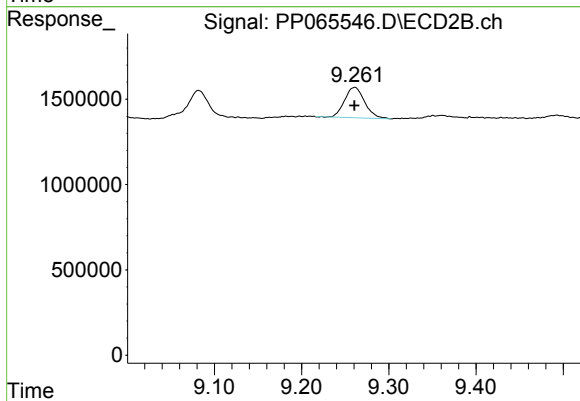

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 2859050
Conc: 1.94 ng/ml