

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061024\
 Data File : PP065547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2024 18:02
 Operator : YP\AJ
 Sample : P2808-02 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-2024-1-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/11/2024
 Supervised By :Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:31:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.825	4.069	2929399	4377920	1.544	1.568
2) SA Decachlor...	10.843	9.261	3627614	2667061	1.844m	1.810

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061024\
Data File : PP065547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 18:02
Operator : YP\AJ
Sample : P2808-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IRV-2024-1-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:31:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

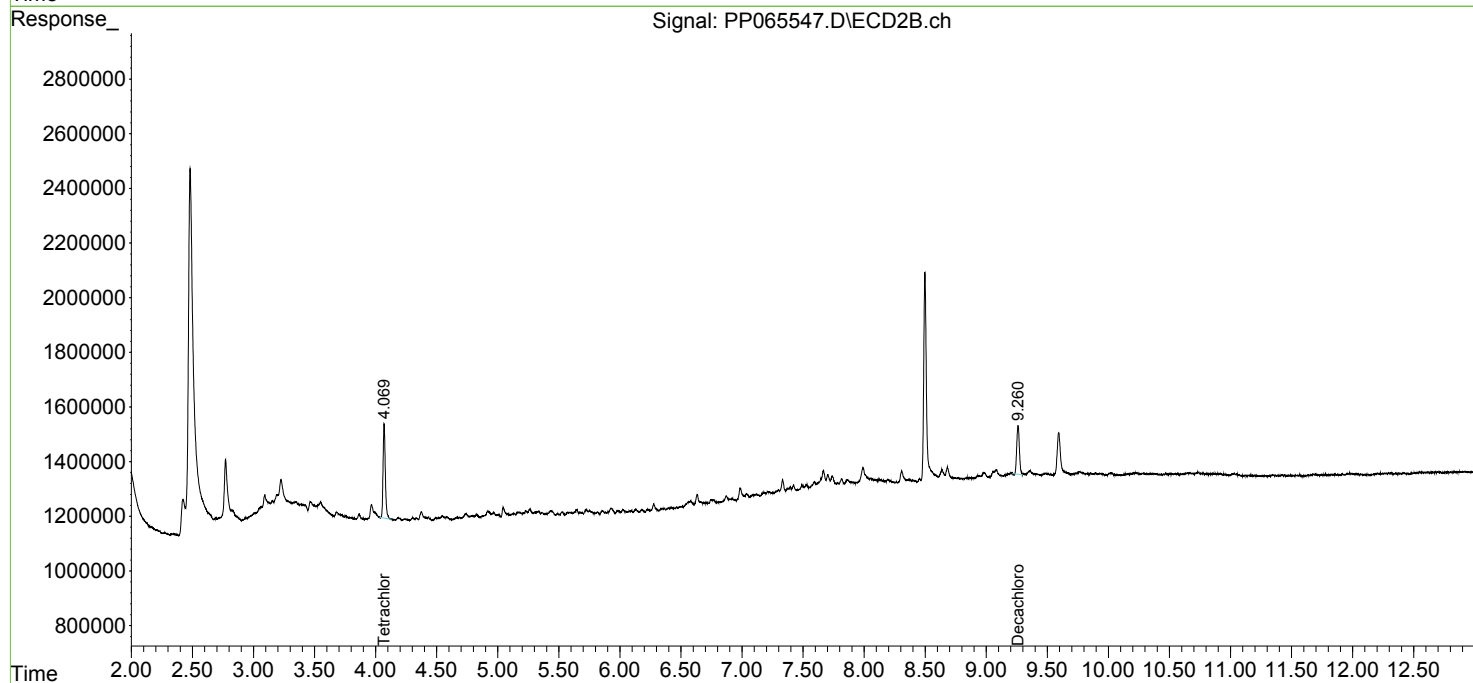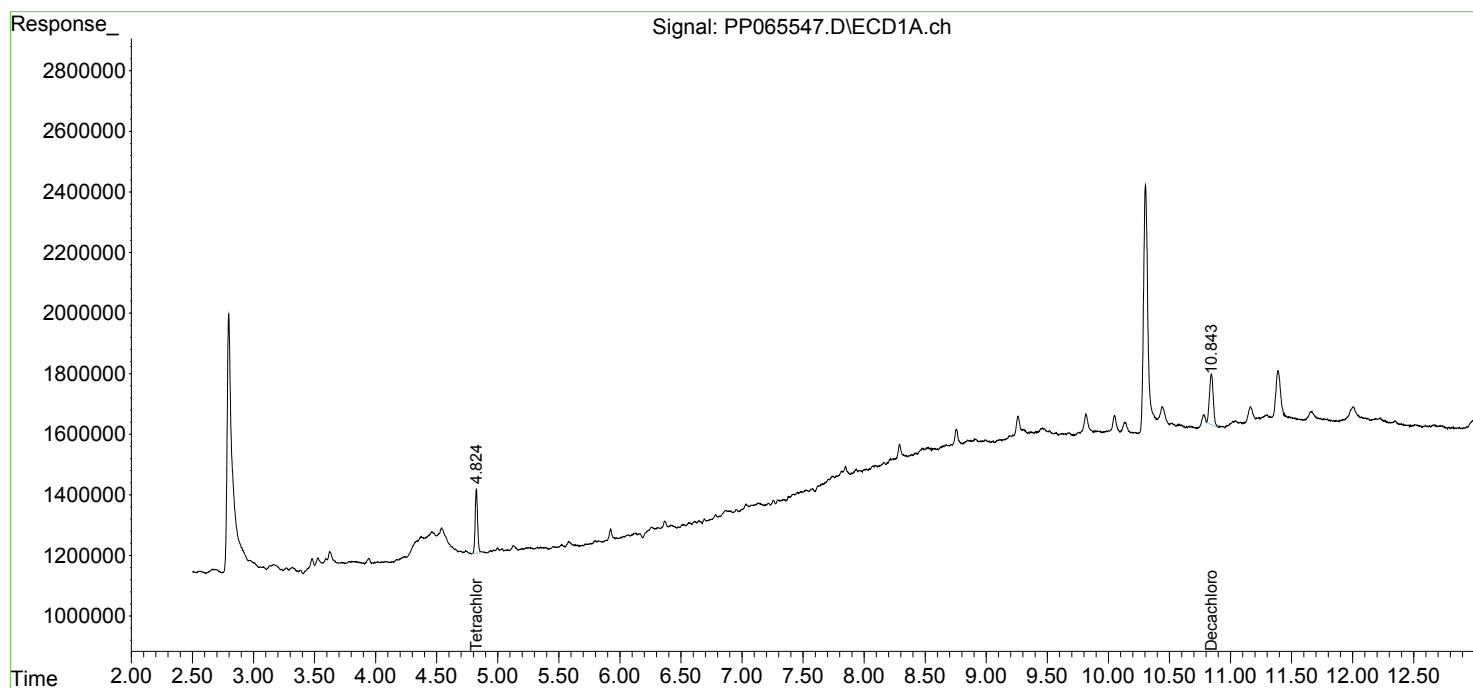

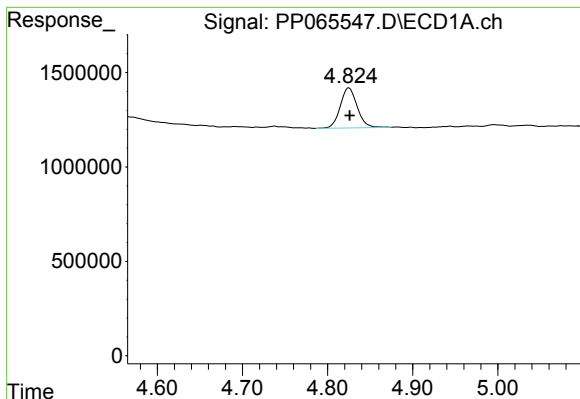


#1 Tetrachloro-m-xylene

R.T.: 4.825 min
Delta R.T.: 0.000 min
Response: 2929399
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2024-1-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

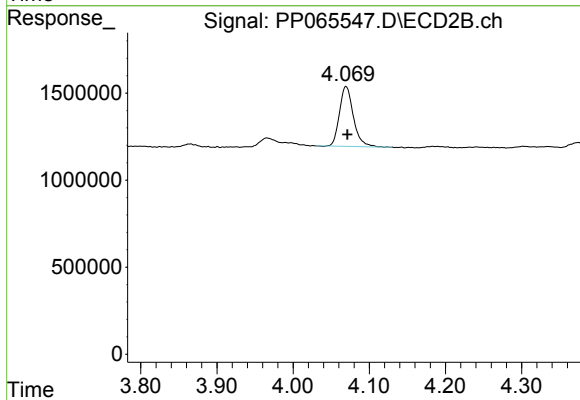


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.002 min
Response: 4377920
Conc: 1.57 ng/ml

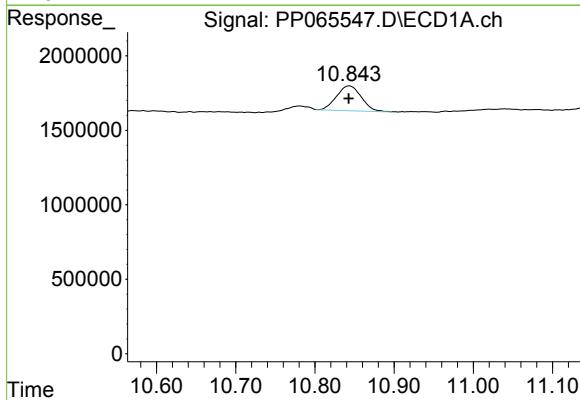

#2 Decachlorobiphenyl

R.T.: 10.843 min
Delta R.T.: 0.000 min
Response: 3627614
Conc: 1.84 ng/ml m

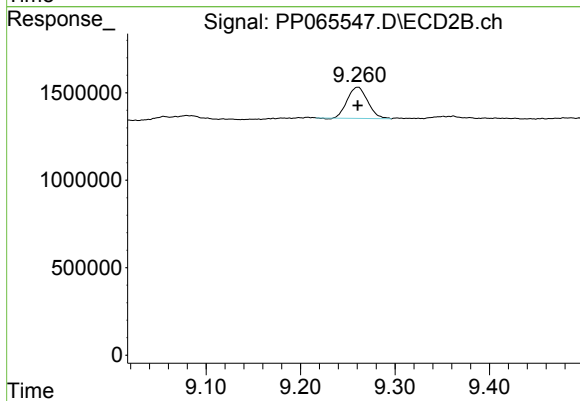

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 2667061
Conc: 1.81 ng/ml