

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061025\
 Data File : PP072784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 15:37
 Operator : YP\AJ
 Sample : Q2274-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-13-MHP-WC

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 06:19:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.792	42128687	37587117	20.951	23.516
2) SA Decachlor...	10.193	8.805	30912409	23691360	18.975m	22.380m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061025\
Data File : PP072784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 15:37
Operator : YP\AJ
Sample : Q2274-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-13-MHP-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 06:19:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

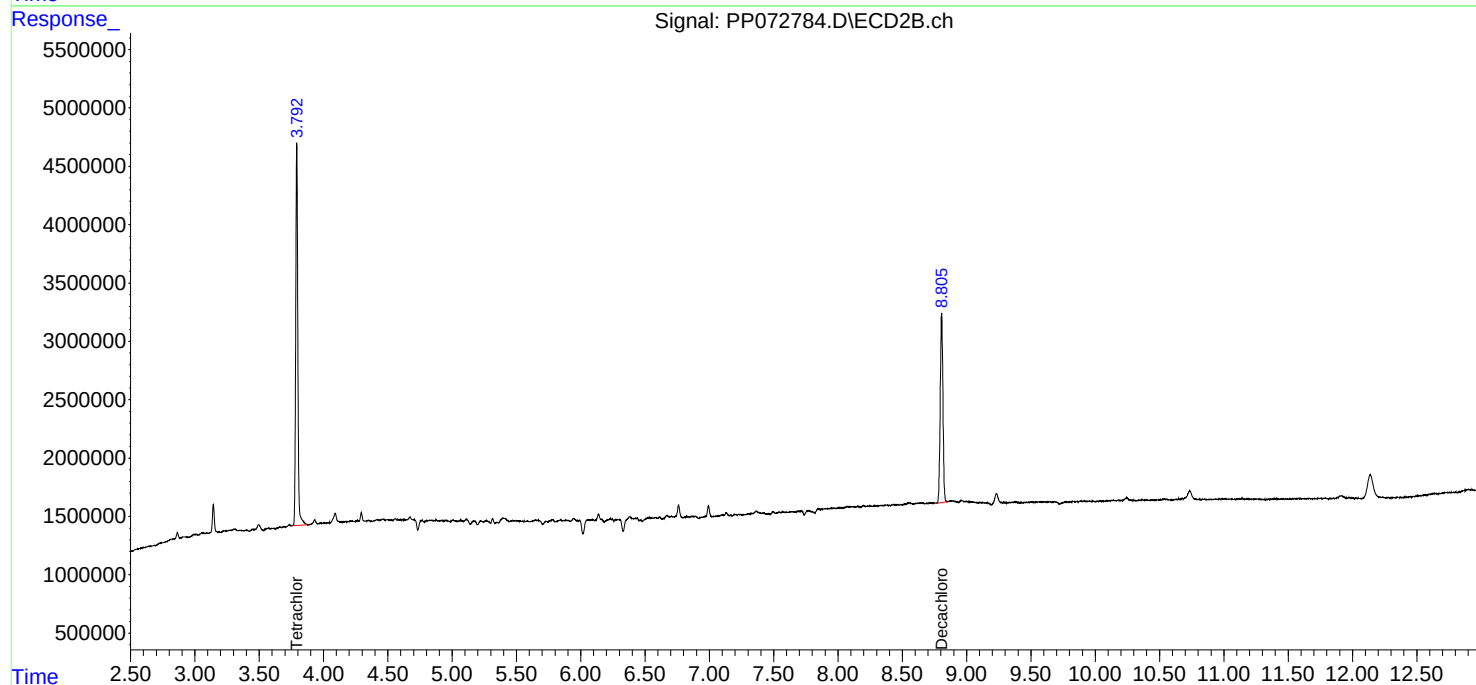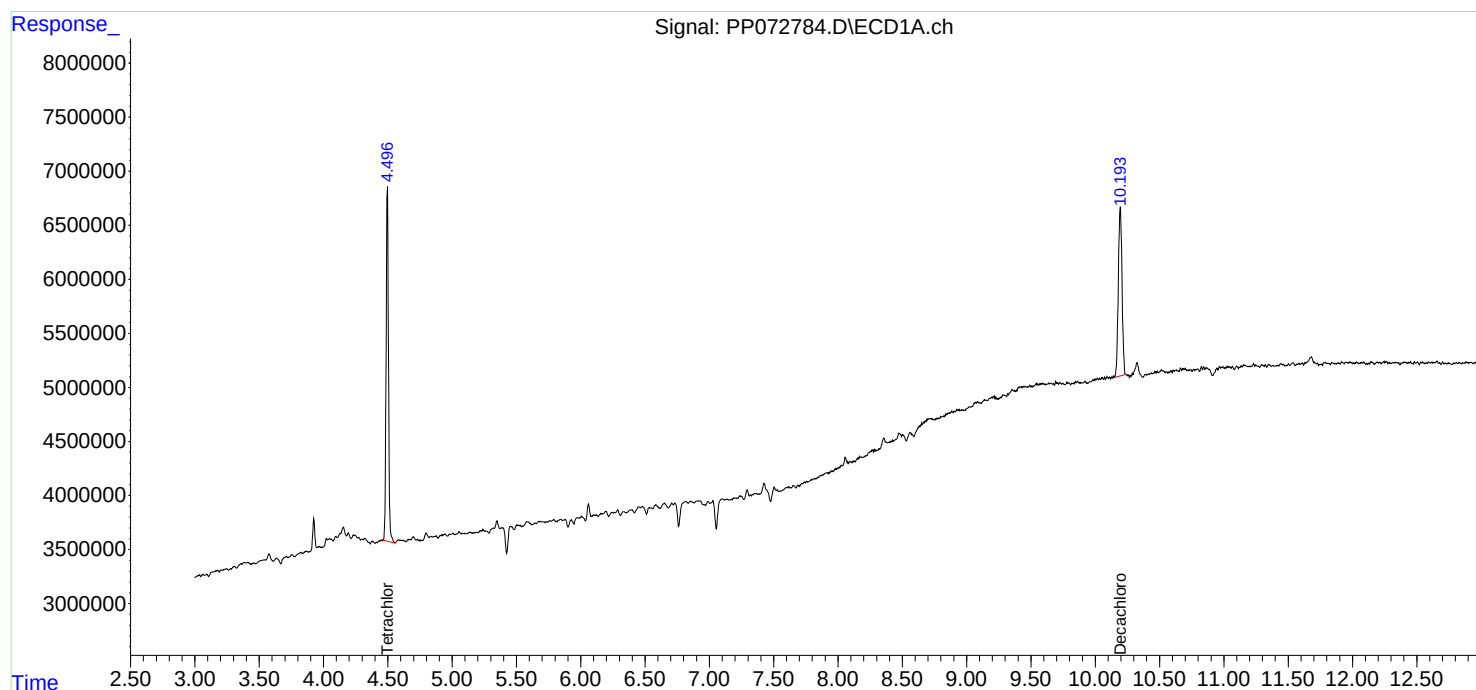

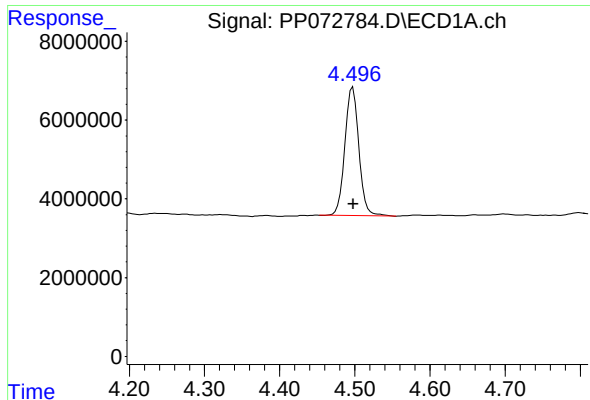


#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: 0.000 min
Response: 42128687
Conc: 20.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-13-MHP-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

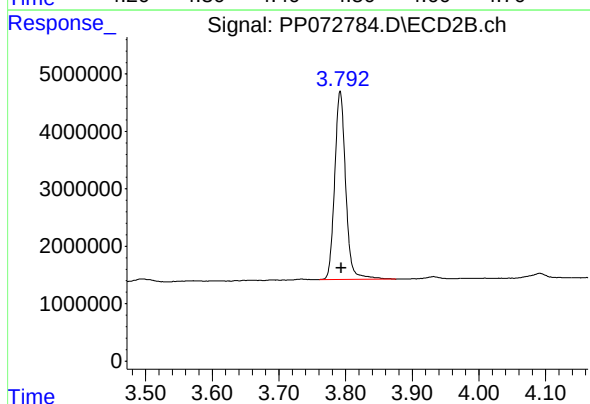


#1 Tetrachloro-m-xylene

R.T.: 3.792 min
Delta R.T.: -0.002 min
Response: 37587117
Conc: 23.52 ng/ml

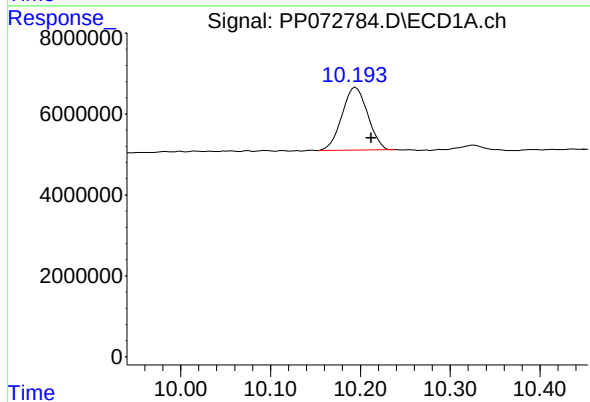

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.019 min
Response: 30912409
Conc: 18.97 ng/ml m

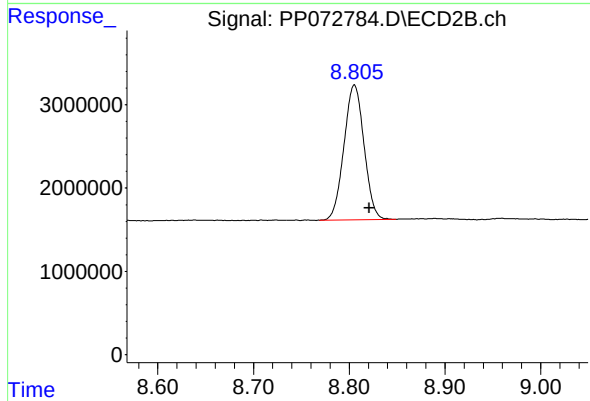

#2 Decachlorobiphenyl

R.T.: 8.805 min
Delta R.T.: -0.016 min
Response: 23691360
Conc: 22.38 ng/ml m