

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061122\
 Data File : PP048709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2022 14:15
 Operator : YP\AJ
 Sample : N3293-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 40804

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/13/2022
 Supervised By :Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 16:31:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 07 11:09:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.060	3.238f	40794212	34782384	17.025m	18.274m
2) SA Decachlor...	10.394	8.621	40602973	24674825	21.303	20.150

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061122\
Data File : PP048709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2022 14:15
Operator : YP\AJ
Sample : N3293-06
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
40804


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 16:31:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 07 11:09:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

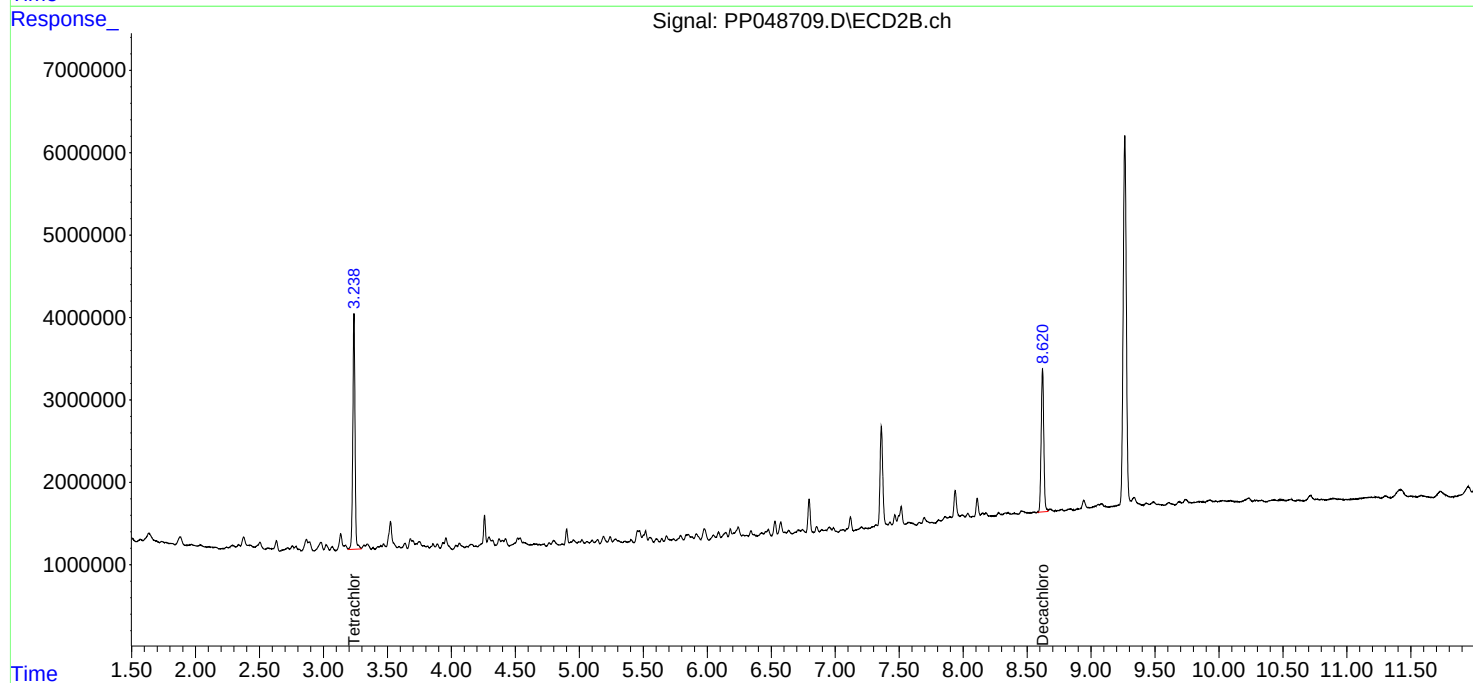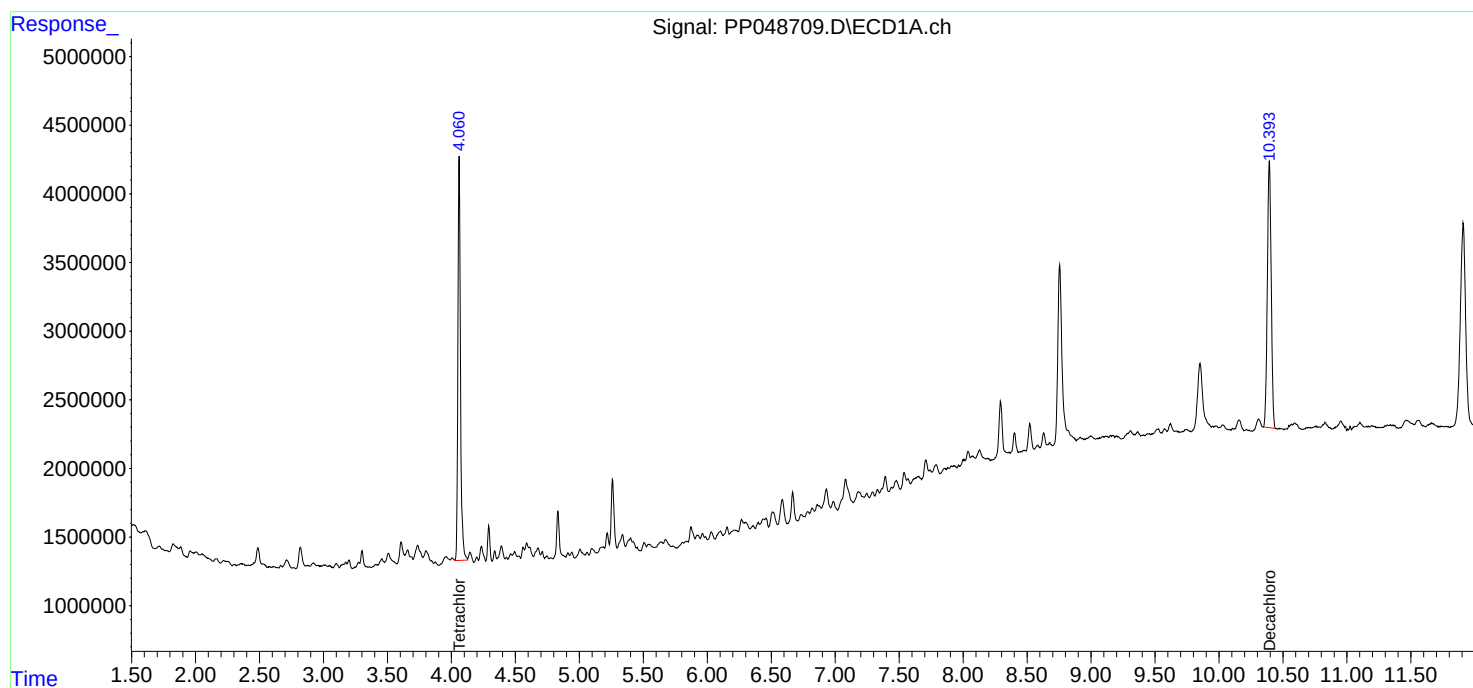

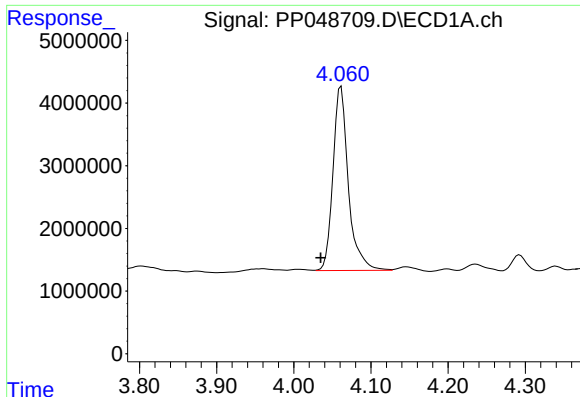


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.025 min
Response: 40794212
Conc: 17.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
40804


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

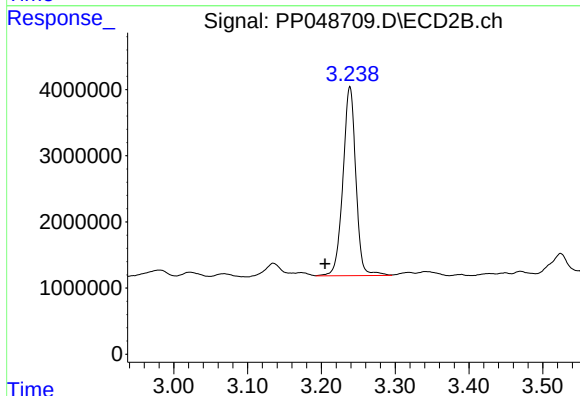


#1 Tetrachloro-m-xylene

R.T.: 3.238 min
Delta R.T.: 0.034 min
Response: 34782384
Conc: 18.27 ng/ml m

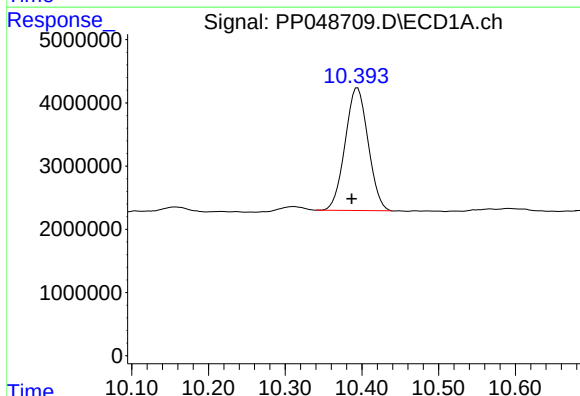

#2 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: 0.008 min
Response: 40602973
Conc: 21.30 ng/ml

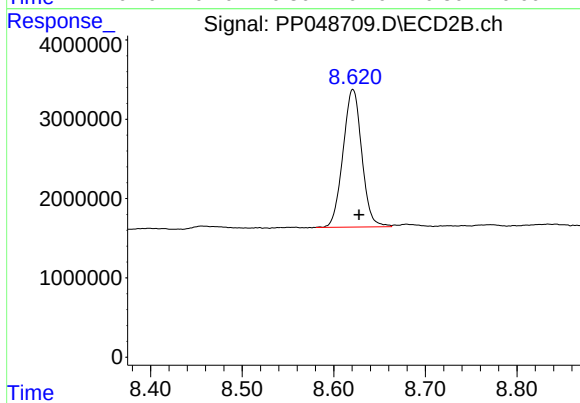

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: -0.007 min
Response: 24674825
Conc: 20.15 ng/ml