

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
 Data File : PP072820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 15:11
 Operator : YP\AJ
 Sample : Q2283-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-25-0166-MOO-25-0167

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/12/2025
 Supervised By :mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:51:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.497	3.794	20294498	20747377	10.093m	12.980 #
2) SA Decachlor...	10.191	8.804	24553018	20448046	15.071m	19.316m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
Data File : PP072820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 15:11
Operator : YP\AJ
Sample : Q2283-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-25-0166-MOO-25-0167


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/12/2025
Supervised By :mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:51:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

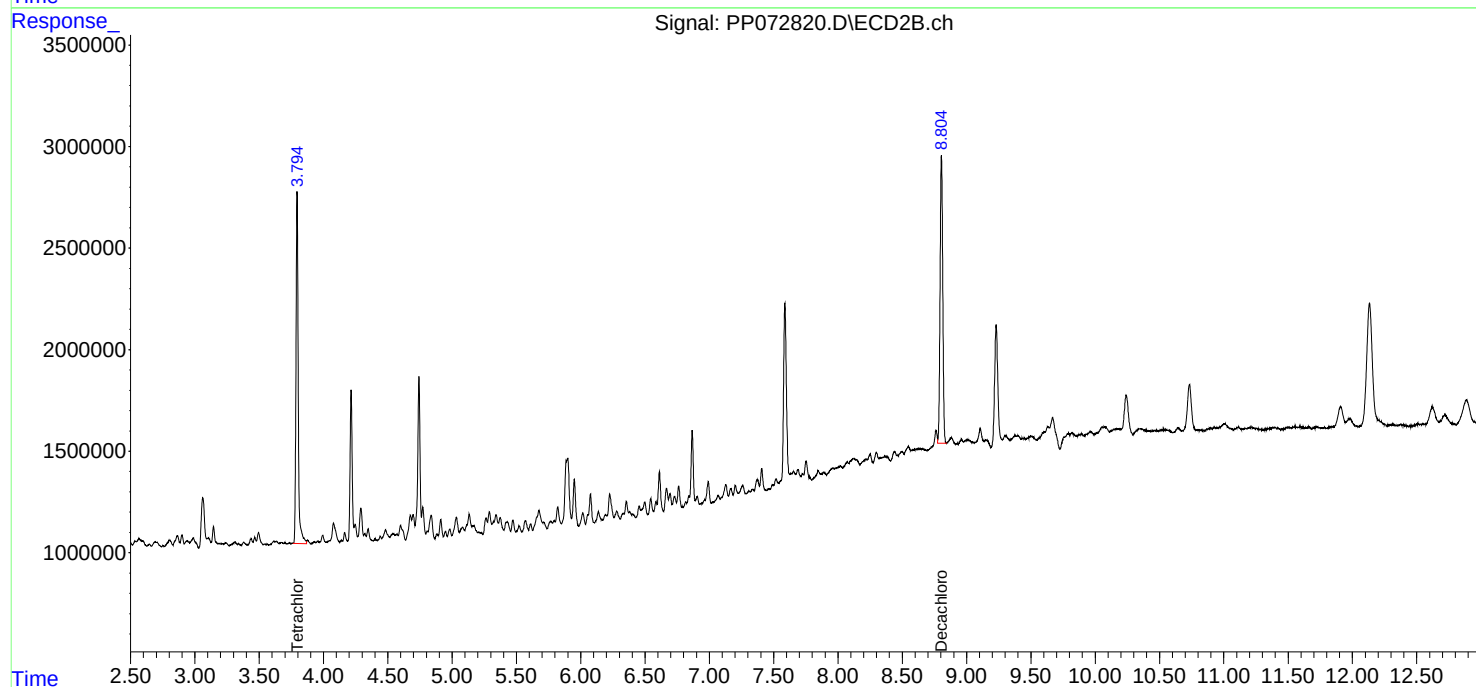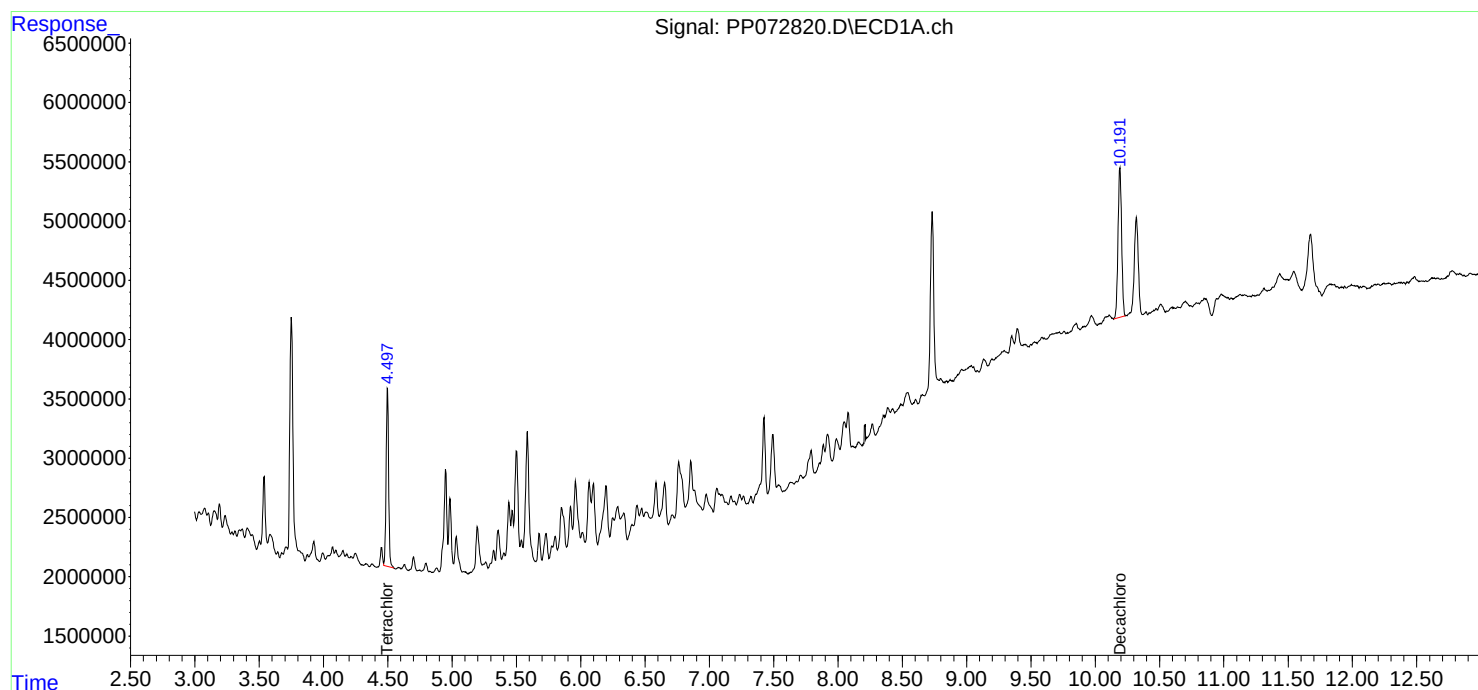

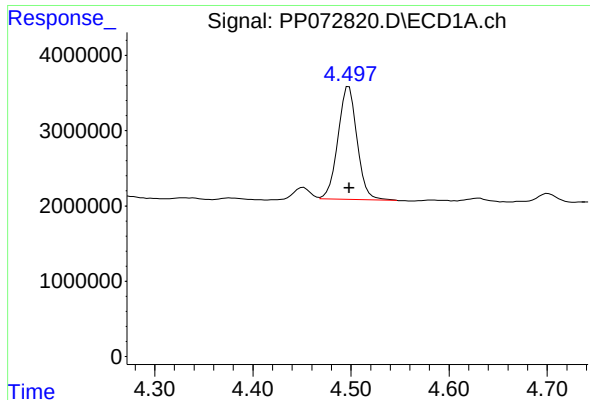


#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: -0.001 min
Response: 20294498
Conc: 10.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-25-0166-MOO-25-0167


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/12/2025
Supervised By :mohammad ahmed 06/16/2025

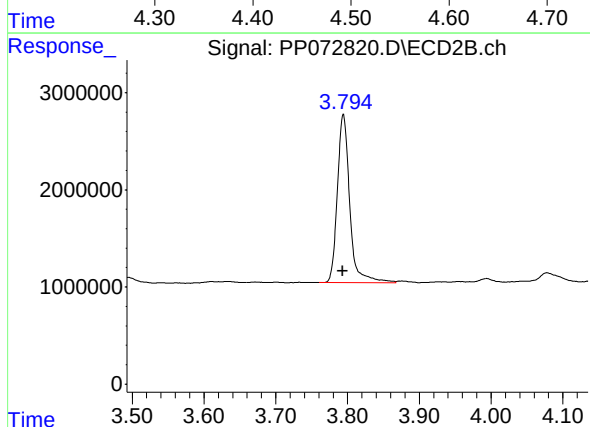


#1 Tetrachloro-m-xylene

R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 20747377
Conc: 12.98 ng/ml

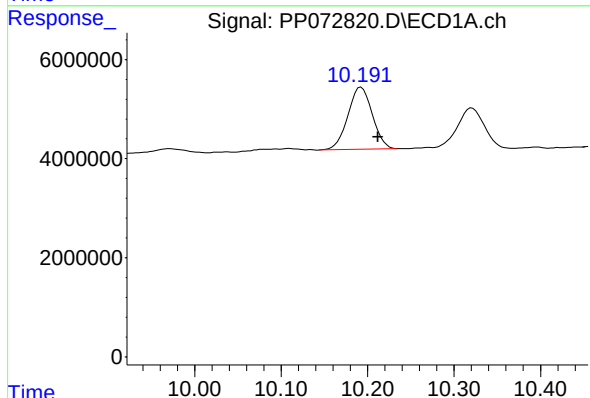

#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: -0.021 min
Response: 24553018
Conc: 15.07 ng/ml m

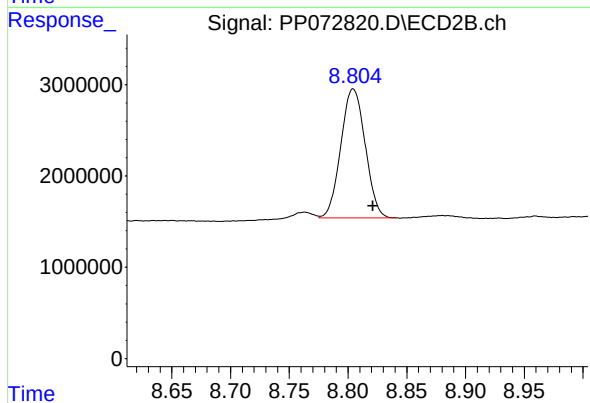

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.017 min
Response: 20448046
Conc: 19.32 ng/ml m