

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
 Data File : PP072841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 22:55
 Operator : YP\AJ
 Sample : PB168421BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB168421BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel
 06/12/2025

Supervised By :monhammad
 ahmed
 06/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:57:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.793	39326050	33768350	19.557	21.127
2) SA Decachlor...	10.193	8.804	32482445	25394365	19.939m	23.989m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
Data File : PP072841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 22:55
Operator : YP\AJ
Sample : PB168421BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB168421BL



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
06/12/2025

Supervised By :mohammad
ahmed
06/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:57:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

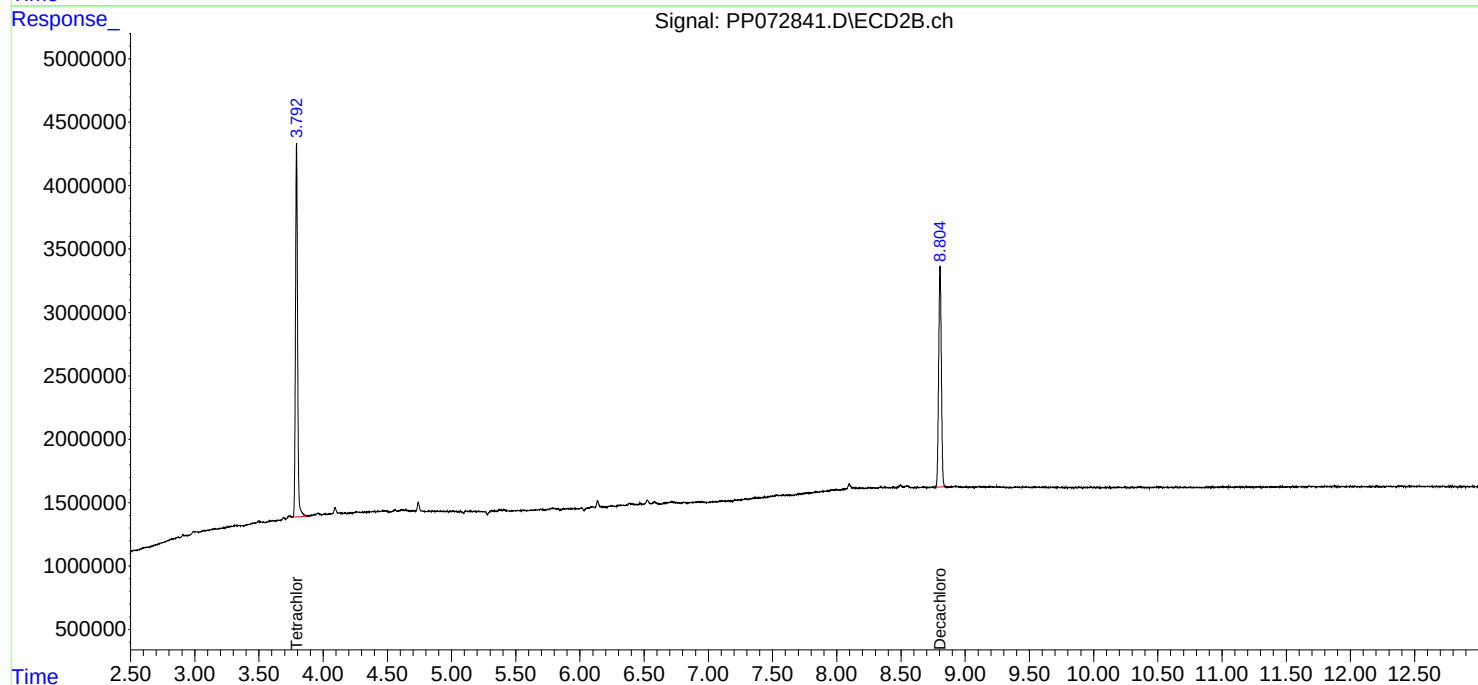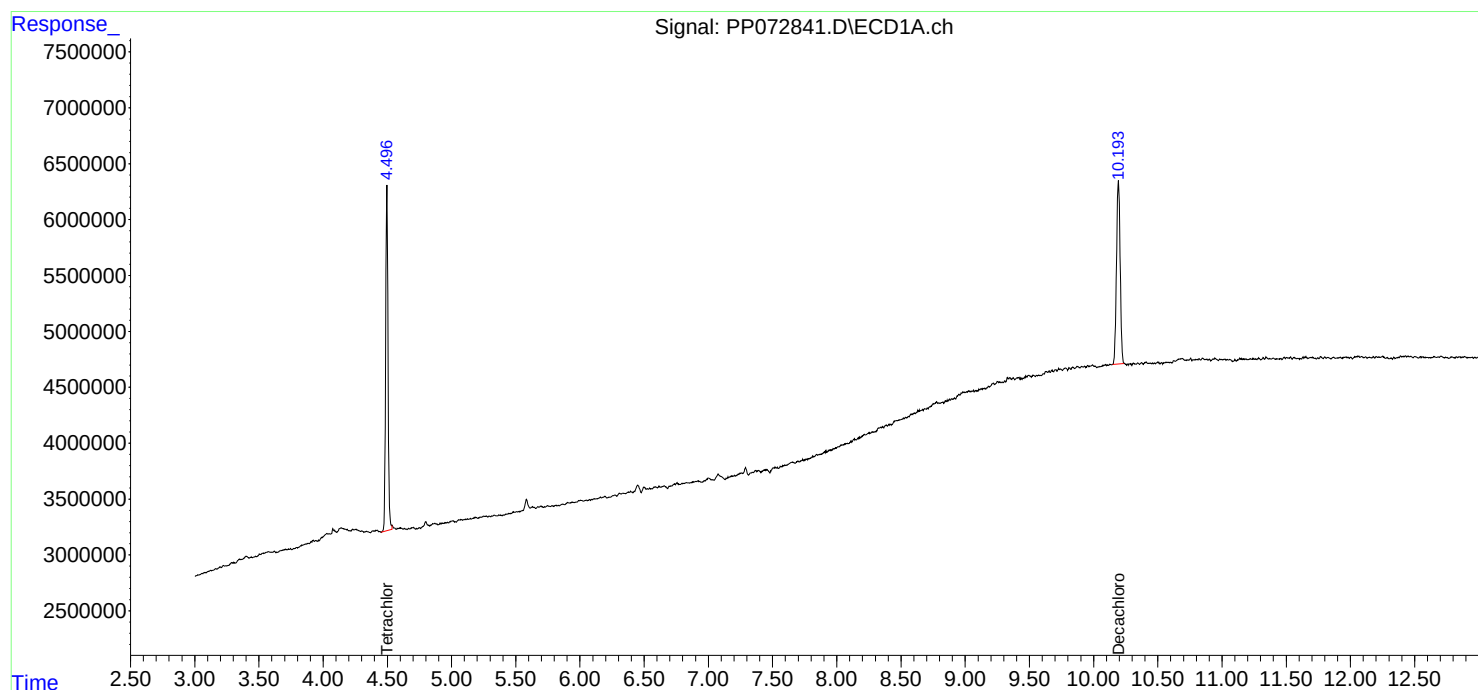

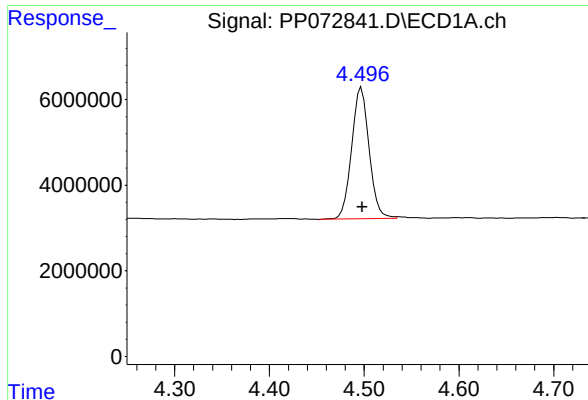

#1 Tetrachloro-m-xylene


R.T.: 4.497 min
Delta R.T.: 0.000 min
Response: 39326050
Conc: 19.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB168421BL

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
06/12/2025

Supervised By :mohammad
ahmed
06/16/2025

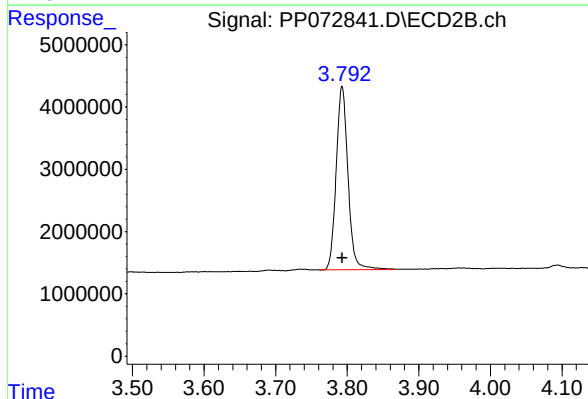


#1 Tetrachloro-m-xylene

R.T.: 3.793 min
Delta R.T.: 0.000 min
Response: 33768350
Conc: 21.13 ng/ml

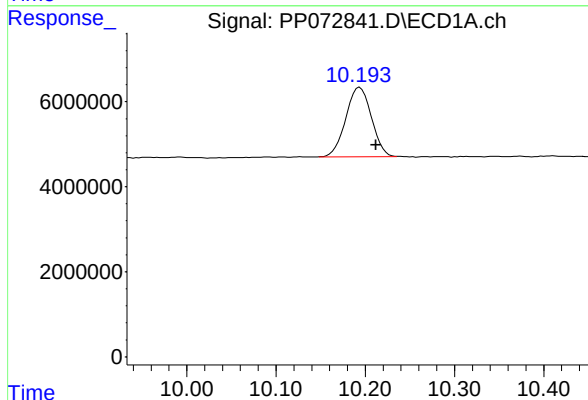

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.020 min
Response: 32482445
Conc: 19.94 ng/ml m

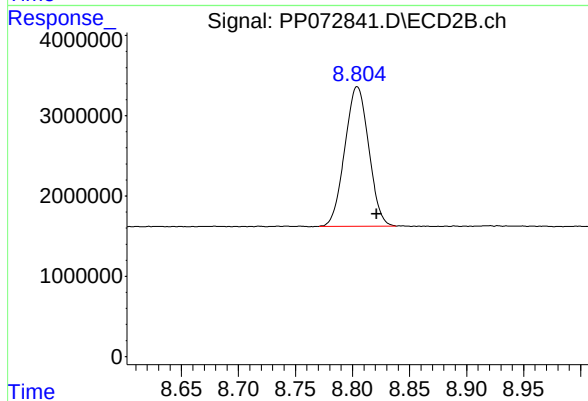

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.018 min
Response: 25394365
Conc: 23.99 ng/ml m