

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
 Data File : PP072847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2025 00:33
 Operator : YP\AJ
 Sample : Q2282-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GAS-AUD-25-0096

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/12/2025
 Supervised By :mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:59:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.792	43415639	36415530	21.591	22.783m
2) SA Decachlor...	10.193	8.803	40405645	29001092	24.802m	27.396m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061125\
Data File : PP072847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2025 00:33
Operator : YP\AJ
Sample : Q2282-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GAS-AUD-25-0096


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/12/2025
Supervised By :mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:59:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

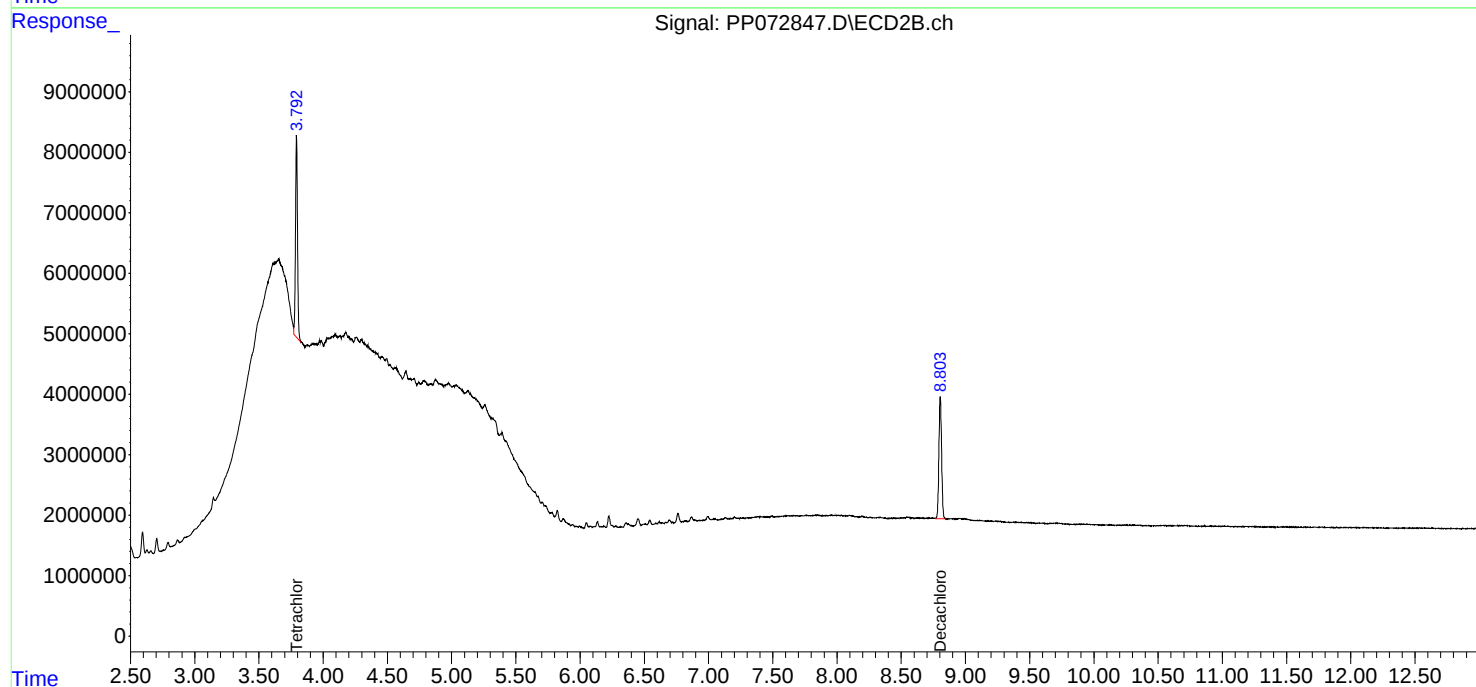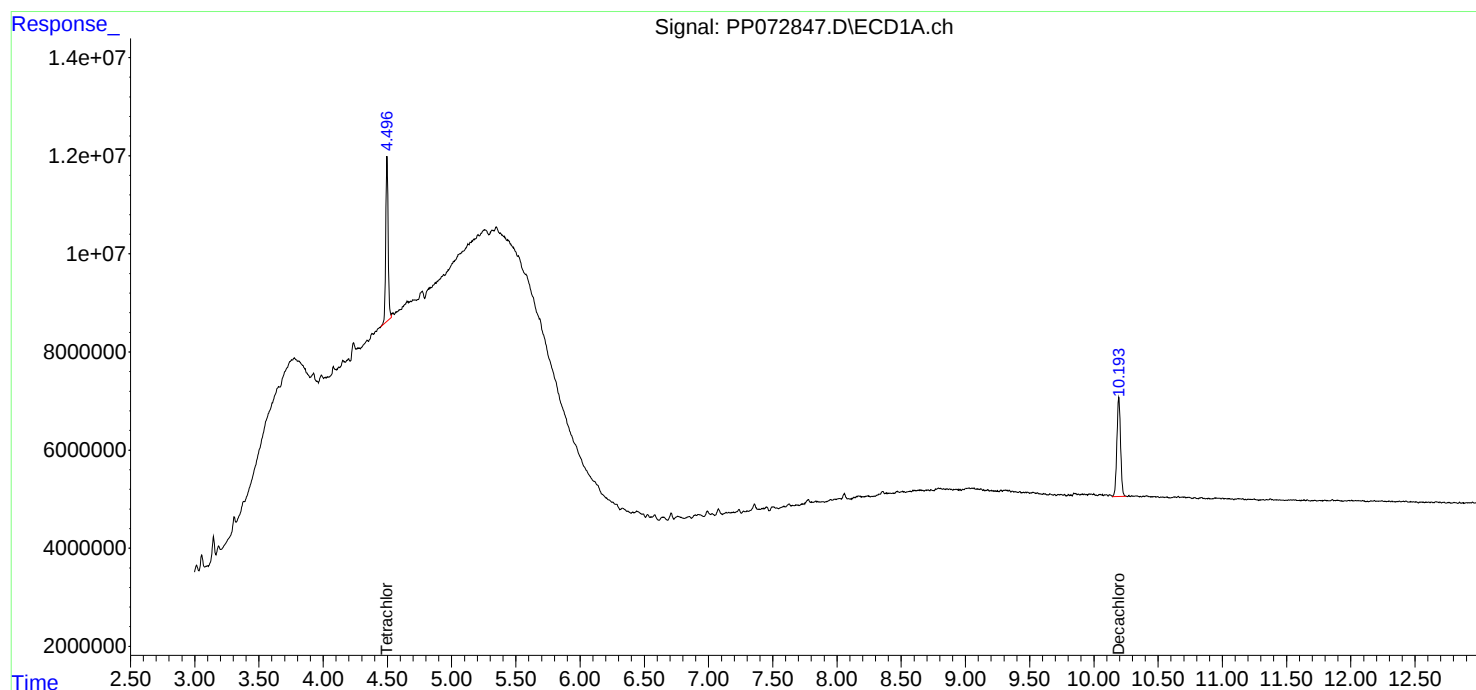

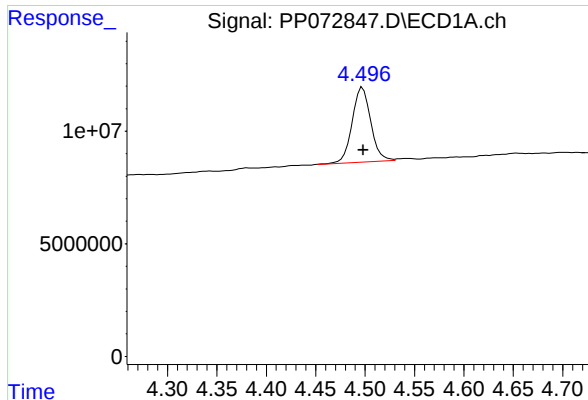


#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: 0.000 min
Response: 43415639
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
GAS-AUD-25-0096


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/12/2025
Supervised By :mohammad ahmed 06/16/2025

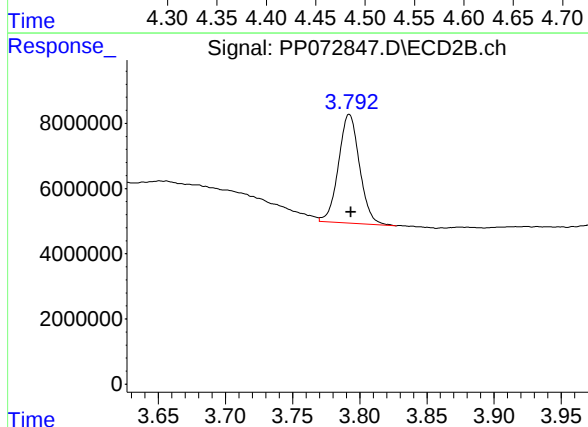


#1 Tetrachloro-m-xylene

R.T.: 3.792 min
Delta R.T.: -0.002 min
Response: 36415530
Conc: 22.78 ng/ml

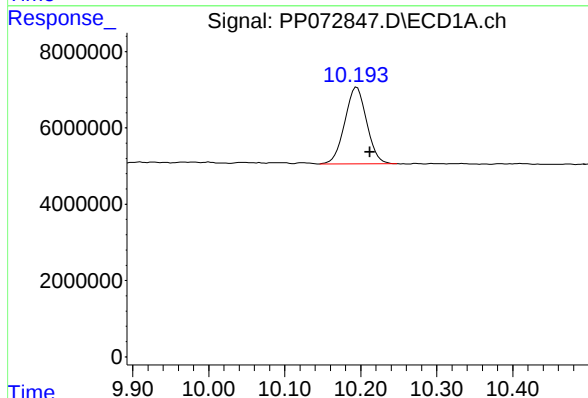

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.019 min
Response: 40405645
Conc: 24.80 ng/ml

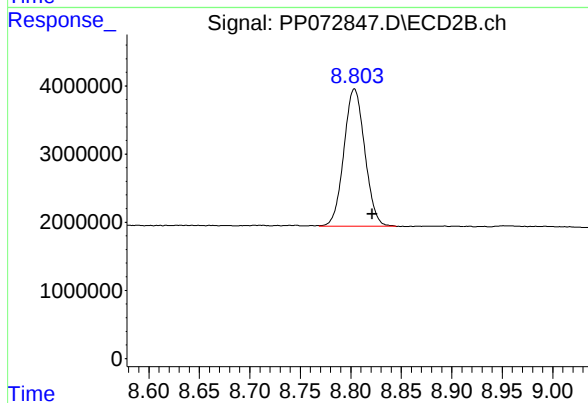

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.018 min
Response: 29001092
Conc: 27.40 ng/ml