

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061224\
 Data File : PP065621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2024 17:29
 Operator : YP\AJ
 Sample : P2848-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PE-1(0-0.5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/13/2024
 Supervised By :Ankita Jodhani 06/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:33:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.824	4.068	28869271	41615284	15.219	14.904
2) SA Decachlor...	10.837	9.253	26323513	19330856	13.383	13.122m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061224\
Data File : PP065621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2024 17:29
Operator : YP\AJ
Sample : P2848-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PE-1(0-0.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/13/2024
Supervised By :Ankita Jodhani 06/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:33:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

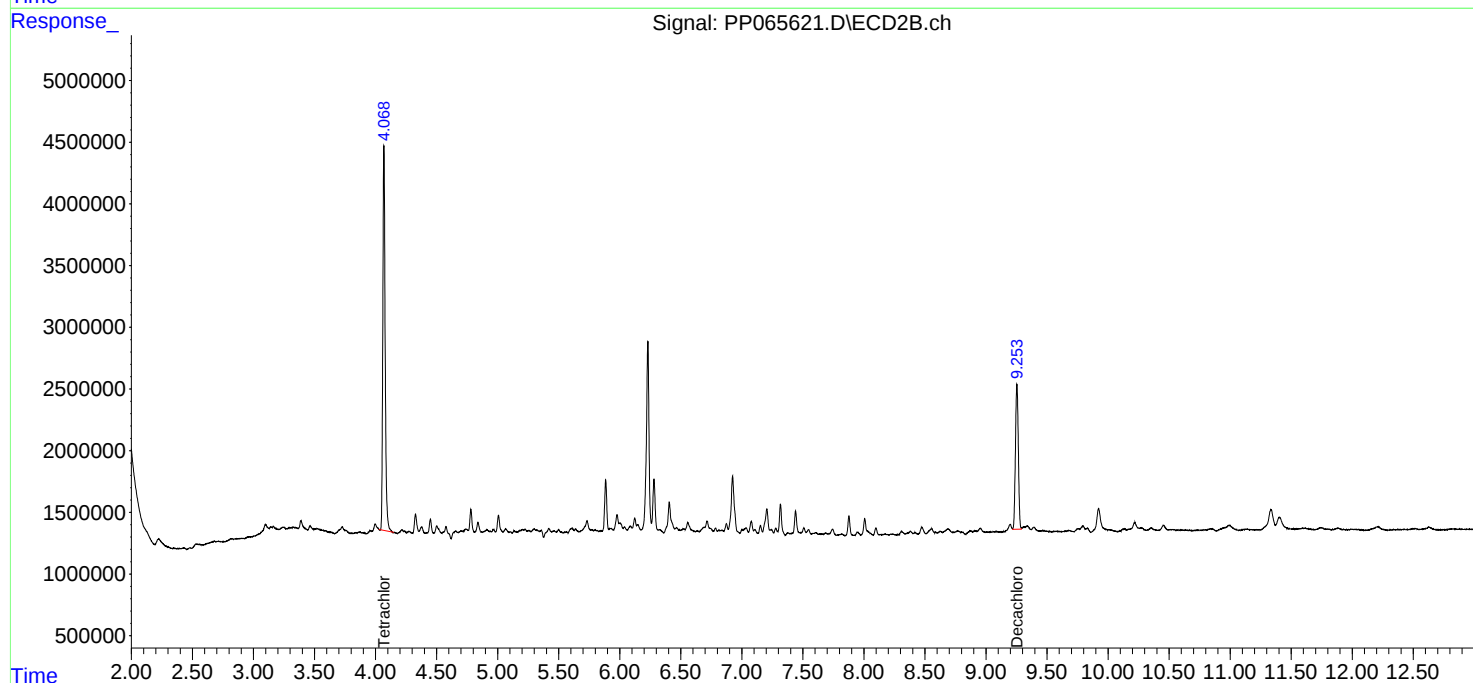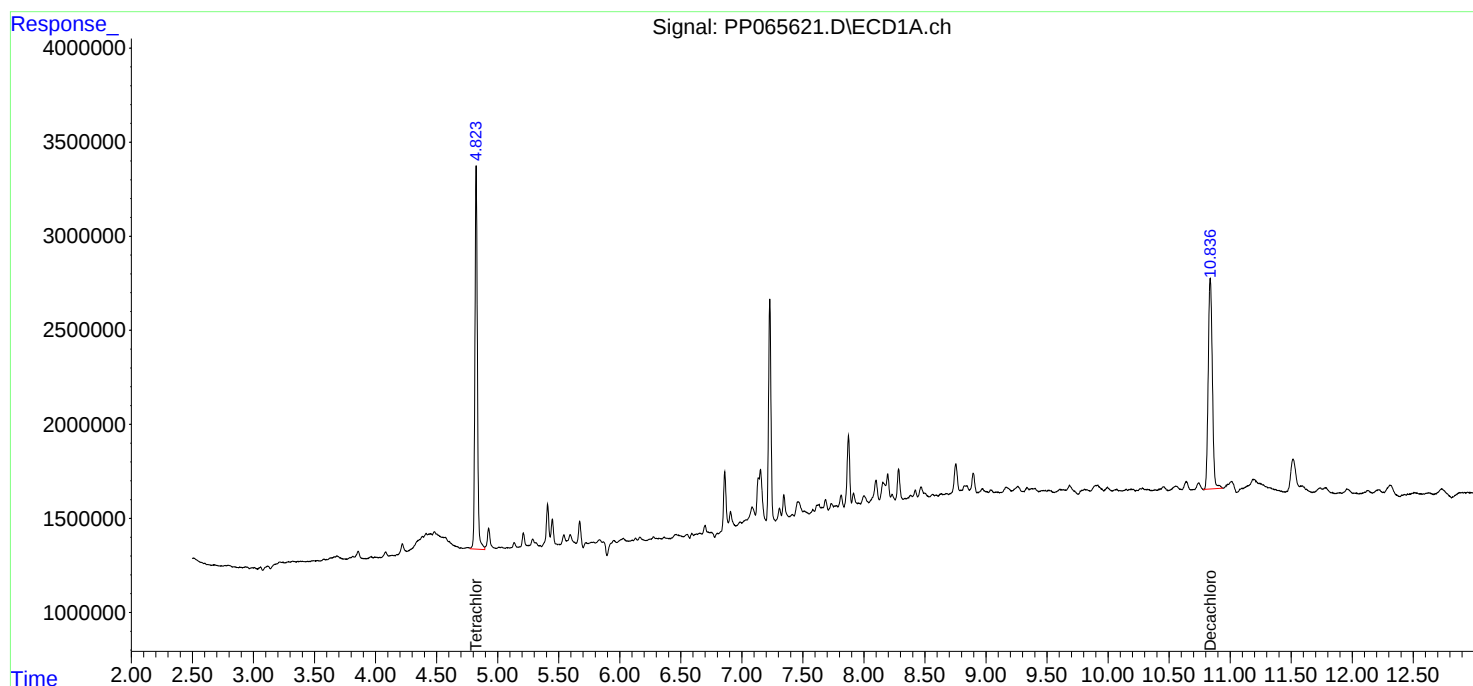

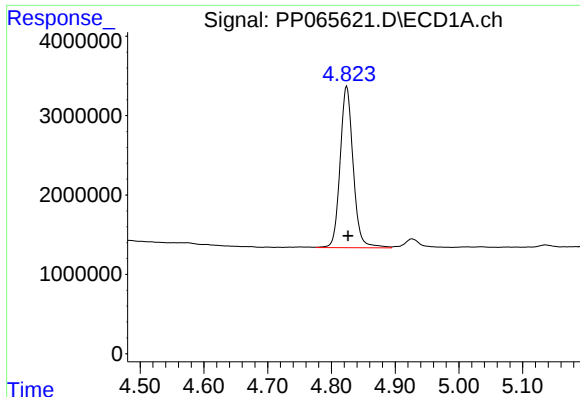


#1 Tetrachloro-m-xylene

R.T.: 4.824 min
Delta R.T.: -0.002 min
Response: 28869271
Conc: 15.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PE-1(0-0.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/13/2024
Supervised By :Ankita Jodhani 06/13/2024

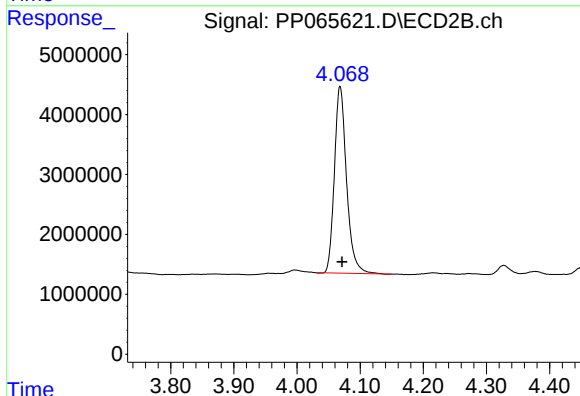


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: -0.003 min
Response: 41615284
Conc: 14.90 ng/ml

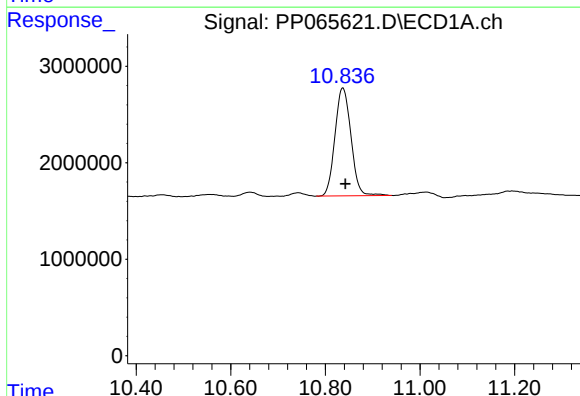

#2 Decachlorobiphenyl

R.T.: 10.837 min
Delta R.T.: -0.006 min
Response: 26323513
Conc: 13.38 ng/ml

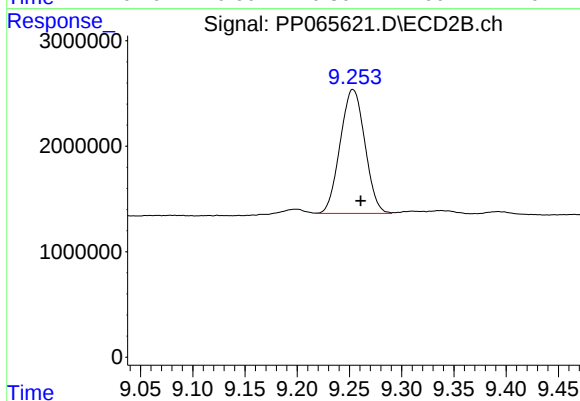

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.008 min
Response: 19330856
Conc: 13.12 ng/ml m