

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
 Data File : PP036383.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 9:11
 Operator : DD\AJ
 Sample : M2673-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:41:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.959	879801	627497	20.836	20.891
2)	SA Decachlor...	10.998	9.266	720813	548520	19.962	17.170
Target Compounds							
9)	L2 AR-1221-2	5.316	0.000	11103	0	28.787	N.D. #
12)	L3 AR-1232-2	6.002	0.000	12701	0	26.569	N.D. #
28)	L6 AR-1254-3	7.821f	0.000	9543	0	3.438	N.D. #
29)	L6 AR-1254-4	0.000	6.878f	0	102629	N.D.	65.195 #
35)	L7 AR-1260-5	9.159	7.890	14432	9291	3.845	2.514 #
37)	L8 AR-1262-2	9.159	7.890	14432	9291	3.022	2.244 #
44)	L9 AR-1268-4	10.281f	0.000	31722	0	16.205	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
Data File : PP036383.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 9:11
Operator : DD\AJ
Sample : M2673-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:41:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

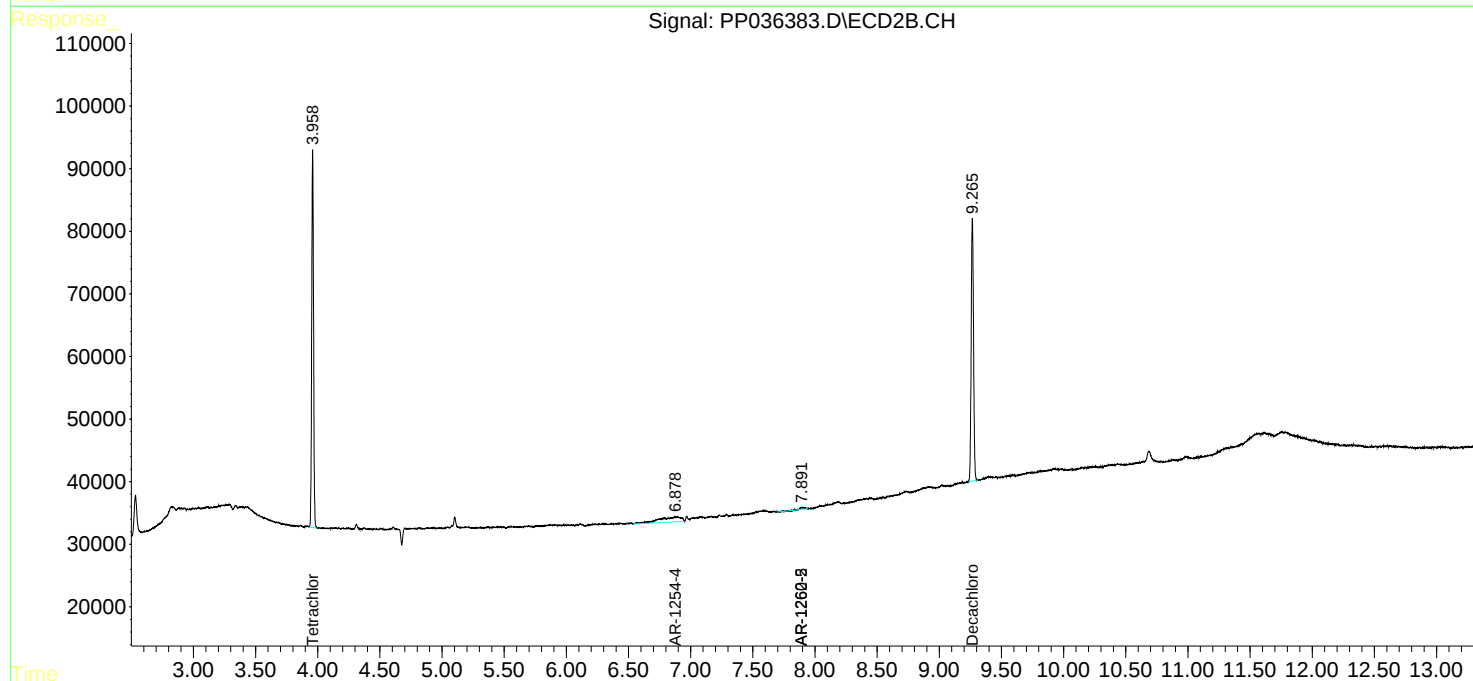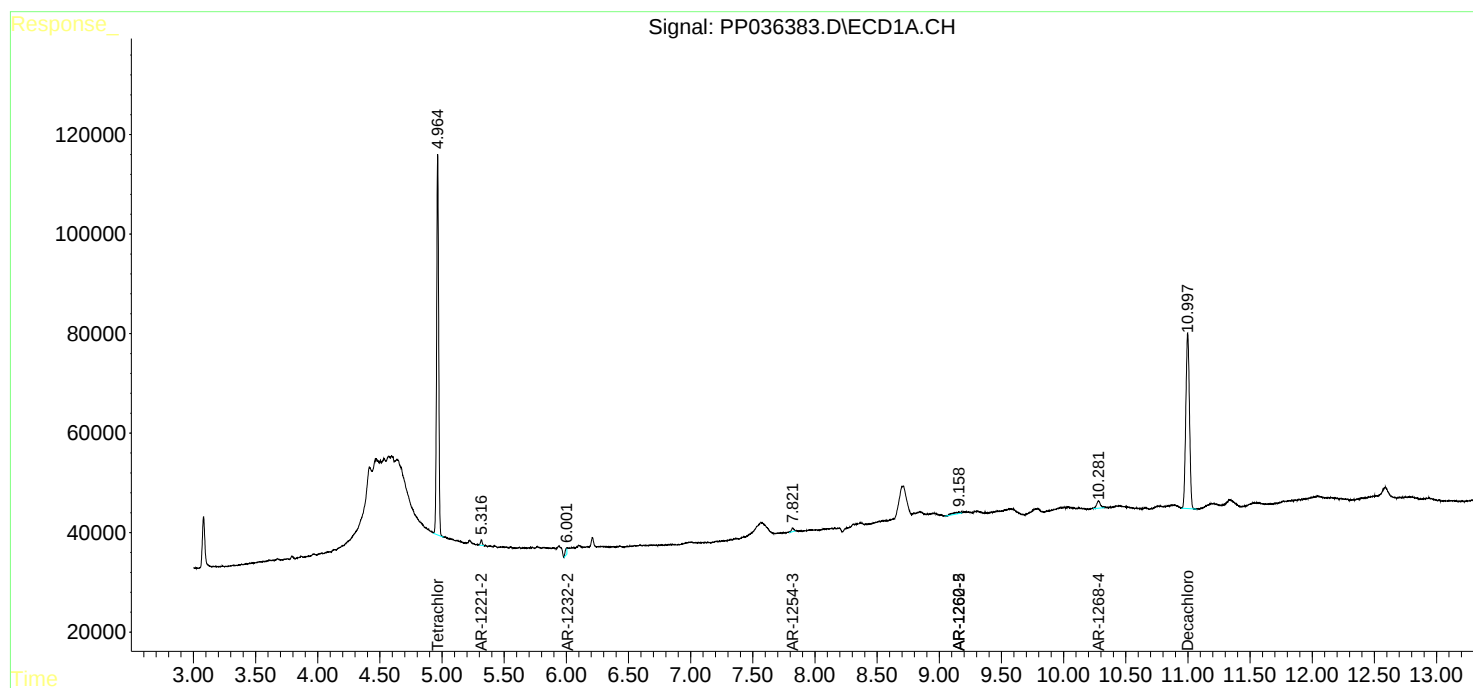


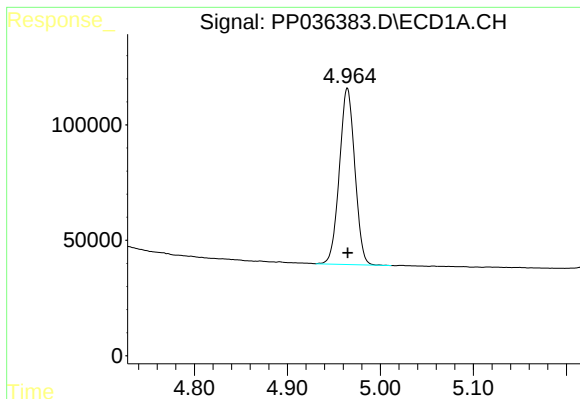

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 879801
Conc: 20.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

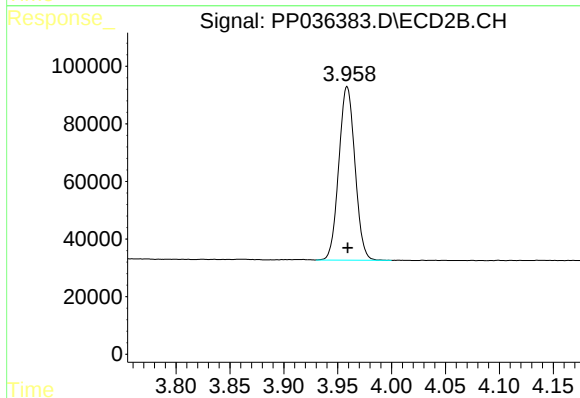


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 627497
Conc: 20.89 ng/ml

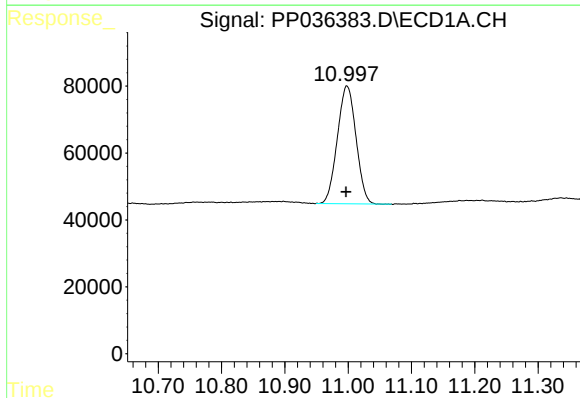


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.001 min
Response: 720813
Conc: 19.96 ng/ml

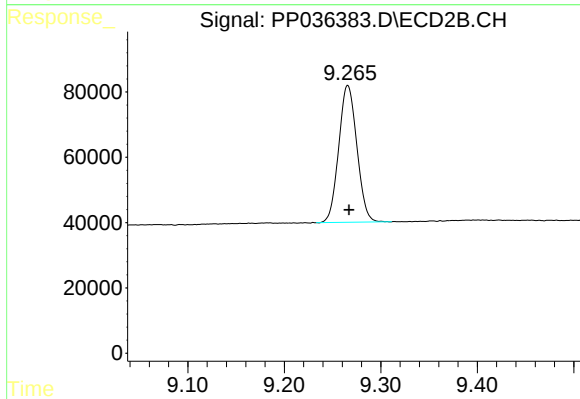

#2 Decachlorobiphenyl


R.T.: 9.266 min
Delta R.T.: -0.001 min
Response: 548520
Conc: 17.17 ng/ml

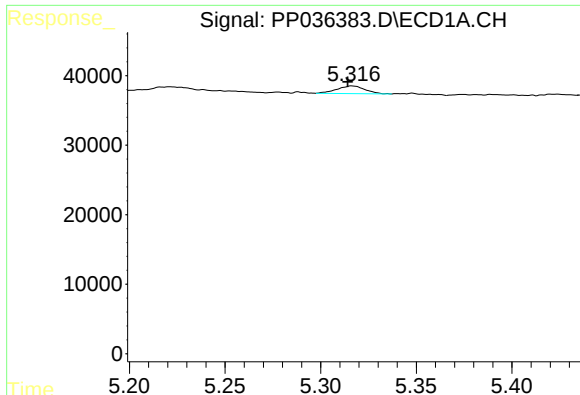

#9 AR-1221-2


R.T.: 5.316 min
Delta R.T.: 0.002 min
Response: 11103
Conc: 28.79 ng/ml

Instrument :
ECD_P
ClientSampleId :

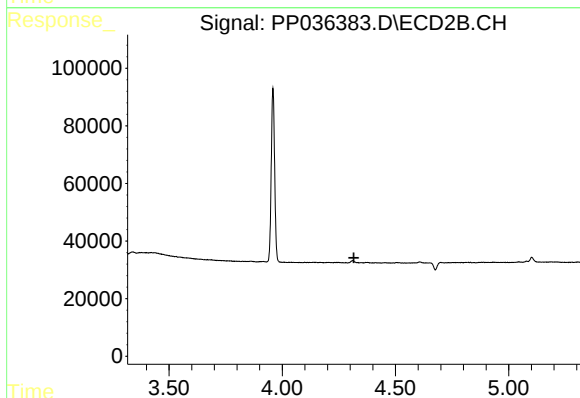


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

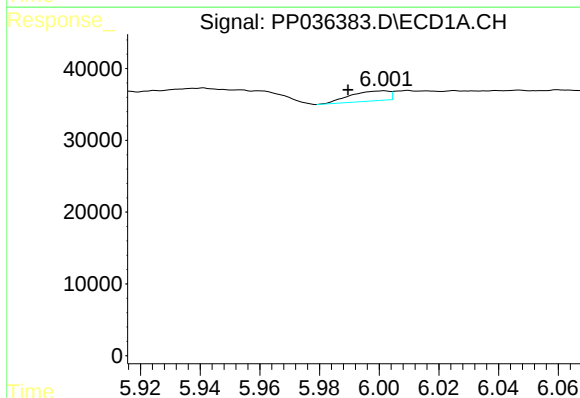


#12 AR-1232-2

R.T.: 6.002 min
Delta R.T.: 0.012 min
Response: 12701
Conc: 26.57 ng/ml

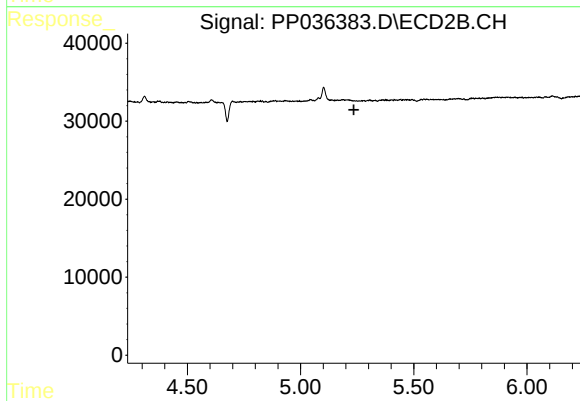

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.235 min
Response: 0
Conc: N.D.

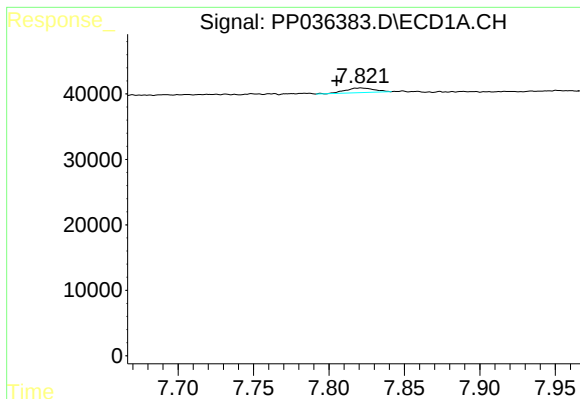

#28 AR-1254-3


R.T.: 7.821 min
Delta R.T.: 0.016 min
Response: 9543
Conc: 3.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

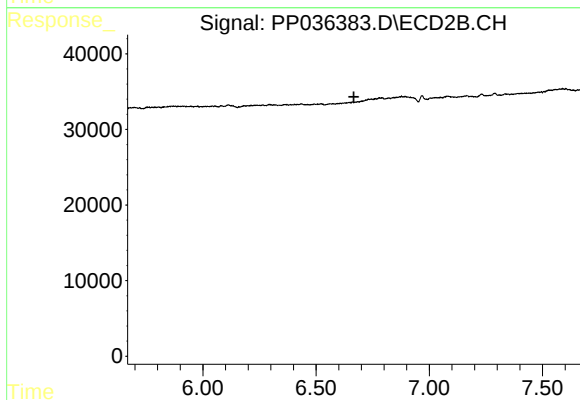


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

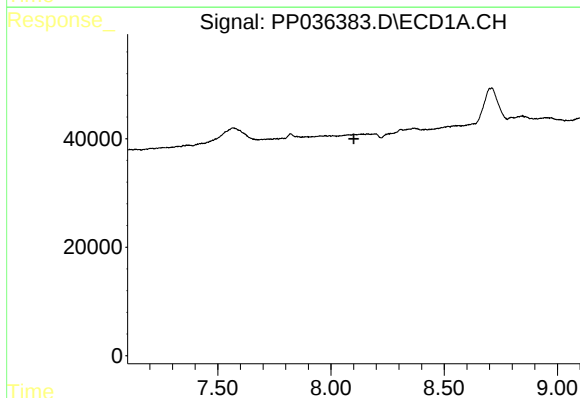


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 8.101 min
Response: 0
Conc: N.D.

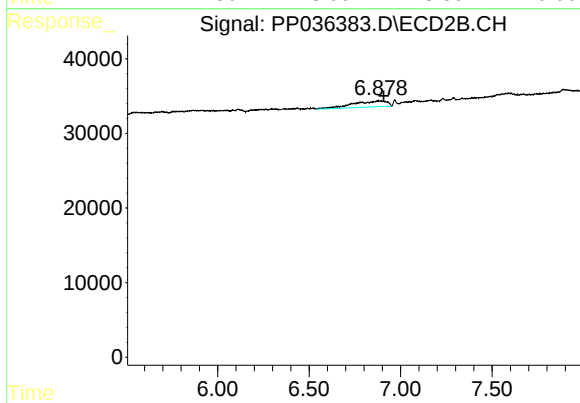

#29 AR-1254-4


R.T.: 6.878 min
Delta R.T.: -0.030 min
Response: 102629
Conc: 65.20 ng/ml

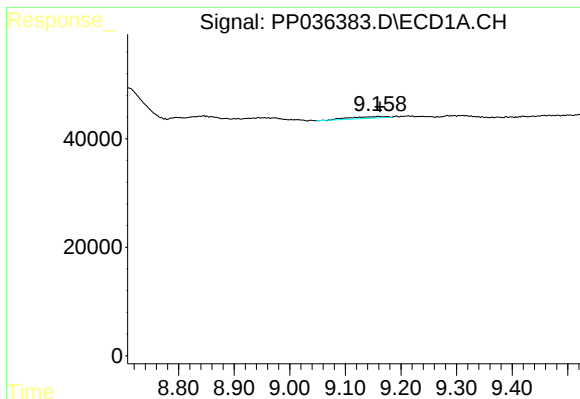

#35 AR-1260-5


R.T.: 9.159 min
Delta R.T.: -0.004 min
Response: 14432
Conc: 3.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

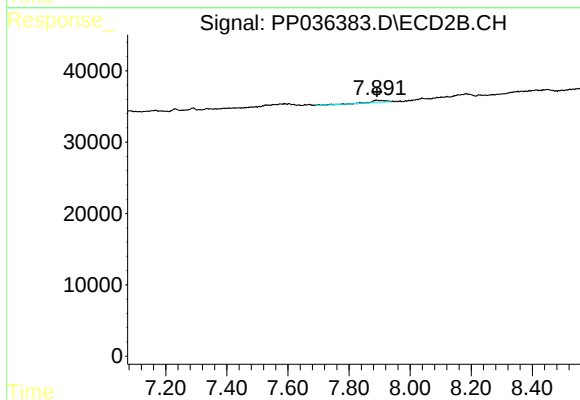


#35 AR-1260-5

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 9291
Conc: 2.51 ng/ml

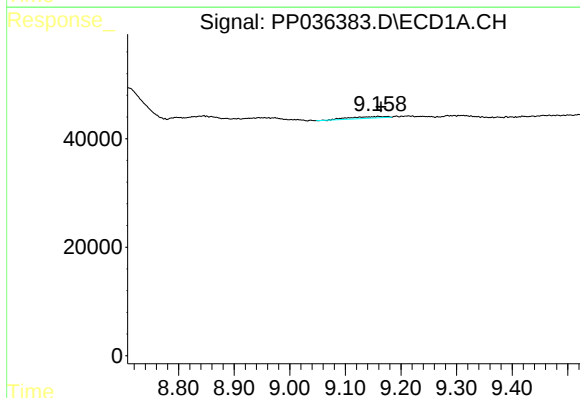


#37 AR-1262-2

R.T.: 9.159 min
Delta R.T.: -0.005 min
Response: 14432
Conc: 3.02 ng/ml

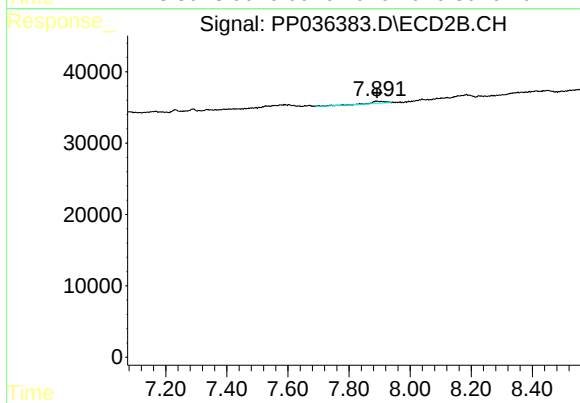

#37 AR-1262-2


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 9291
Conc: 2.24 ng/ml

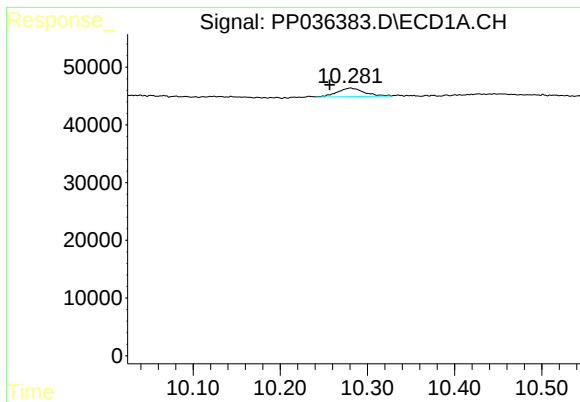

#44 AR-1268-4

R.T.: 10.281 min
Delta R.T.: 0.024 min
Response: 31722
Conc: 16.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

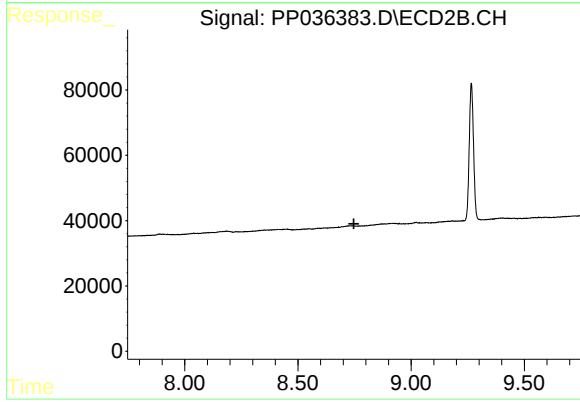

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.747 min
Response: 0
Conc: N.D.