

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
 Data File : PP036386.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 10:01
 Operator : DD\AJ
 Sample : M2673-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:42:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.960	992500	710819	23.505	23.665
2)	SA Decachlor...	11.000	9.267	902659	696561	24.998	21.804
Target Compounds							
8)	L2 AR-1221-1	5.222	0.000	173562	0	348.986	N.D. #
9)	L2 AR-1221-2	5.318	4.329	24797	50662	64.293	205.086 #
10)	L2 AR-1221-3	5.427f	0.000	79839	0	69.909	N.D. #
11)	L3 AR-1232-1	5.427f	0.000	79839	0	86.279	N.D. #
28)	L6 AR-1254-3	7.824f	0.000	9244	0	3.331	N.D. #
29)	L6 AR-1254-4	0.000	6.897	0	17045	N.D.	10.828 #
30)	L6 AR-1254-5	8.534	0.000	2508	0	1.077	N.D. #
44)	L9 AR-1268-4	10.281f	0.000	15544	0	7.941	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
Data File : PP036386.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 10:01
Operator : DD\AJ
Sample : M2673-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:42:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

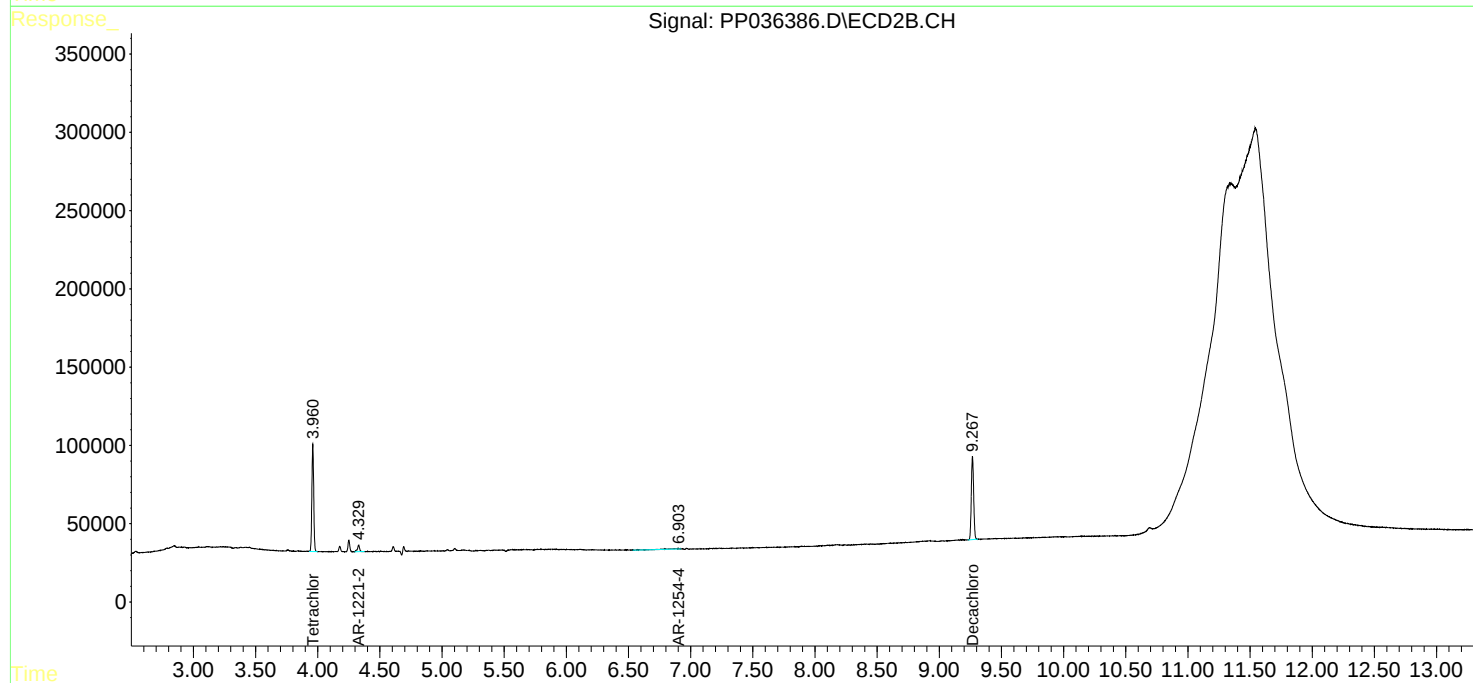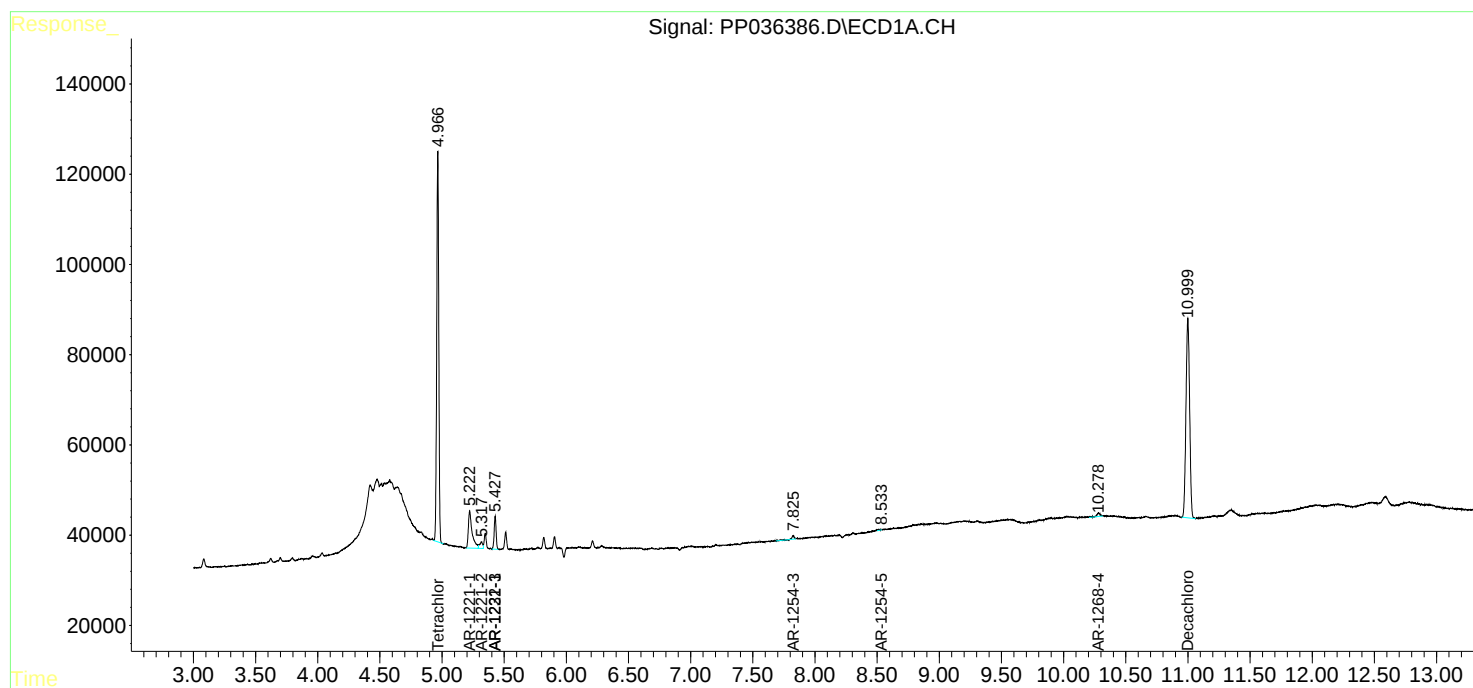


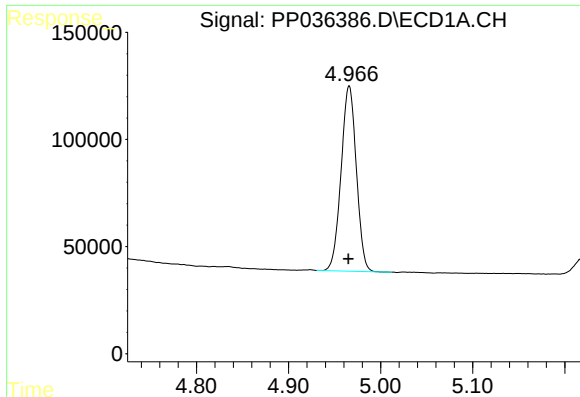

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 992500
Conc: 23.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

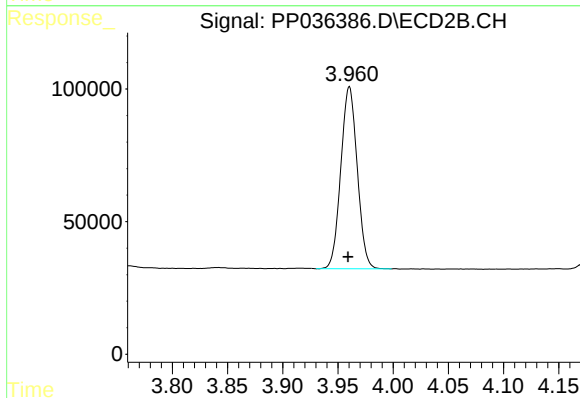


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.001 min
Response: 710819
Conc: 23.66 ng/ml

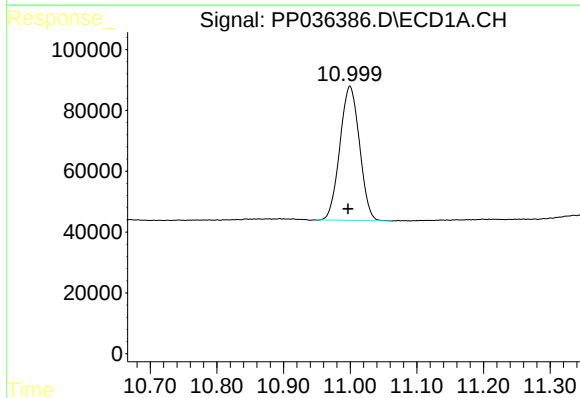


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.003 min
Response: 902659
Conc: 25.00 ng/ml

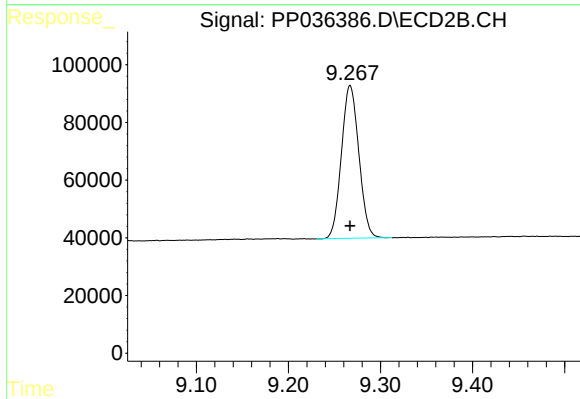

#2 Decachlorobiphenyl


R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 696561
Conc: 21.80 ng/ml

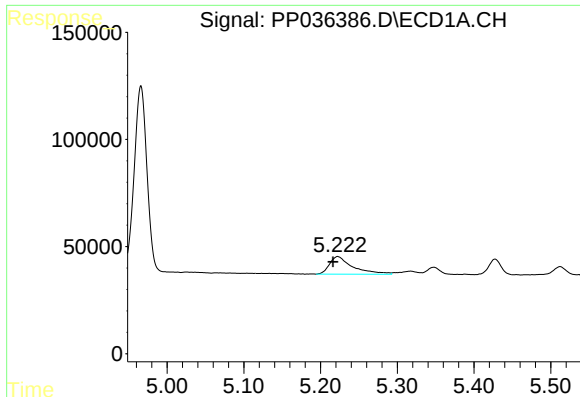

#8 AR-1221-1


R.T.: 5.222 min
Delta R.T.: 0.006 min
Response: 173562
Conc: 348.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

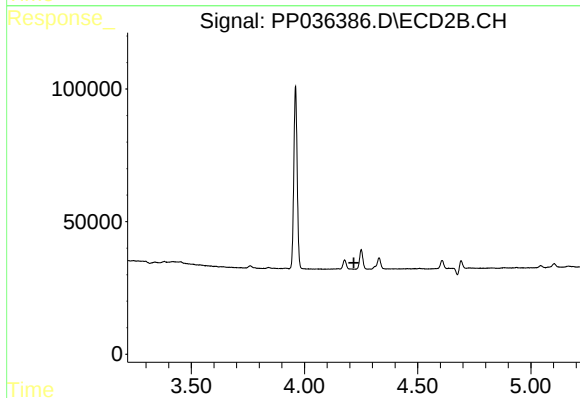


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

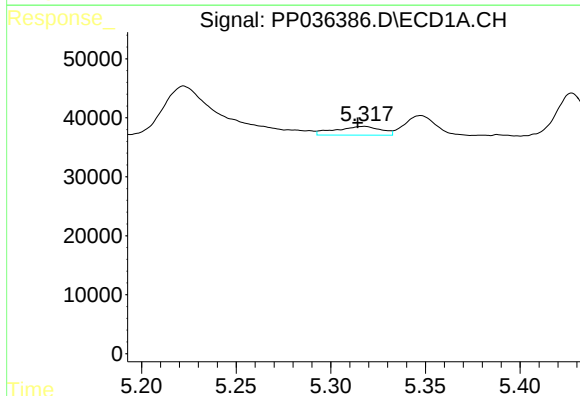


#9 AR-1221-2

R.T.: 5.318 min
Delta R.T.: 0.004 min
Response: 24797
Conc: 64.29 ng/ml

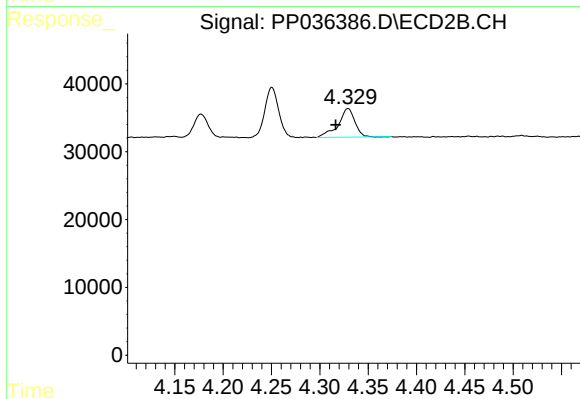

#9 AR-1221-2


R.T.: 4.329 min
Delta R.T.: 0.013 min
Response: 50662
Conc: 205.09 ng/ml

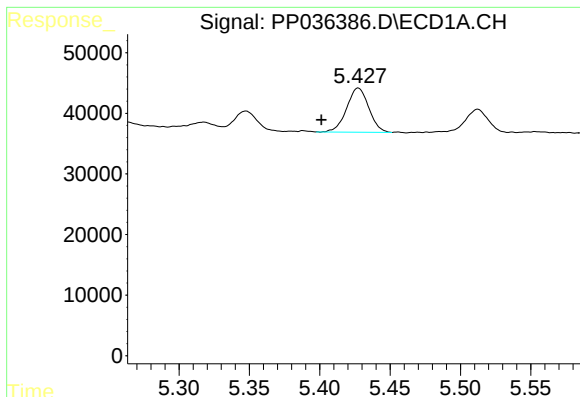

#10 AR-1221-3


R.T.: 5.427 min
Delta R.T.: 0.026 min
Response: 79839
Conc: 69.91 ng/ml

Instrument :
ECD_P
ClientSampleId :

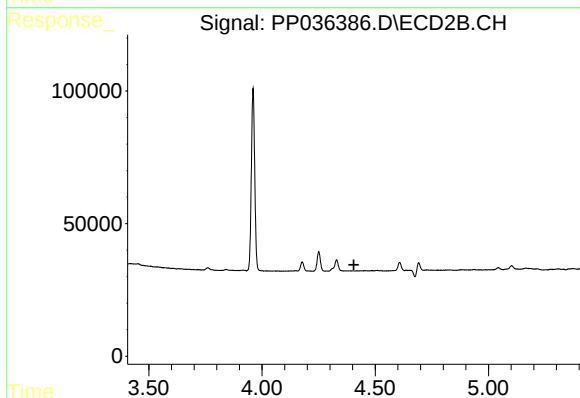


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.405 min
Response: 0
Conc: N.D.

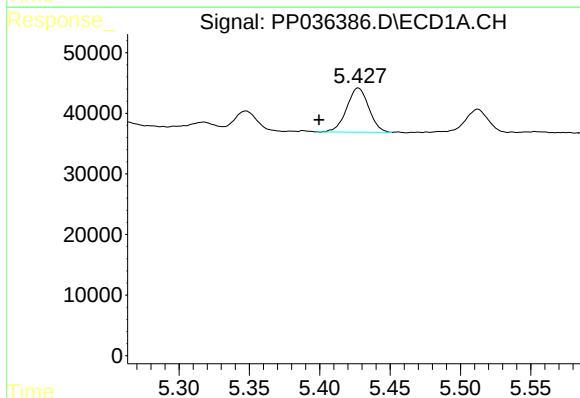


#11 AR-1232-1

R.T.: 5.427 min
Delta R.T.: 0.028 min
Response: 79839
Conc: 86.28 ng/ml

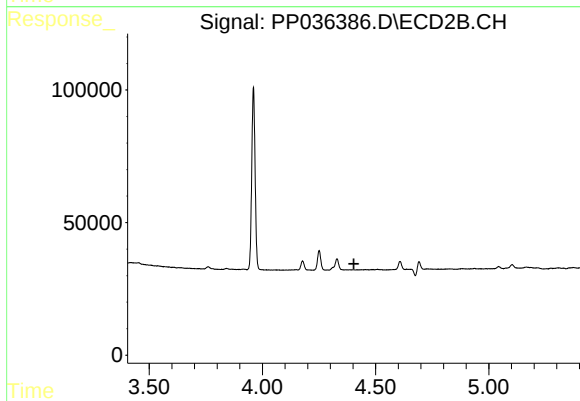

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

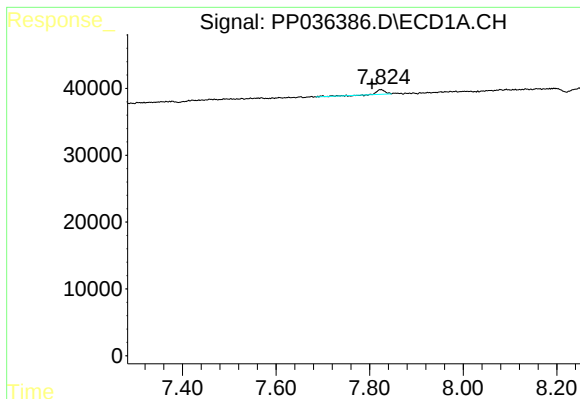

#28 AR-1254-3


R.T.: 7.824 min
Delta R.T.: 0.019 min
Response: 9244
Conc: 3.33 ng/ml

Instrument :
ECD_P
ClientSampleId :

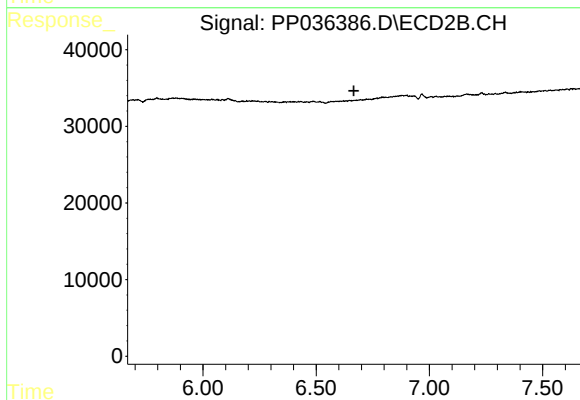


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

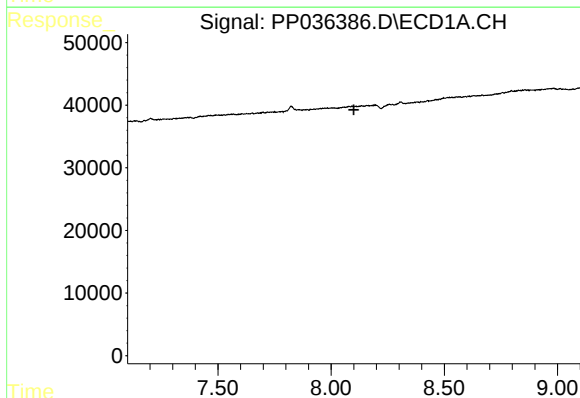


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 8.101 min
Response: 0
Conc: N.D.

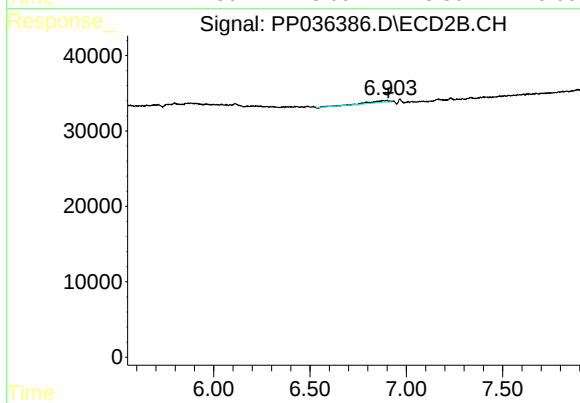

#29 AR-1254-4


R.T.: 6.897 min
Delta R.T.: -0.010 min
Response: 17045
Conc: 10.83 ng/ml

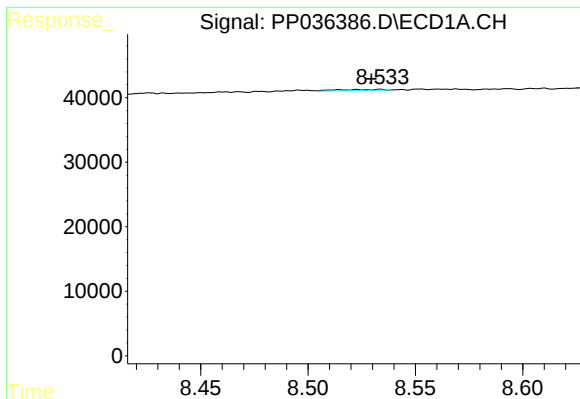

#30 AR-1254-5


R.T.: 8.534 min
Delta R.T.: 0.004 min
Response: 2508
Conc: 1.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

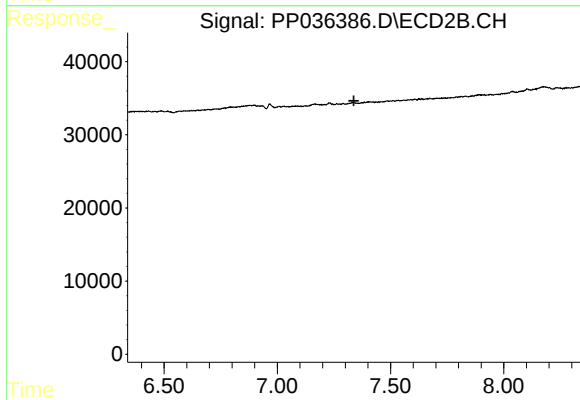


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

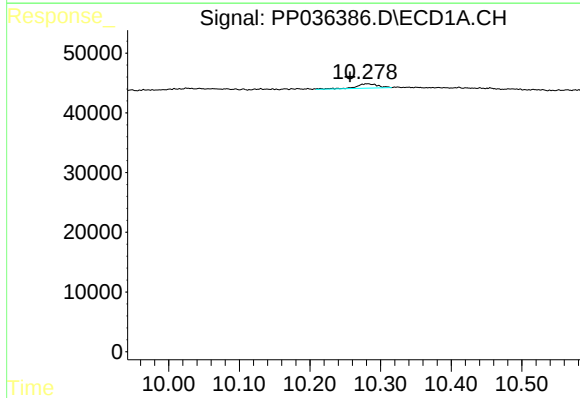

#44 AR-1268-4

R.T.: 10.281 min
Delta R.T.: 0.024 min
Response: 15544
Conc: 7.94 ng/ml

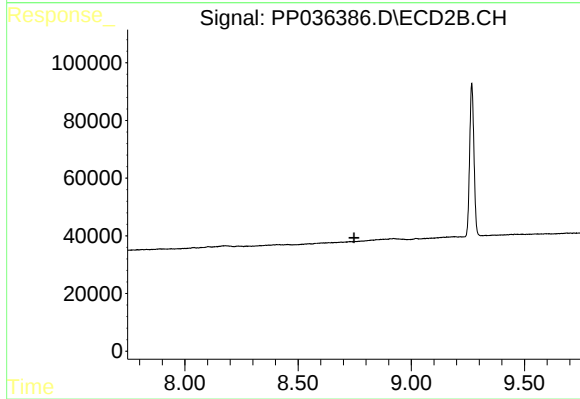

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.747 min
Response: 0
Conc: N.D.