

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
 Data File : PP036401.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 14:29
 Operator : DD\AJ
 Sample : M2676-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:48:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.959	922728	651768	21.853	21.699
2)	SA Decachlor...	10.998	9.265	903269	686953	25.014	21.503
Target Compounds							
8)	L2 AR-1221-1	5.218	0.000	189097	0	380.222	N.D. #
9)	L2 AR-1221-2	5.316	0.000	18643	0	48.336	N.D. #
28)	L6 AR-1254-3	7.822f	0.000	9918	0	3.573	N.D. #
39)	L8 AR-1262-4	9.565	8.246	2132	7426	0.795	2.367 #
41)	L9 AR-1268-1	9.508f	0.000	15563	0	2.988	N.D. #
42)	L9 AR-1268-2	9.565f	8.246	2132	7426	0.433	1.726 #
44)	L9 AR-1268-4	10.280f	0.000	14420	0	7.366	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
Data File : PP036401.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 14:29
Operator : DD\AJ
Sample : M2676-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:48:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

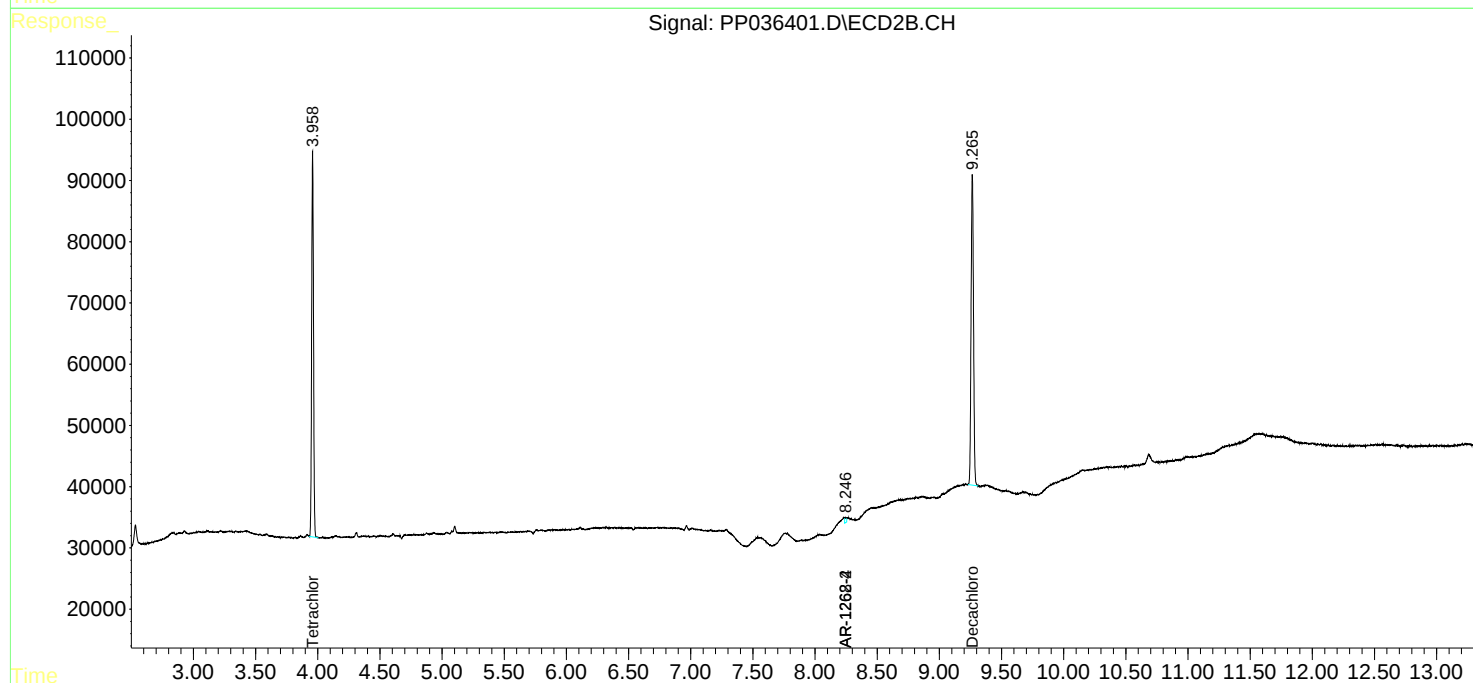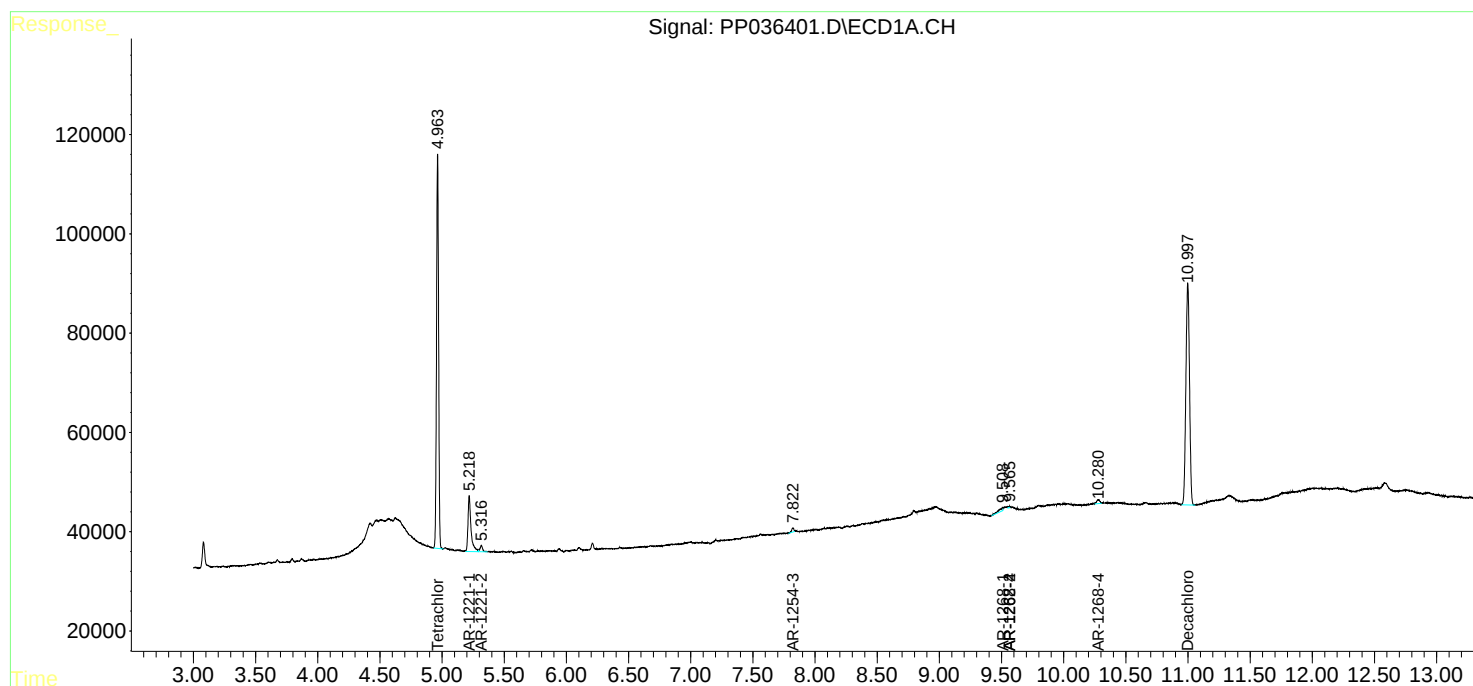


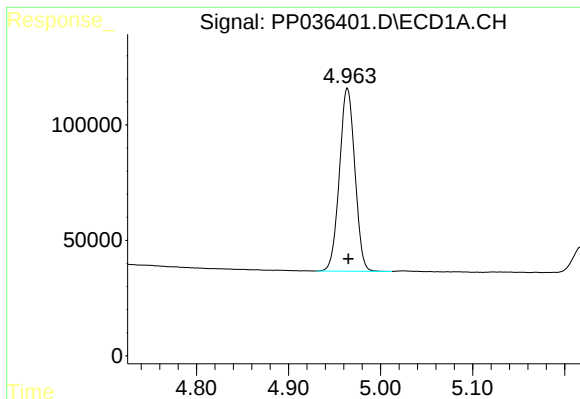

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 922728
Conc: 21.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

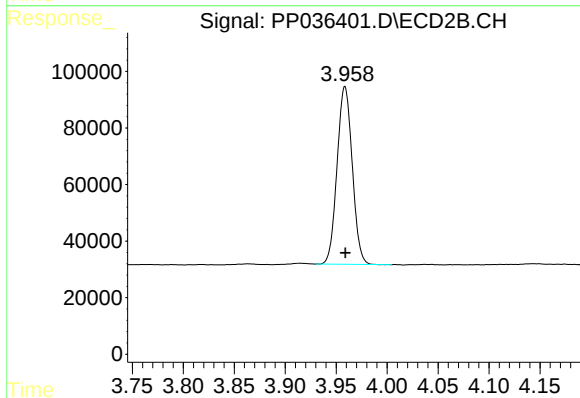


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 651768
Conc: 21.70 ng/ml

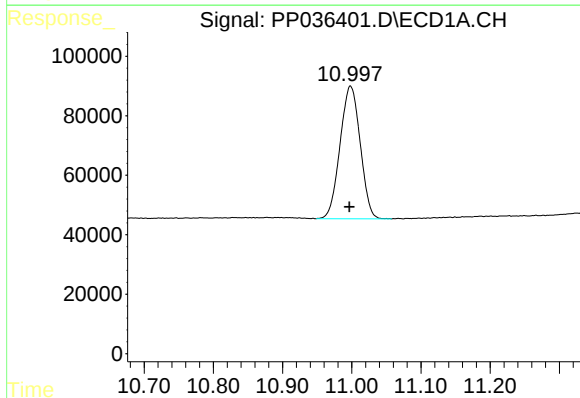


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.001 min
Response: 903269
Conc: 25.01 ng/ml

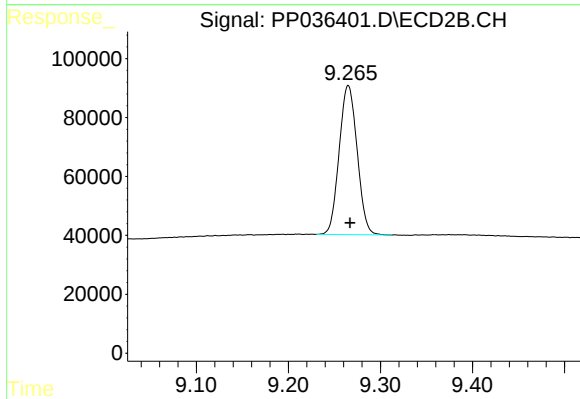

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 686953
Conc: 21.50 ng/ml

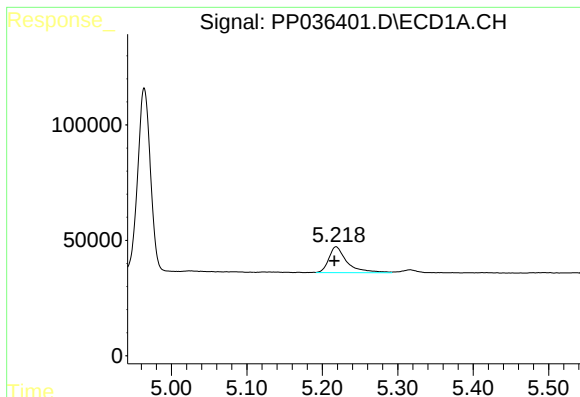

#8 AR-1221-1


R.T.: 5.218 min
Delta R.T.: 0.002 min
Response: 189097
Conc: 380.22 ng/ml

Instrument :
ECD_P
ClientSampleId :

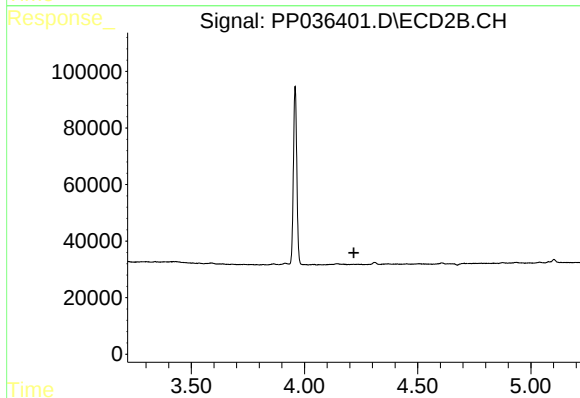


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

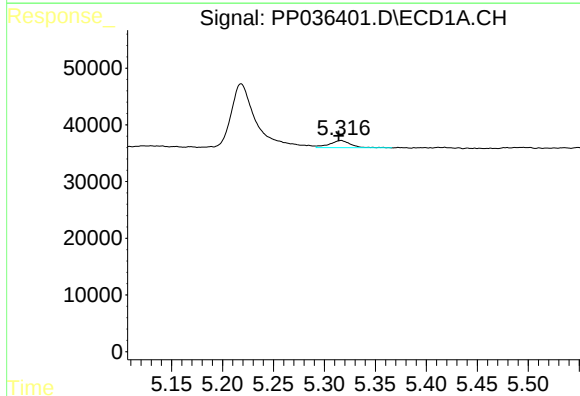


#9 AR-1221-2

R.T.: 5.316 min
Delta R.T.: 0.002 min
Response: 18643
Conc: 48.34 ng/ml

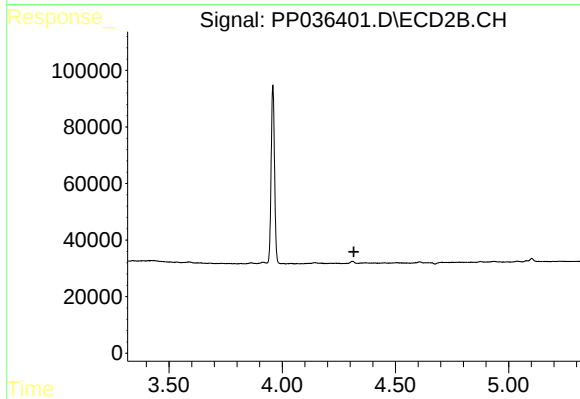

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

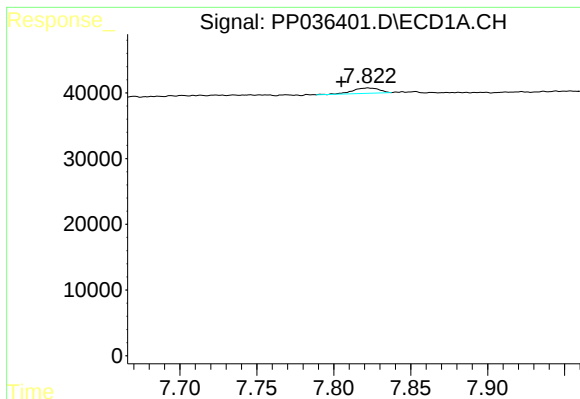

#28 AR-1254-3


R.T.: 7.822 min
Delta R.T.: 0.017 min
Response: 9918
Conc: 3.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

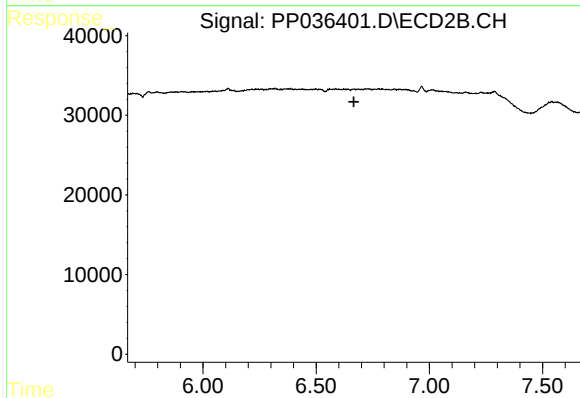


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

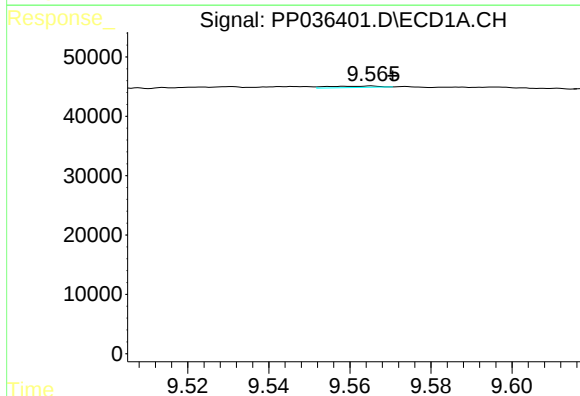


#39 AR-1262-4

R.T.: 9.565 min
Delta R.T.: -0.005 min
Response: 2132
Conc: 0.80 ng/ml

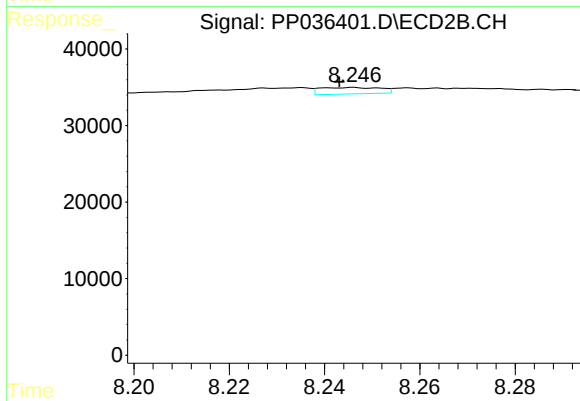

#39 AR-1262-4


R.T.: 8.246 min
Delta R.T.: 0.003 min
Response: 7426
Conc: 2.37 ng/ml

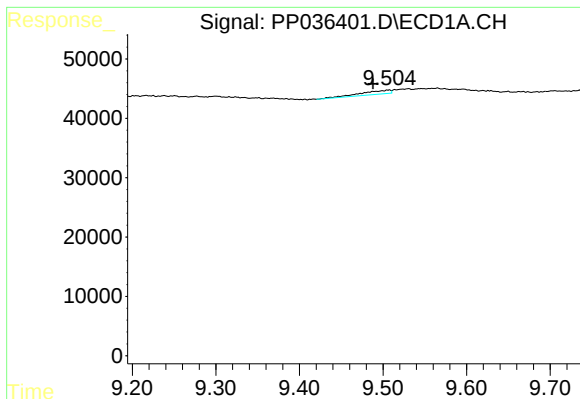

#41 AR-1268-1


R.T.: 9.508 min
Delta R.T.: 0.020 min
Response: 15563
Conc: 2.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

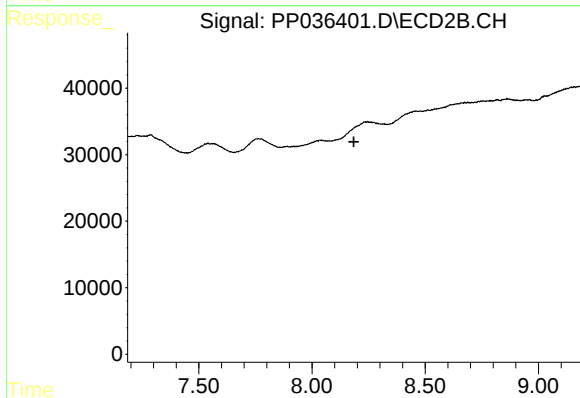


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.185 min
Response: 0
Conc: N.D.

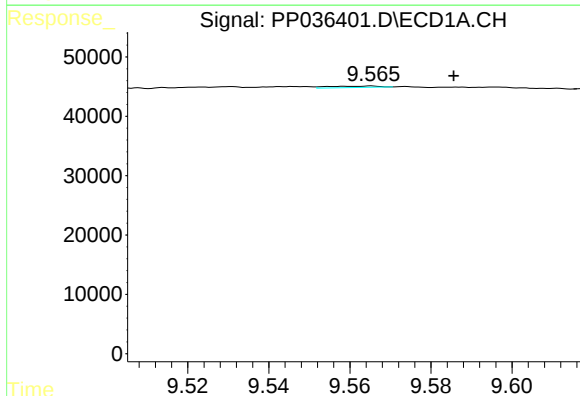


#42 AR-1268-2

R.T.: 9.565 min
Delta R.T.: -0.020 min
Response: 2132
Conc: 0.43 ng/ml

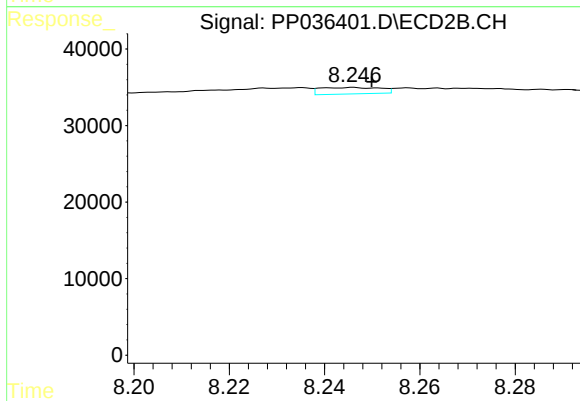

#42 AR-1268-2


R.T.: 8.246 min
Delta R.T.: -0.004 min
Response: 7426
Conc: 1.73 ng/ml

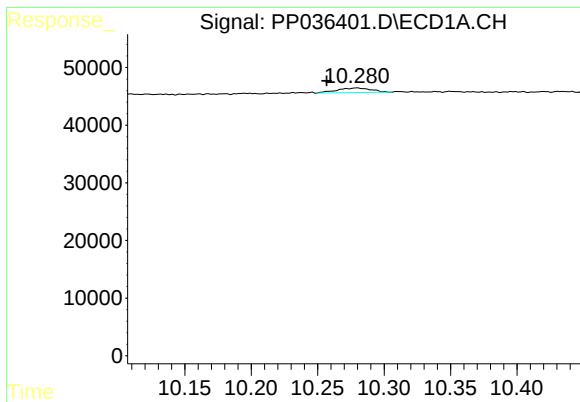

#44 AR-1268-4

R.T.: 10.280 min
Delta R.T.: 0.023 min
Response: 14420
Conc: 7.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

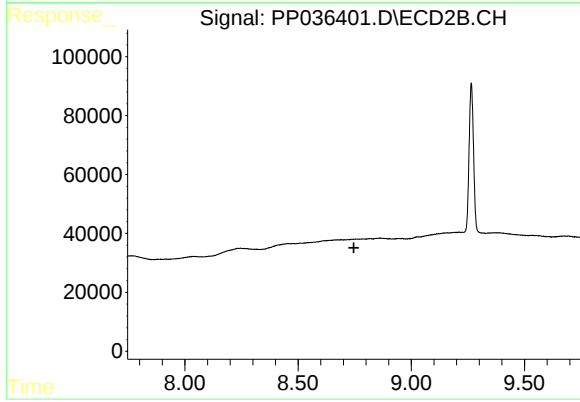

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.747 min
Response: 0
Conc: N.D.