

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
 Data File : PP036402.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 14:46
 Operator : DD\AJ
 Sample : M2676-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:48:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.959	884408	620756	20.946	20.666
2)	SA Decachlor...	10.998	9.265	889135	653316	24.623	20.450
Target Compounds							
8)	L2 AR-1221-1	5.219	0.000	59726	0	120.093	N.D. #
9)	L2 AR-1221-2	5.316	4.310	13902	7501	36.046	30.366
38)	L8 AR-1262-3	0.000	8.192	0	19070	N.D.	11.131 #
39)	L8 AR-1262-4	0.000	8.243	0	32864	N.D.	10.476 #
41)	L9 AR-1268-1	9.509f	8.192	6738	19070	1.294	4.130 #
42)	L9 AR-1268-2	0.000	8.243	0	32864	N.D.	7.640 #
44)	L9 AR-1268-4	10.274f	0.000	23158	0	11.830	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
Data File : PP036402.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 14:46
Operator : DD\AJ
Sample : M2676-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:48:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

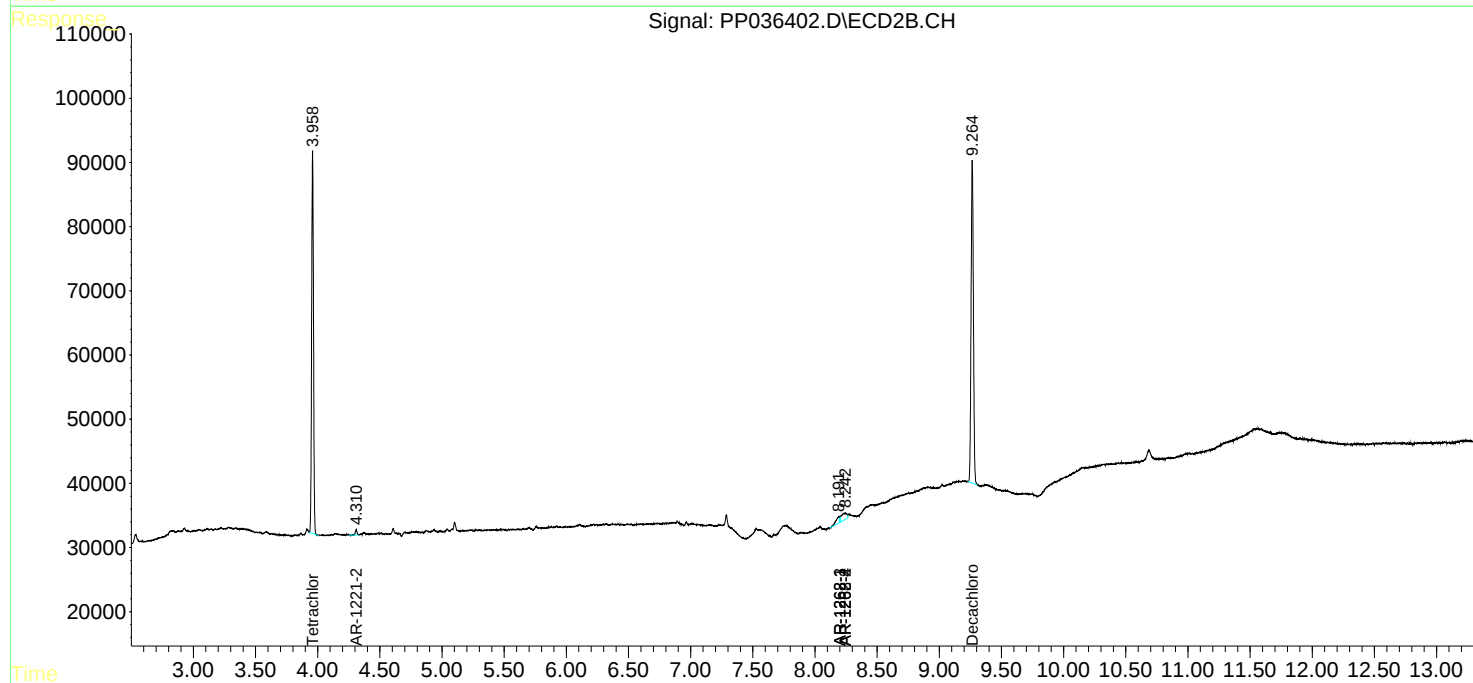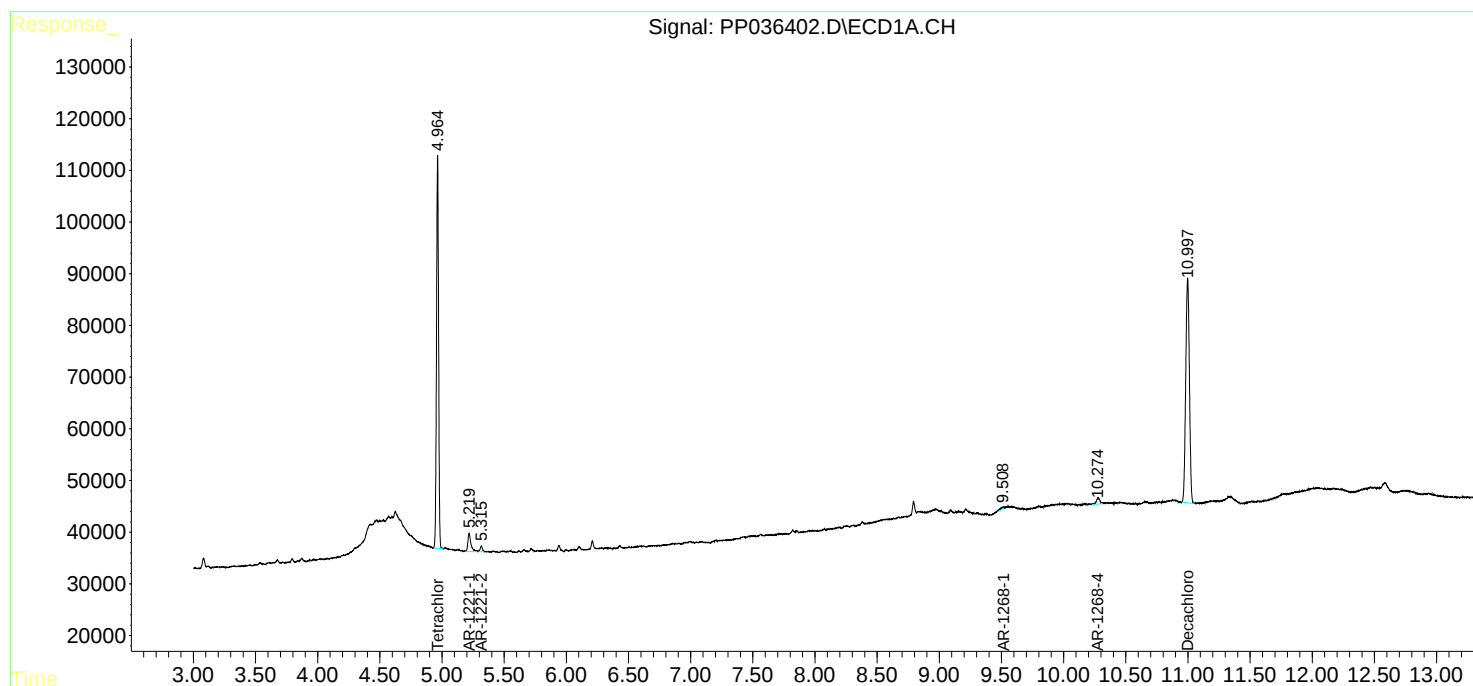


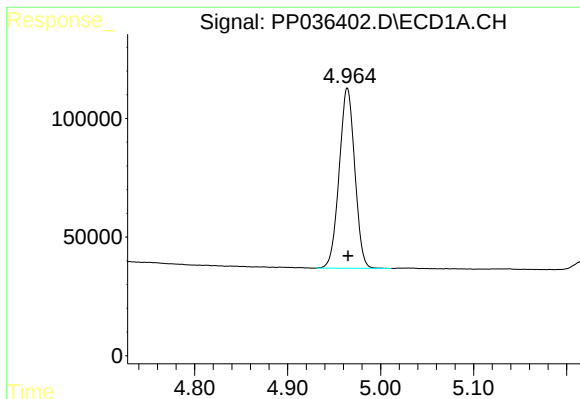

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 884408
Conc: 20.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

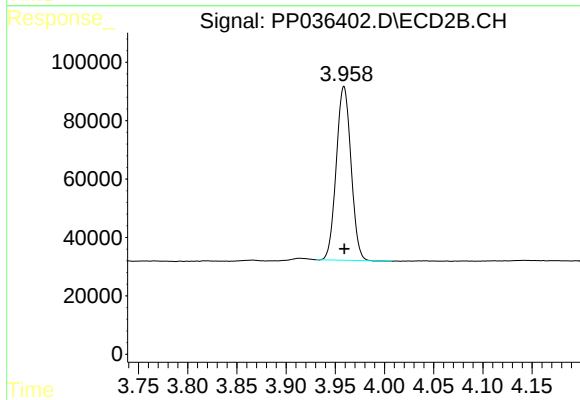


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 620756
Conc: 20.67 ng/ml

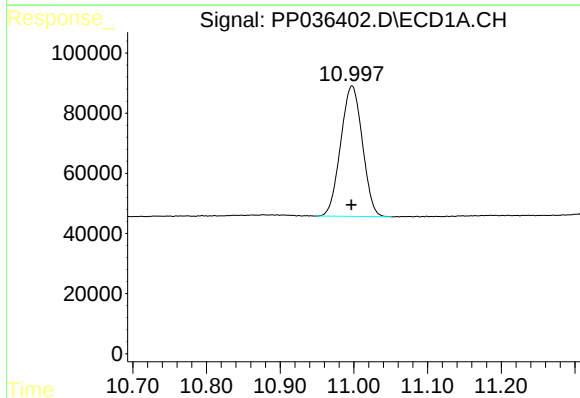


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 889135
Conc: 24.62 ng/ml

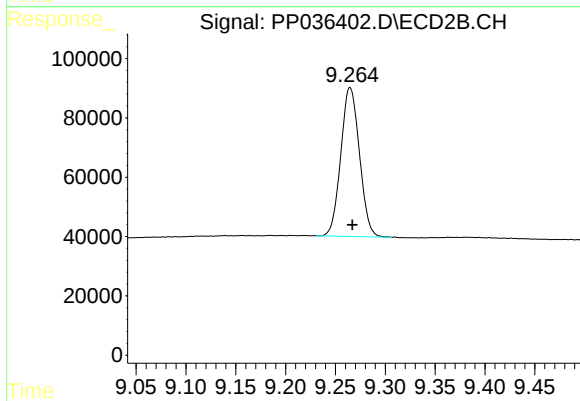

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 653316
Conc: 20.45 ng/ml

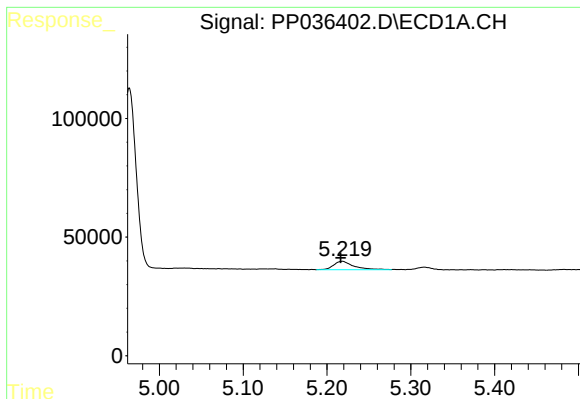

#8 AR-1221-1


R.T.: 5.219 min
Delta R.T.: 0.002 min
Response: 59726
Conc: 120.09 ng/ml

Instrument :
ECD_P
ClientSampleId :

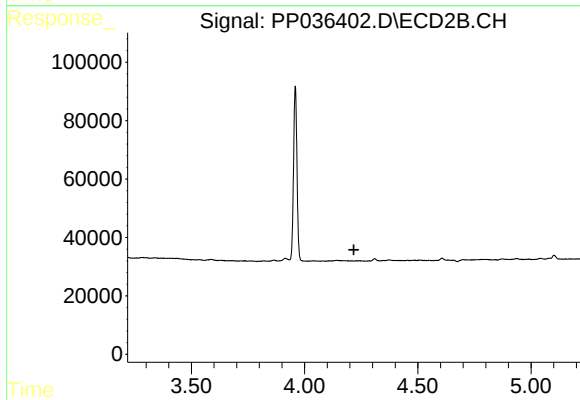


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

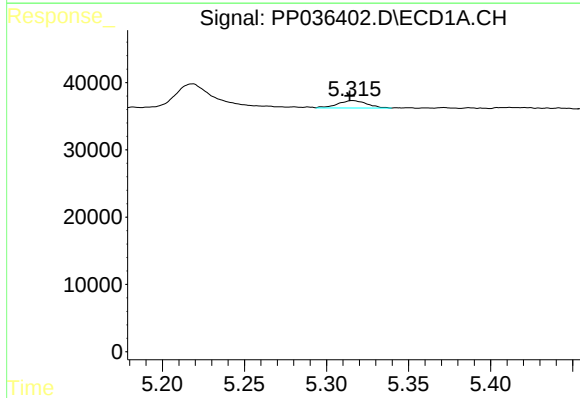


#9 AR-1221-2

R.T.: 5.316 min
Delta R.T.: 0.002 min
Response: 13902
Conc: 36.05 ng/ml

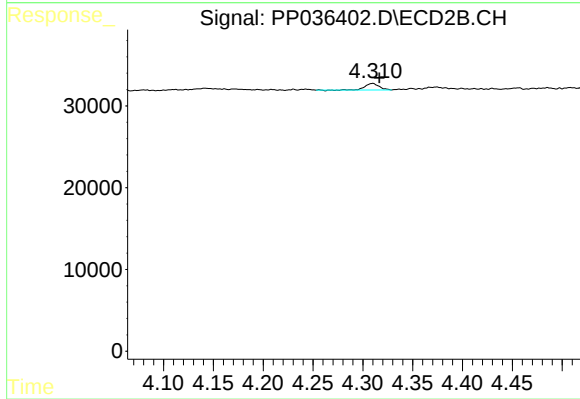

#9 AR-1221-2


R.T.: 4.310 min
Delta R.T.: -0.006 min
Response: 7501
Conc: 30.37 ng/ml

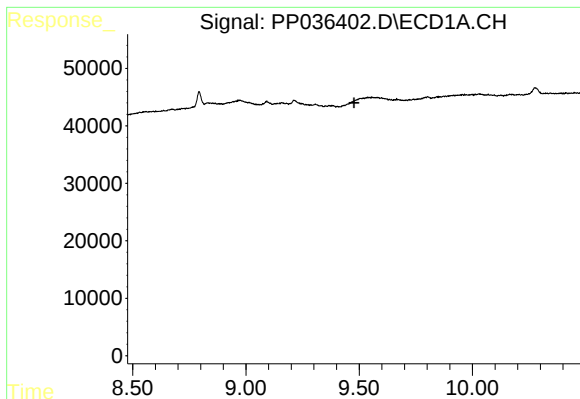

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

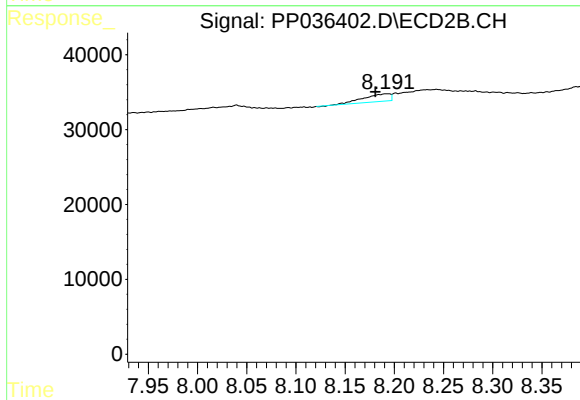


#38 AR-1262-3

R.T.: 8.192 min
Delta R.T.: 0.011 min
Response: 19070
Conc: 11.13 ng/ml

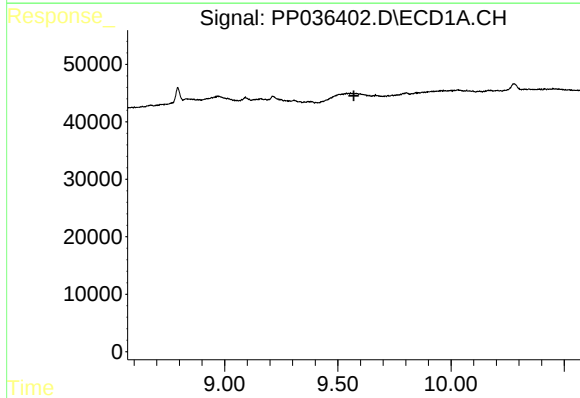


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

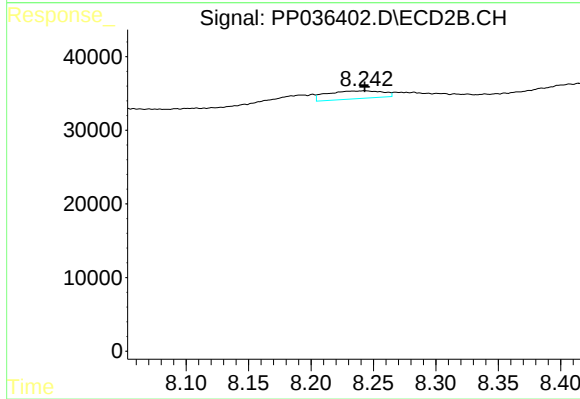

#39 AR-1262-4


R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 32864
Conc: 10.48 ng/ml

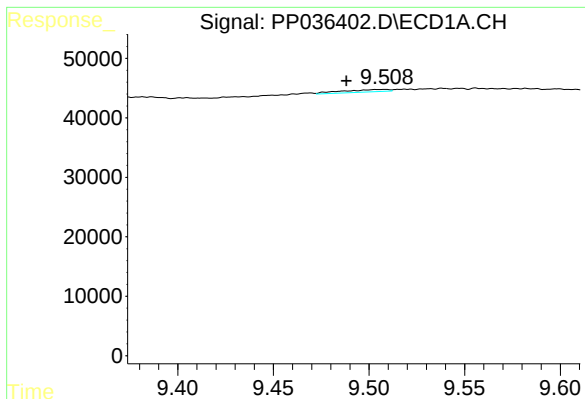

#41 AR-1268-1


R.T.: 9.509 min
Delta R.T.: 0.020 min
Response: 6738
Conc: 1.29 ng/ml

Instrument :
ECD_P
ClientSampleId :

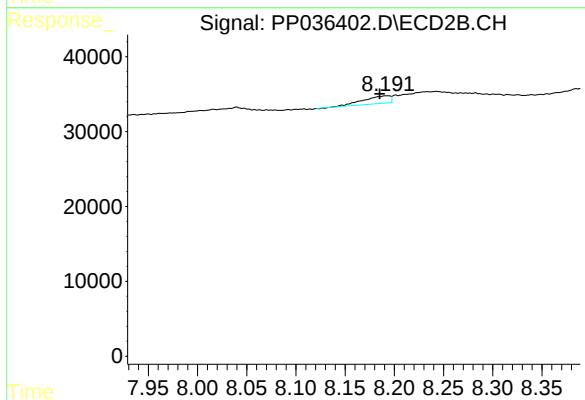


#41 AR-1268-1

R.T.: 8.192 min
Delta R.T.: 0.006 min
Response: 19070
Conc: 4.13 ng/ml

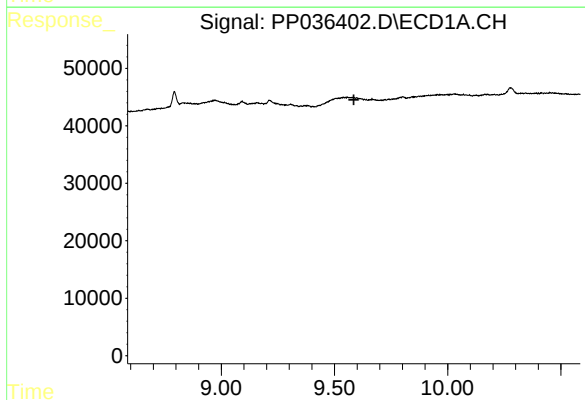


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.586 min
Response: 0
Conc: N.D.

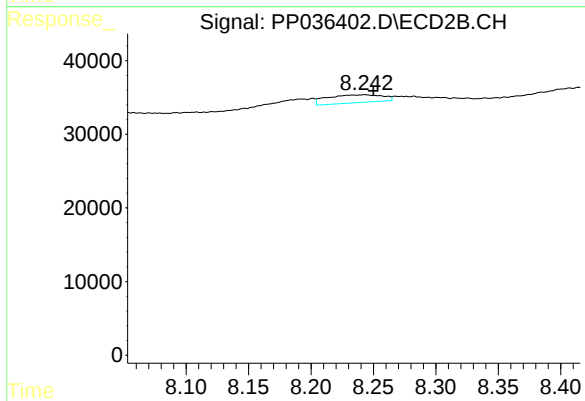

#42 AR-1268-2


R.T.: 8.243 min
Delta R.T.: -0.007 min
Response: 32864
Conc: 7.64 ng/ml

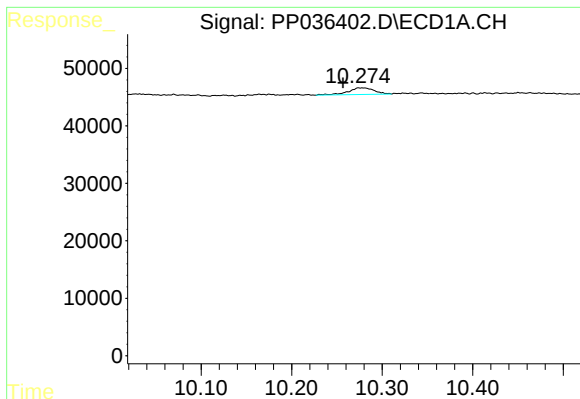

#44 AR-1268-4

R.T.: 10.274 min
Delta R.T.: 0.017 min
Response: 23158
Conc: 11.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

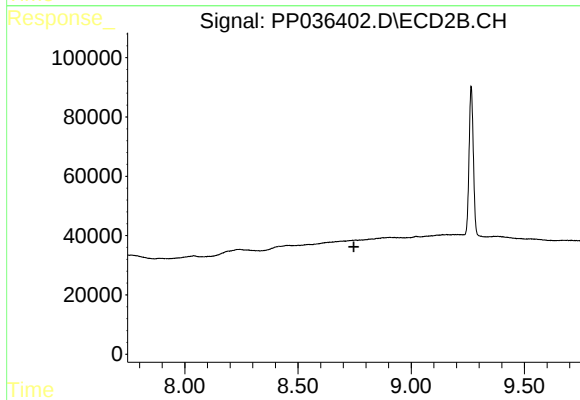

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.747 min
Response: 0
Conc: N.D.