

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
 Data File : PP036403.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 15:03
 Operator : DD\AJ
 Sample : M2676-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:49:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.959	918725	643636	21.758	21.428
2)	SA Decachlor...	10.998	9.265	912075	677494	25.258	21.207
Target Compounds							
8)	L2 AR-1221-1	5.219	0.000	42296	0	85.046	N.D. #
9)	L2 AR-1221-2	5.315	0.000	12655	0	32.812	N.D. #
28)	L6 AR-1254-3	7.823f	0.000	6599	0	2.377	N.D. #
30)	L6 AR-1254-5	8.531	0.000	2100	0	0.902	N.D. #
33)	L7 AR-1260-3	8.589	0.000	2546	0	1.456	N.D. #
34)	L7 AR-1260-4	8.827	0.000	6386	0	3.419	N.D. #
35)	L7 AR-1260-5	9.177	0.000	4222	0	1.125	N.D. #
36)	L8 AR-1262-1	8.589f	0.000	2546	0	0.947	N.D. #
37)	L8 AR-1262-2	9.177	0.000	4222	0	0.884	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061321\
Data File : PP036403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 15:03
Operator : DD\AJ
Sample : M2676-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:49:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

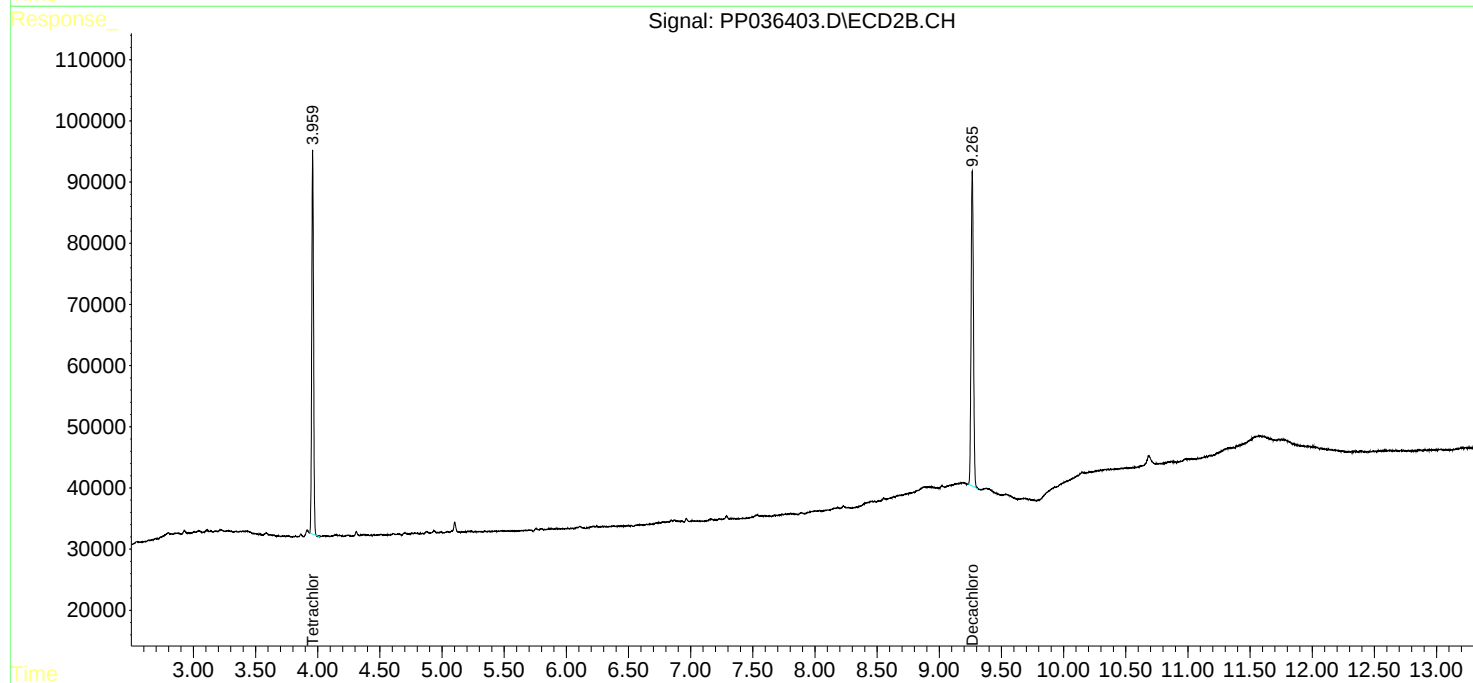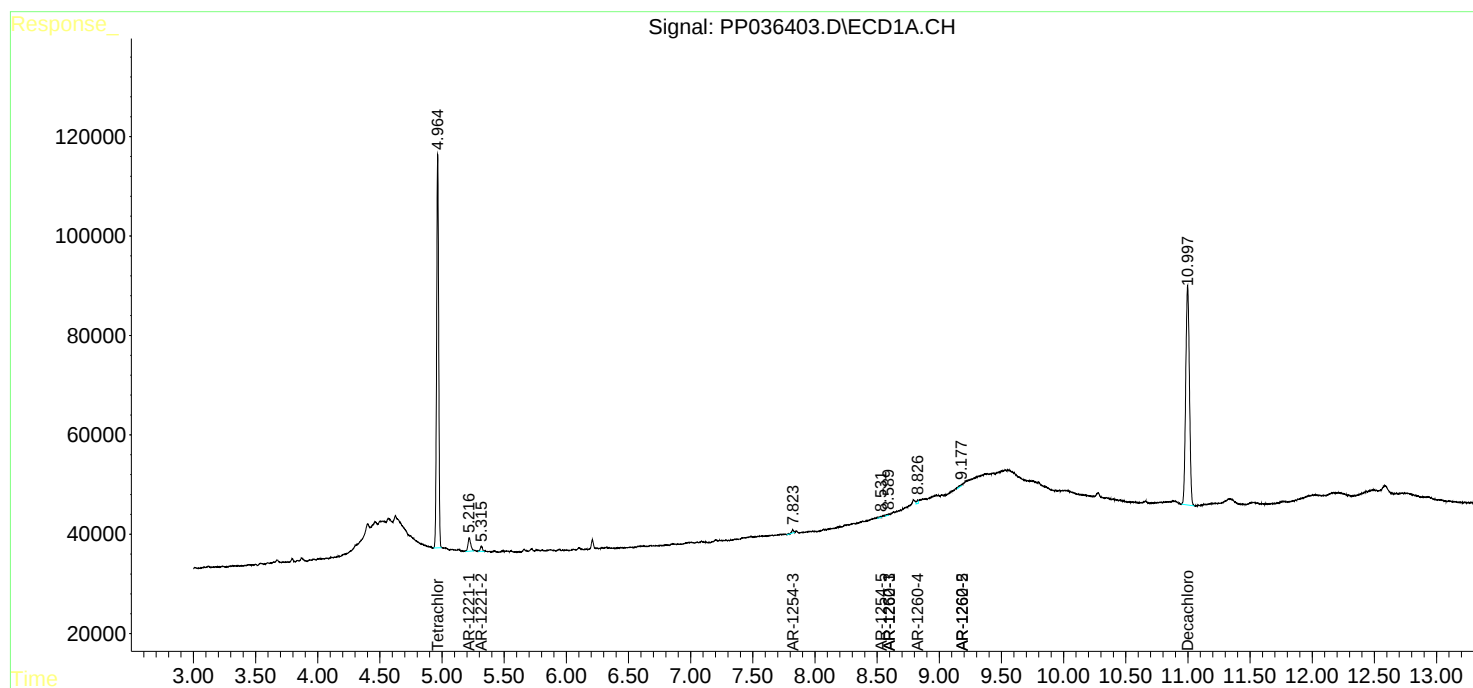


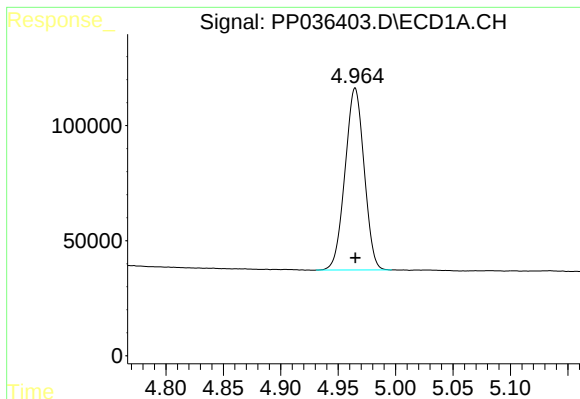

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 918725
Conc: 21.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

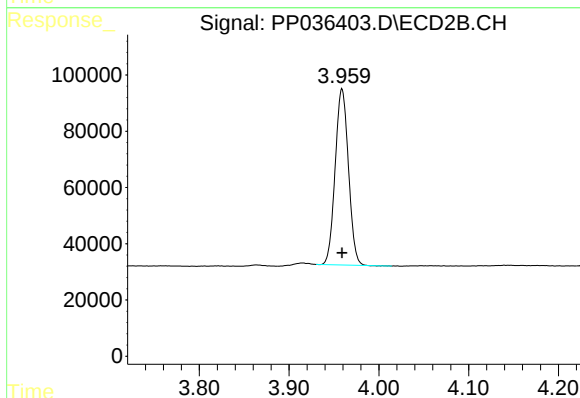


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 643636
Conc: 21.43 ng/ml

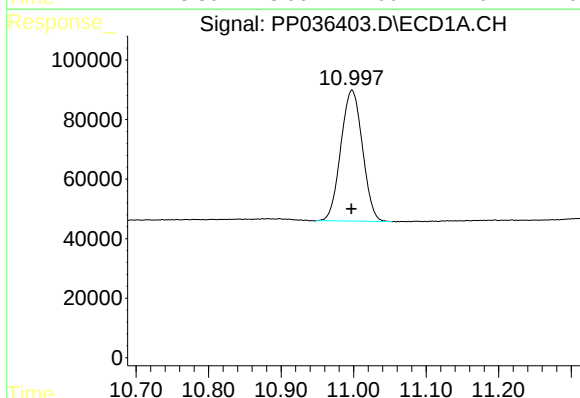


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 912075
Conc: 25.26 ng/ml

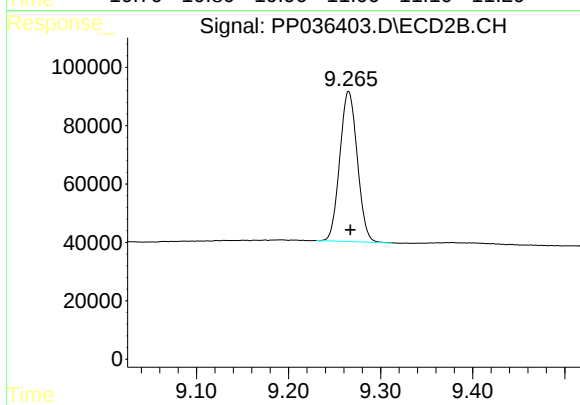

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 677494
Conc: 21.21 ng/ml

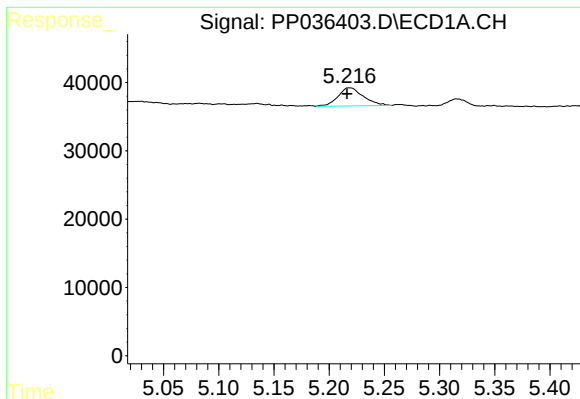

#8 AR-1221-1


R.T.: 5.219 min
Delta R.T.: 0.003 min
Response: 42296
Conc: 85.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

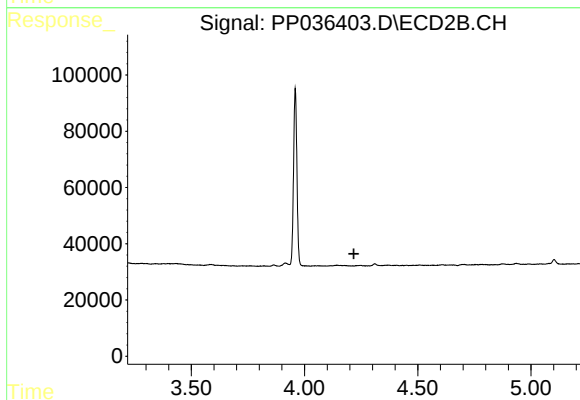


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

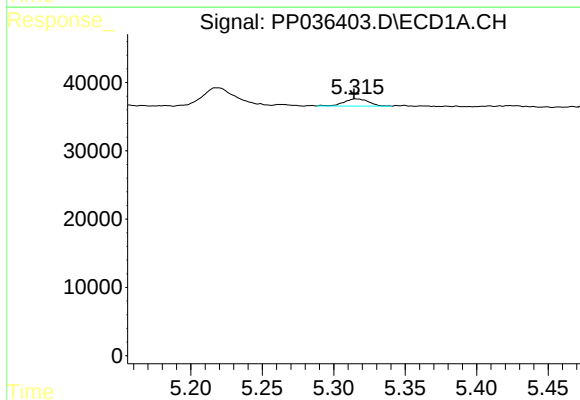


#9 AR-1221-2

R.T.: 5.315 min
Delta R.T.: 0.001 min
Response: 12655
Conc: 32.81 ng/ml

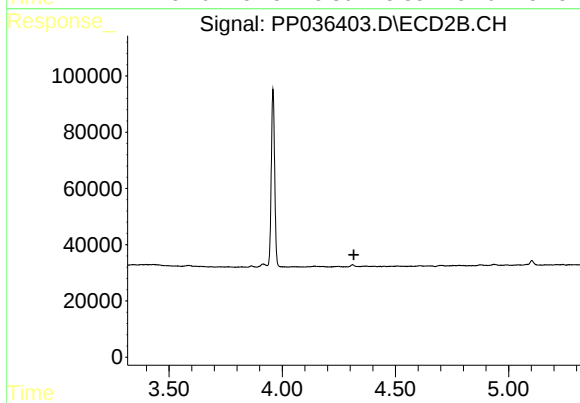

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

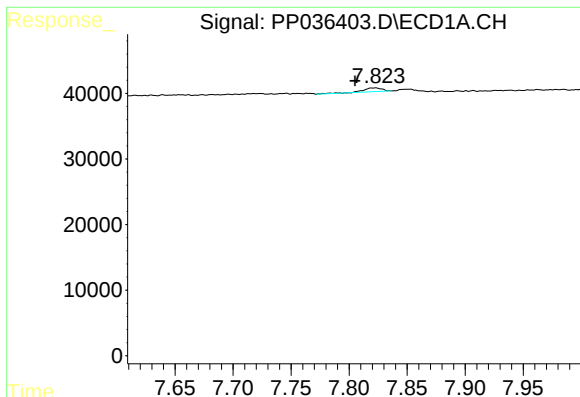

#28 AR-1254-3


R.T.: 7.823 min
Delta R.T.: 0.018 min
Response: 6599
Conc: 2.38 ng/ml

Instrument :
ECD_P
ClientSampleId :

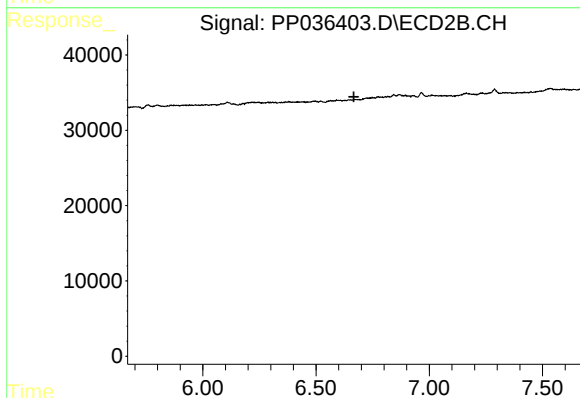


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

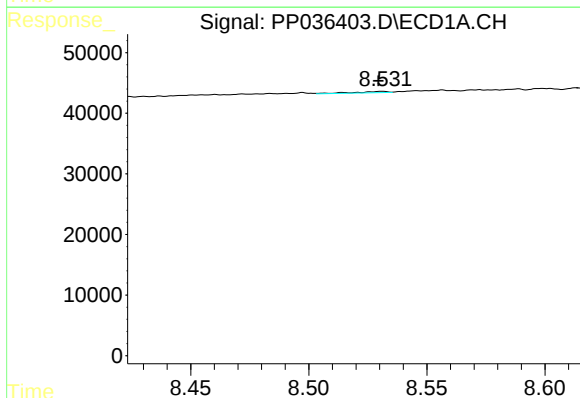


#30 AR-1254-5

R.T.: 8.531 min
Delta R.T.: 0.002 min
Response: 2100
Conc: 0.90 ng/ml

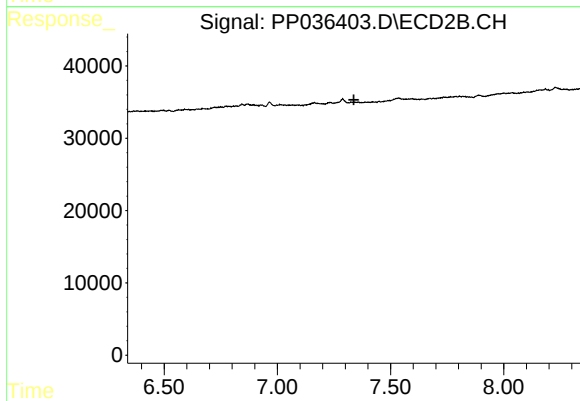

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

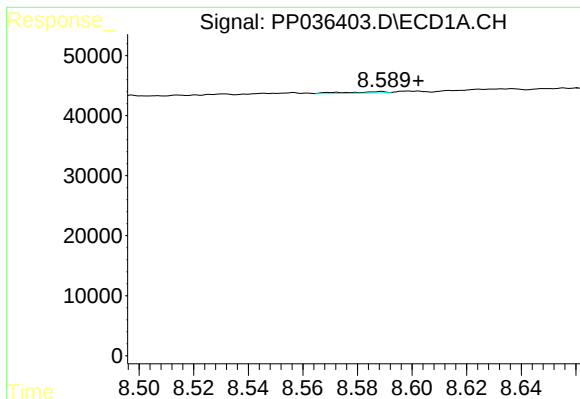

#33 AR-1260-3


R.T.: 8.589 min
Delta R.T.: -0.013 min
Response: 2546
Conc: 1.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

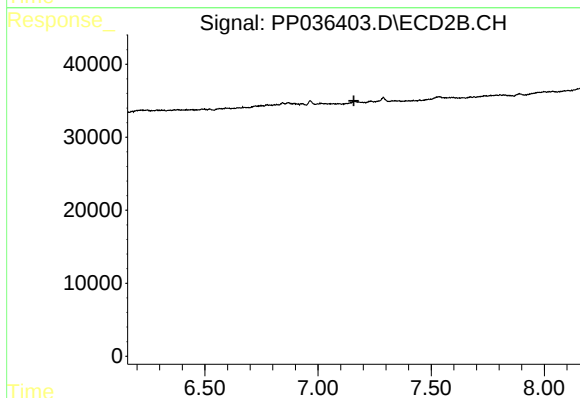


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

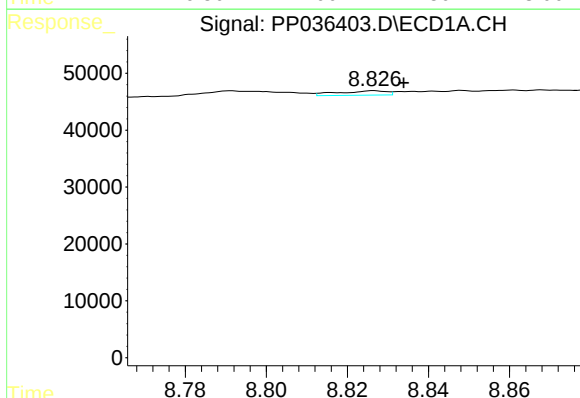


#34 AR-1260-4

R.T.: 8.827 min
Delta R.T.: -0.007 min
Response: 6386
Conc: 3.42 ng/ml

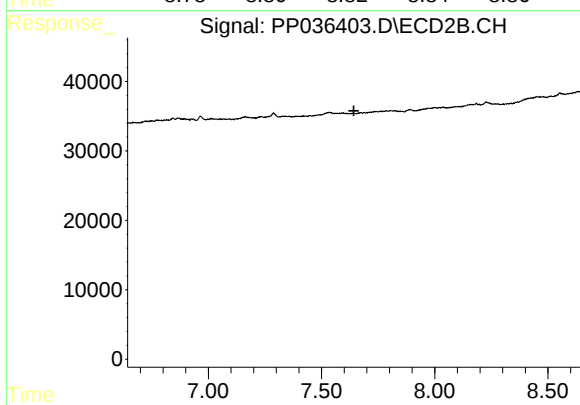

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.643 min
Response: 0
Conc: N.D.

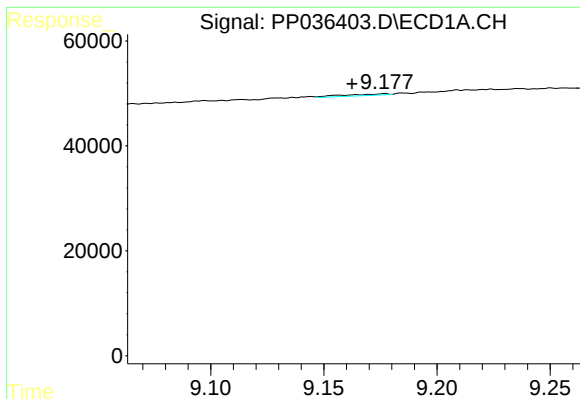

#35 AR-1260-5


R.T.: 9.177 min
Delta R.T.: 0.015 min
Response: 4222
Conc: 1.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

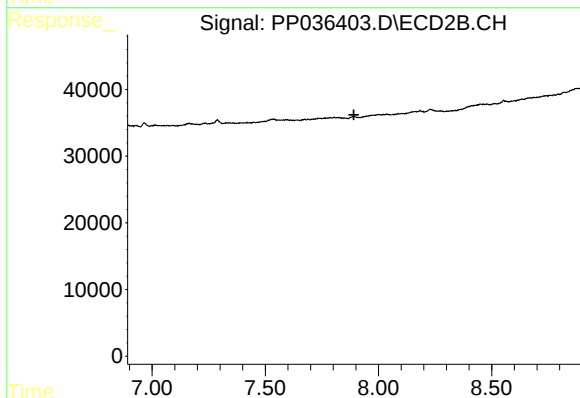


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.891 min
Response: 0
Conc: N.D.

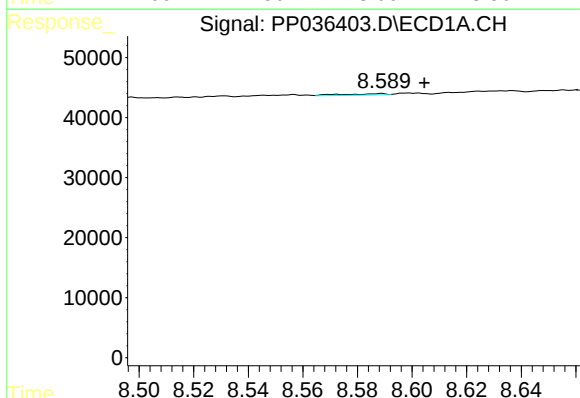


#36 AR-1262-1

R.T.: 8.589 min
Delta R.T.: -0.016 min
Response: 2546
Conc: 0.95 ng/ml

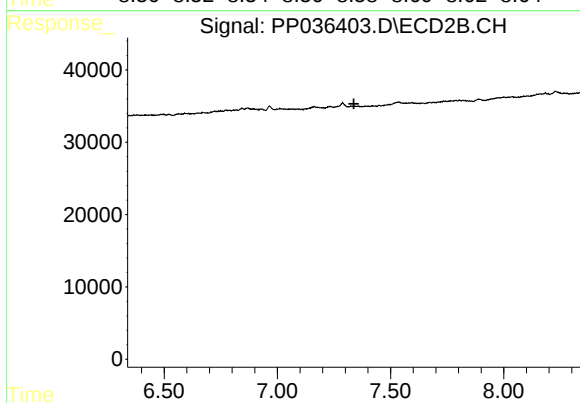

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

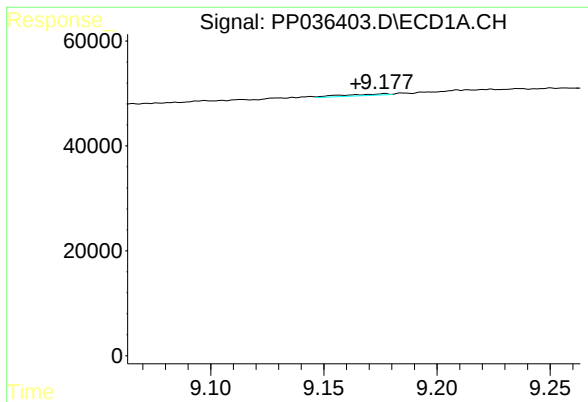

#37 AR-1262-2

R.T.: 9.177 min
Delta R.T.: 0.013 min
Response: 4222
Conc: 0.88 ng/ml

Instrument :
ECD_P
ClientSampleId :

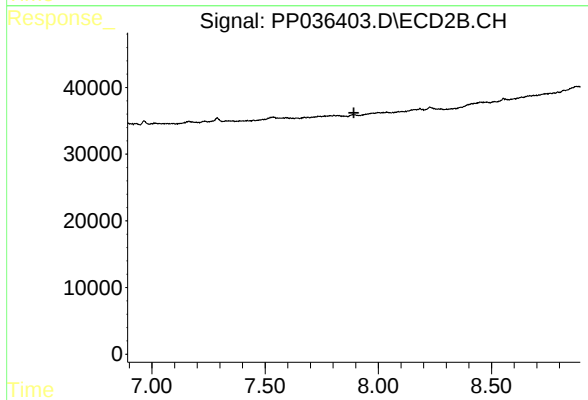

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.