

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061323\
 Data File : PP058444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2023 12:44
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 13:49:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 13 13:49:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.612	93194177	93289438	50.000	50.000
2) SA Decachlor...	10.194	8.668	34559641	68004109	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.583	3.828	9895820	11594157	500.000	500.000
9) L2 AR-1221-2	4.670	3.914	7405921	8847385	500.000	500.000
10) L2 AR-1221-3	4.747	3.991	20658363	25683468	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061323\
Data File : PP058444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2023 12:44
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 13:49:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 13 13:49:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

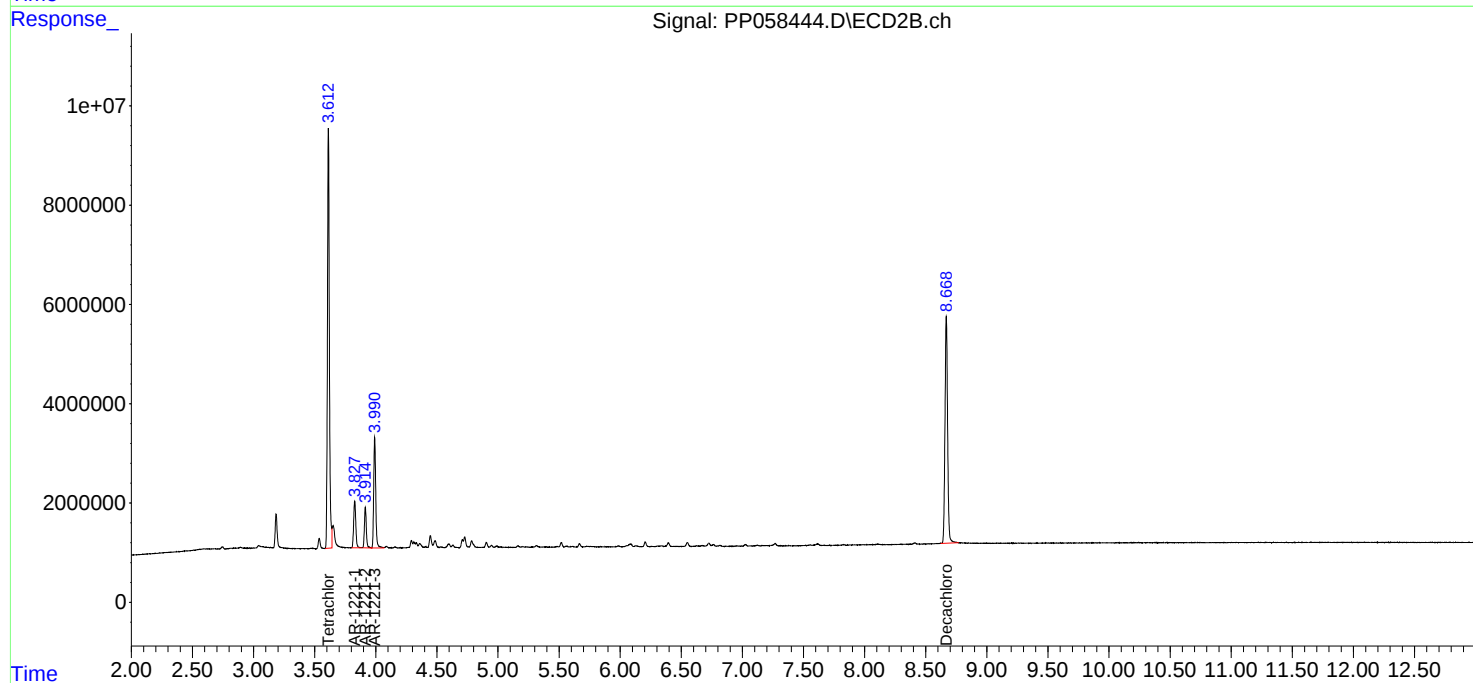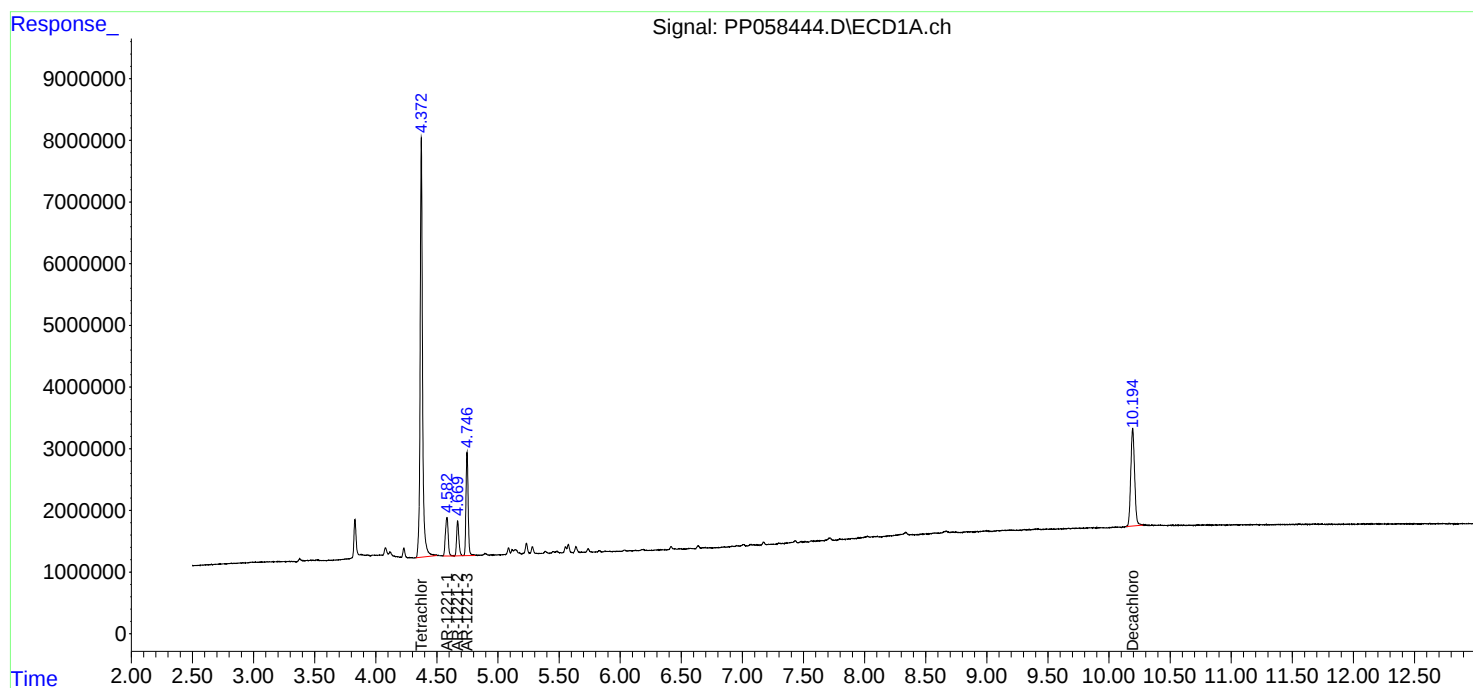


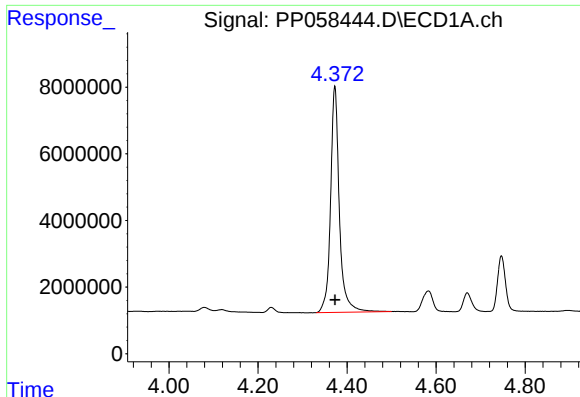

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 93194177
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

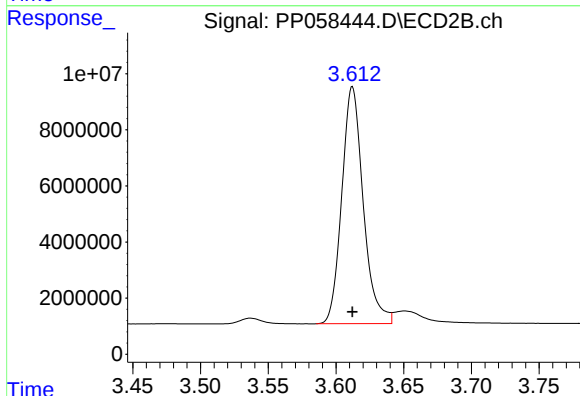


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: 0.000 min
Response: 93289438
Conc: 50.00 ng/ml

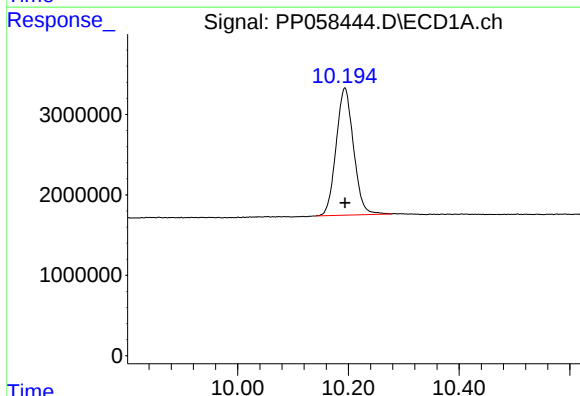


#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: 0.000 min
Response: 34559641
Conc: 50.00 ng/ml

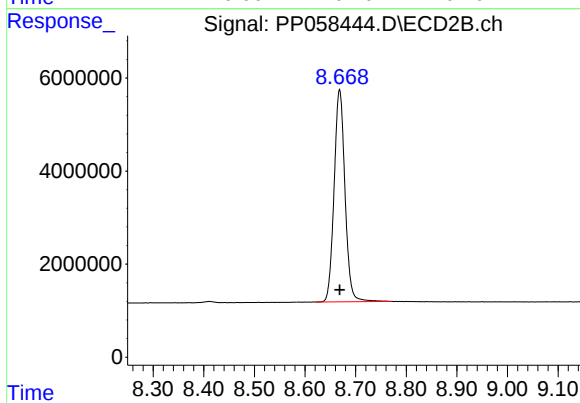

#2 Decachlorobiphenyl


R.T.: 8.668 min
Delta R.T.: 0.000 min
Response: 68004109
Conc: 50.00 ng/ml

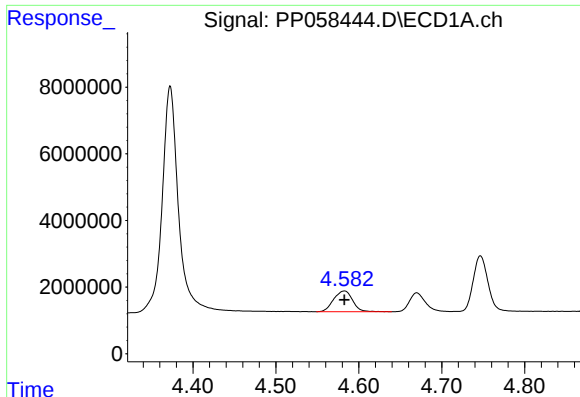

#8 AR-1221-1


R.T.: 4.583 min
Delta R.T.: 0.000 min
Response: 9895820
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

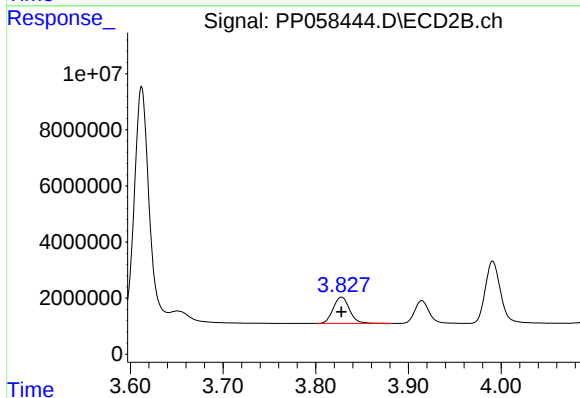


#8 AR-1221-1

R.T.: 3.828 min
Delta R.T.: 0.000 min
Response: 11594157
Conc: 500.00 ng/ml

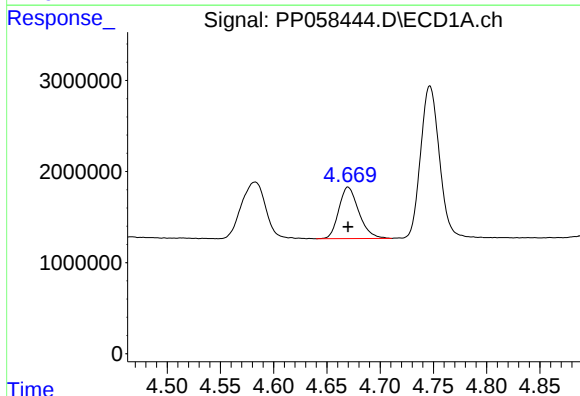


#9 AR-1221-2

R.T.: 4.670 min
Delta R.T.: 0.000 min
Response: 7405921
Conc: 500.00 ng/ml

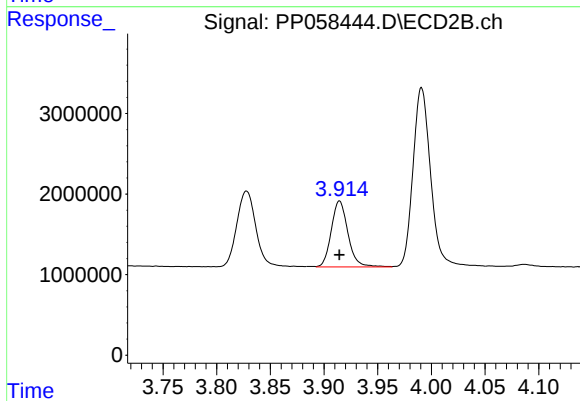

#9 AR-1221-2


R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 8847385
Conc: 500.00 ng/ml

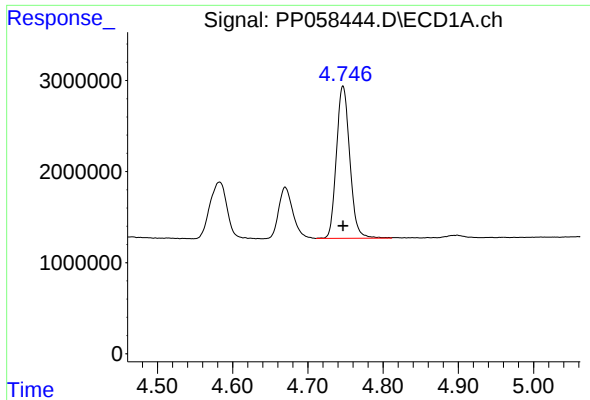

#10 AR-1221-3

R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 20658363
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

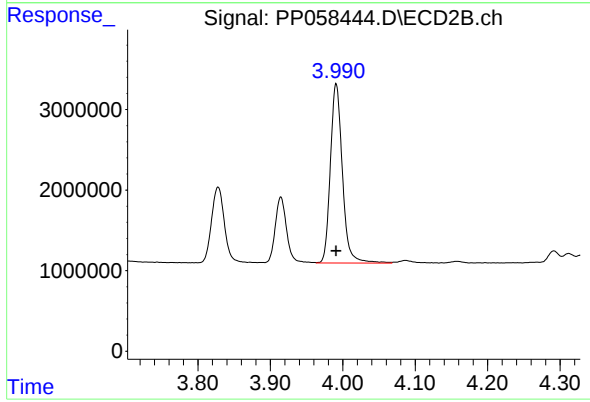

#10 AR-1221-3

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 25683468
Conc: 500.00 ng/ml