

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061323\
 Data File : PP058460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2023 17:08
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/14/2023
 Supervised By :Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 17:46:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 13 17:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.612	8446013	9518952	4.889	5.075
2) SA Decachlor...	10.191	8.668	4179915	7794873	6.079m	5.755
Target Compounds						
26) L6 AR-1254-1	6.416	5.517	2611198	5075739	54.154m	55.688
27) L6 AR-1254-2	6.637	5.666	3563939	4566689	53.852m	55.925
28) L6 AR-1254-3	7.007	6.074	3599409	6918812	58.360	54.063
29) L6 AR-1254-4	7.297	6.305	2191615	3853388	52.953	52.196
30) L6 AR-1254-5	7.719	6.726	2501381	6299475	54.249	53.648

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061323\
Data File : PP058460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2023 17:08
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 17:46:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 13 17:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

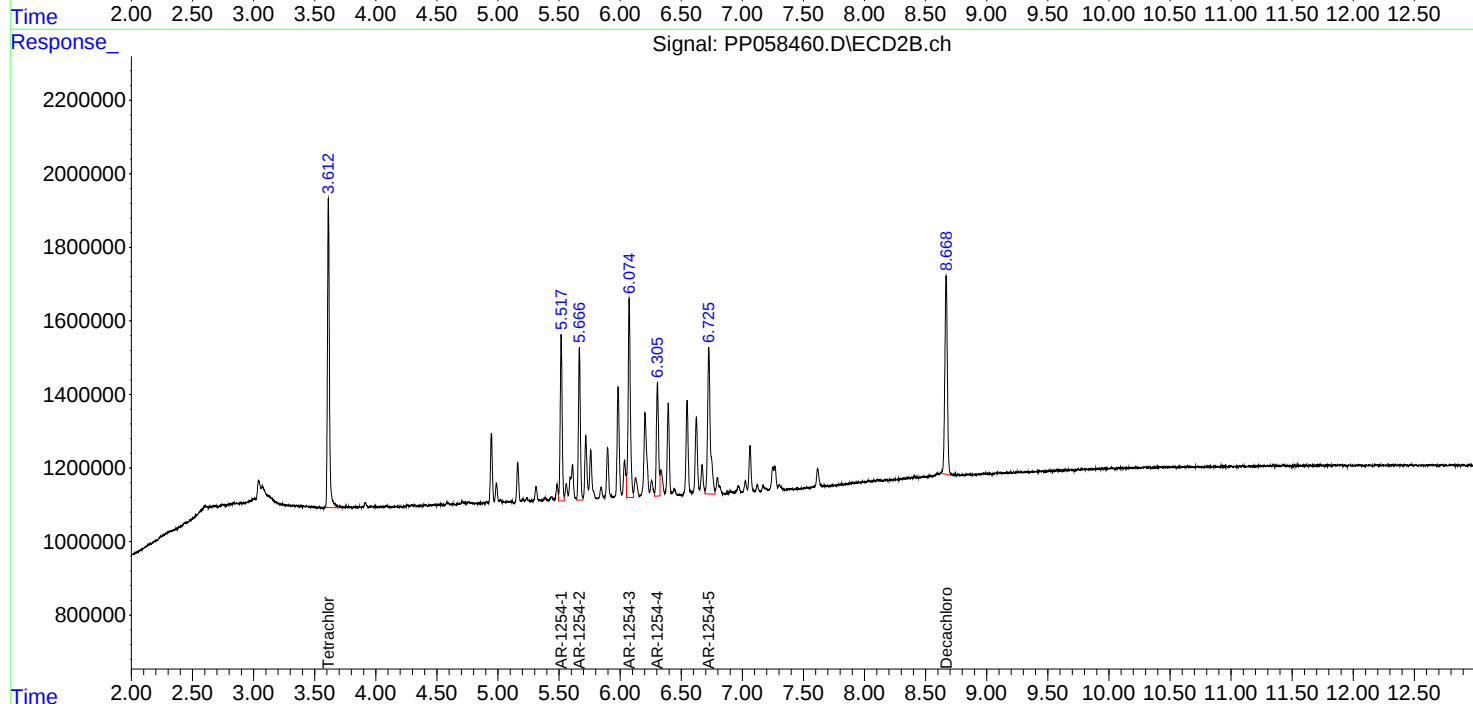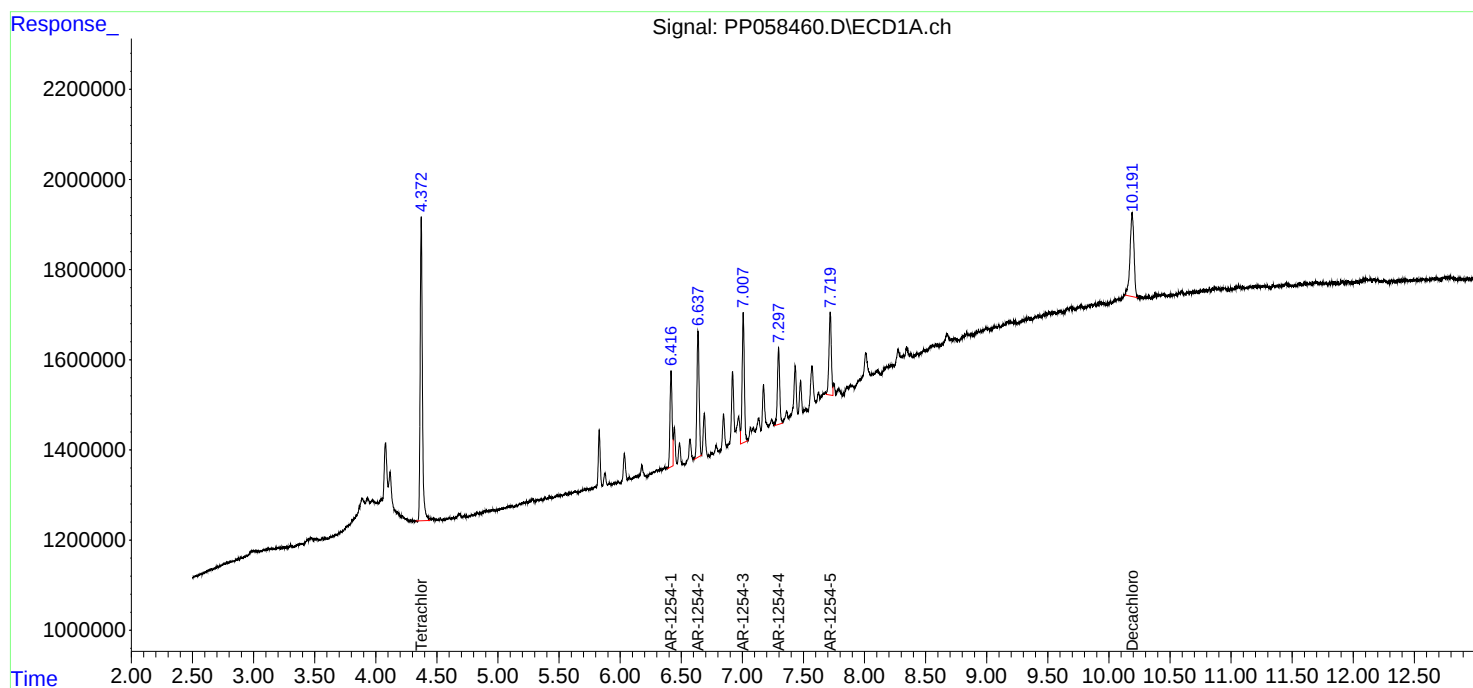

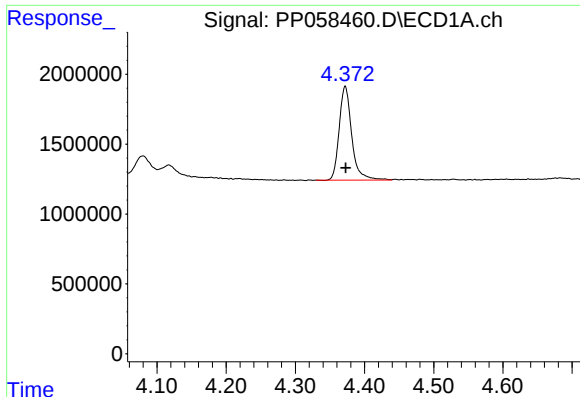


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 8446013
Conc: 4.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

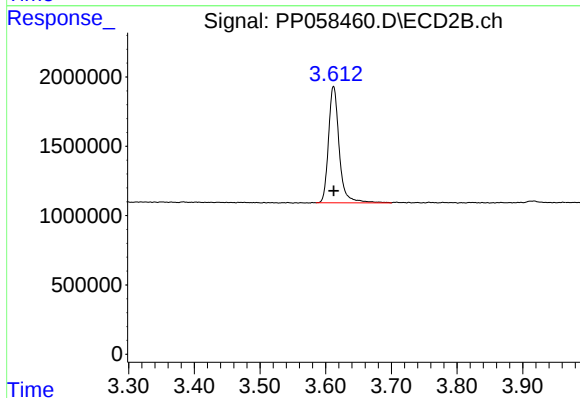


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: 0.000 min
Response: 9518952
Conc: 5.07 ng/ml

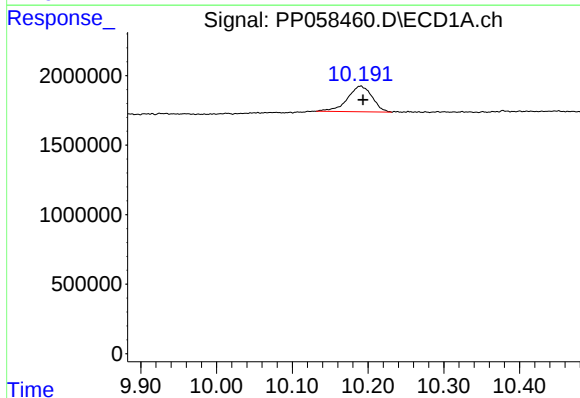


#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: -0.003 min
Response: 4179915
Conc: 6.08 ng/ml m

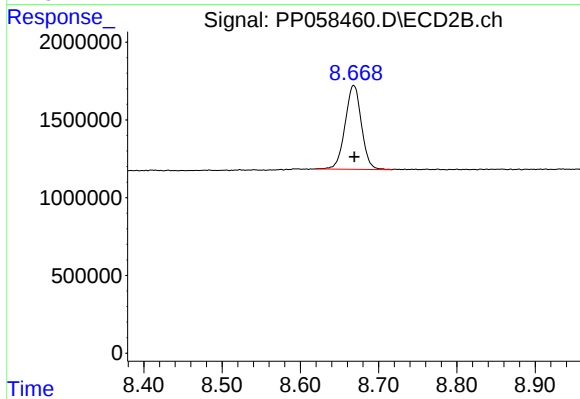

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: 0.000 min
Response: 7794873
Conc: 5.76 ng/ml

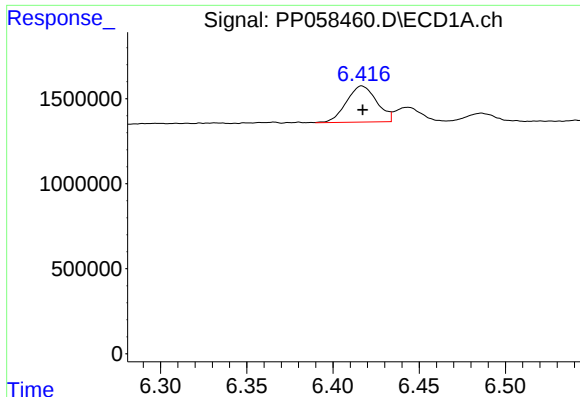


#26 AR-1254-1

R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 2611198
Conc: 54.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

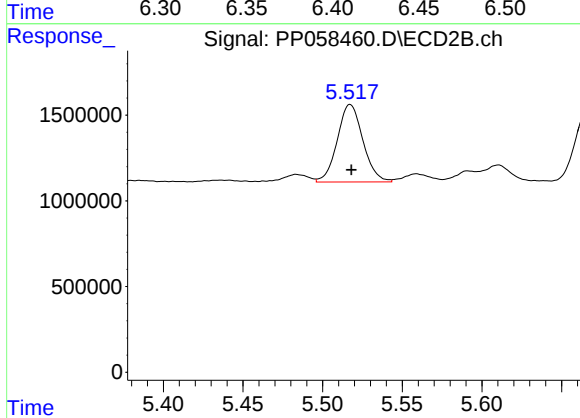


#26 AR-1254-1

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 5075739
Conc: 55.69 ng/ml

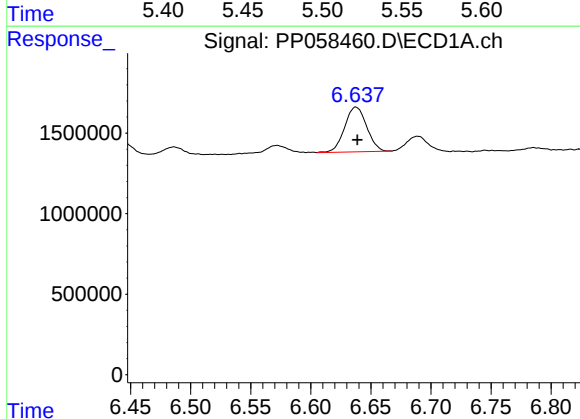


#27 AR-1254-2

R.T.: 6.637 min
Delta R.T.: -0.002 min
Response: 3563939
Conc: 53.85 ng/ml m

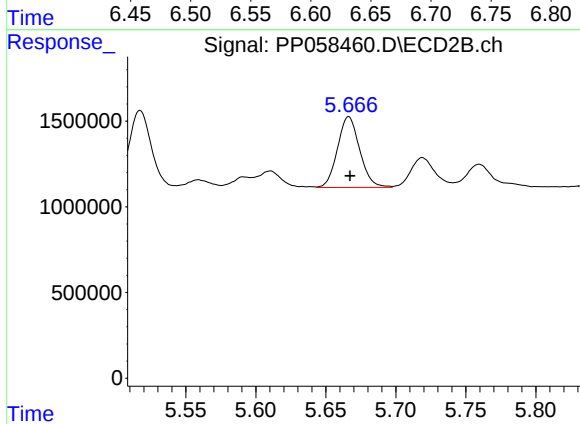

#27 AR-1254-2

R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 4566689
Conc: 55.92 ng/ml

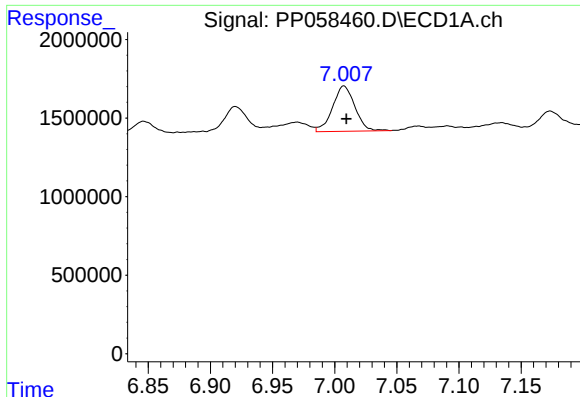


#28 AR-1254-3

R.T.: 7.007 min
Delta R.T.: -0.002 min
Response: 3599409
Conc: 58.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

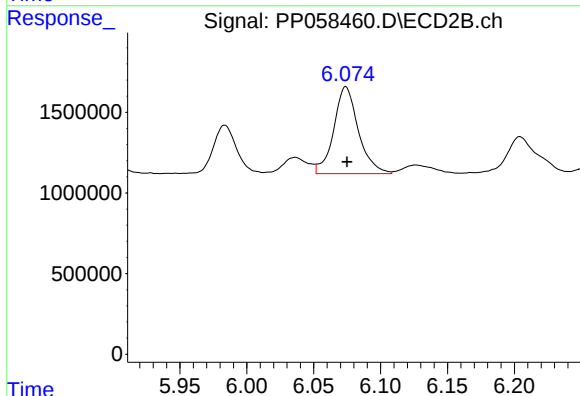


#28 AR-1254-3

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 6918812
Conc: 54.06 ng/ml

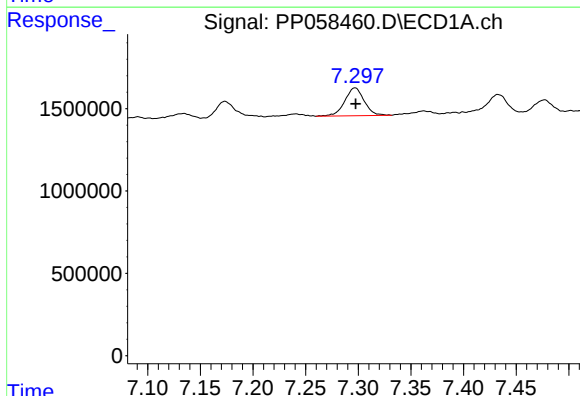


#29 AR-1254-4

R.T.: 7.297 min
Delta R.T.: 0.000 min
Response: 2191615
Conc: 52.95 ng/ml

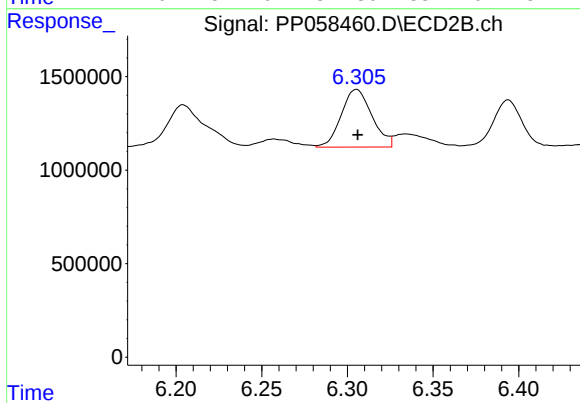

#29 AR-1254-4

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 3853388
Conc: 52.20 ng/ml

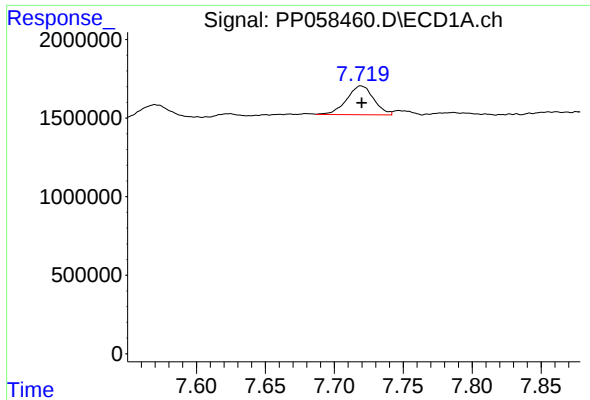


#30 AR-1254-5

R.T.: 7.719 min
Delta R.T.: 0.000 min
Response: 2501381
Conc: 54.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

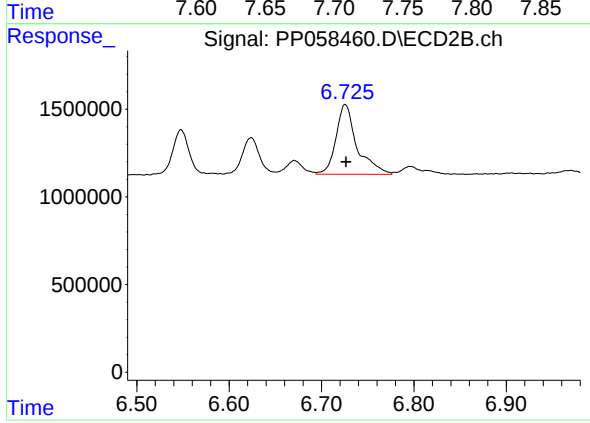

#30 AR-1254-5

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 6299475
Conc: 53.65 ng/ml